

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
 Data File : P0053708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 18:11
 Operator : SM/SJ
 Sample : K1361-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-006-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:44:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.095	3.159	39271483	4472282	20.149	18.646
2) SA Decachlor...	9.481	7.766	16039380	4246998	16.457	17.008

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020419\
Data File : PO053708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 18:11
Operator : SM/SJ
Sample : K1361-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-006-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:44:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

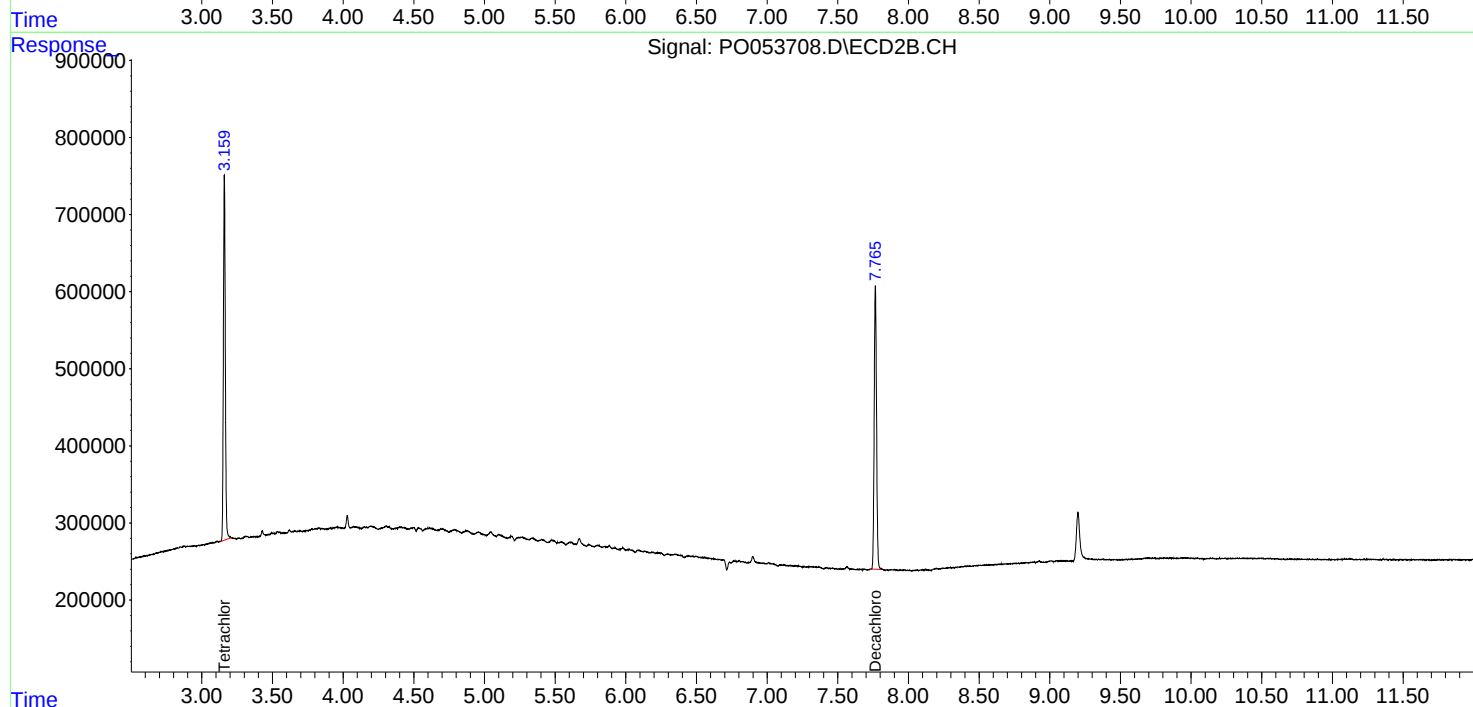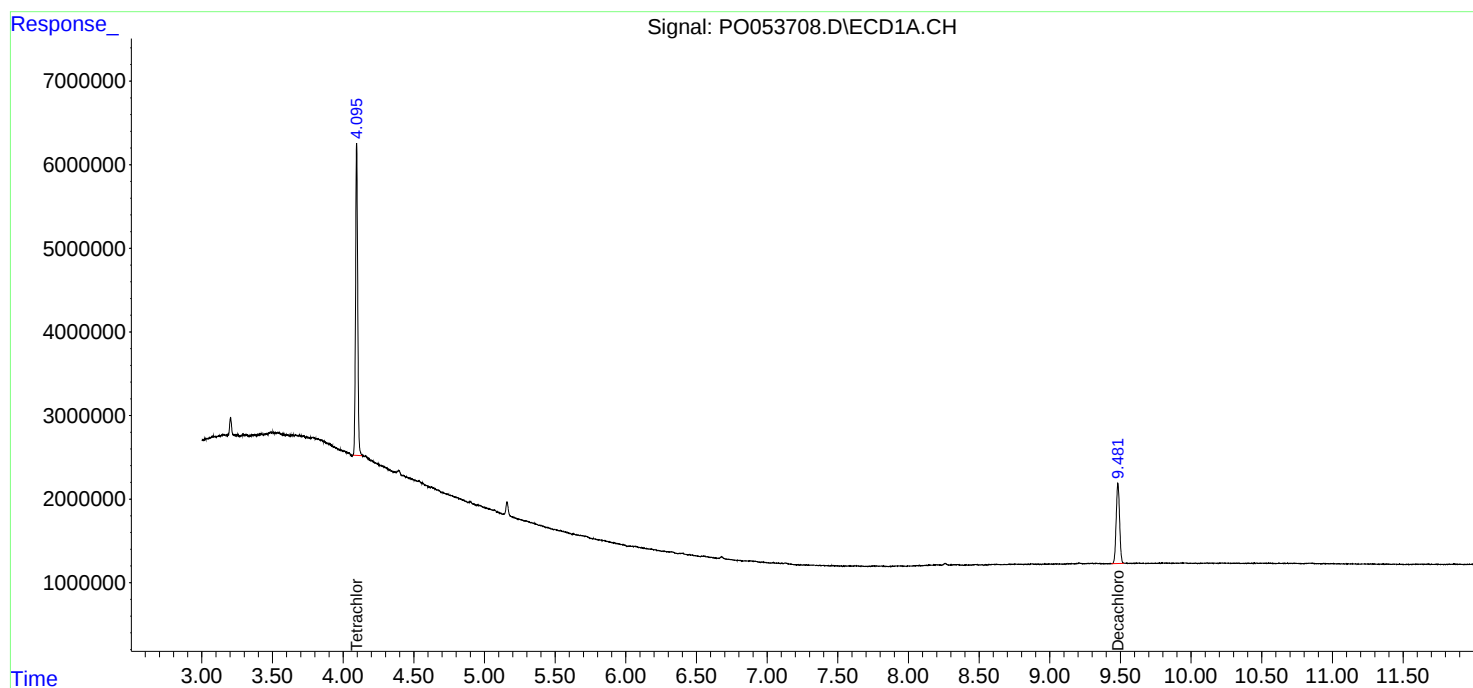


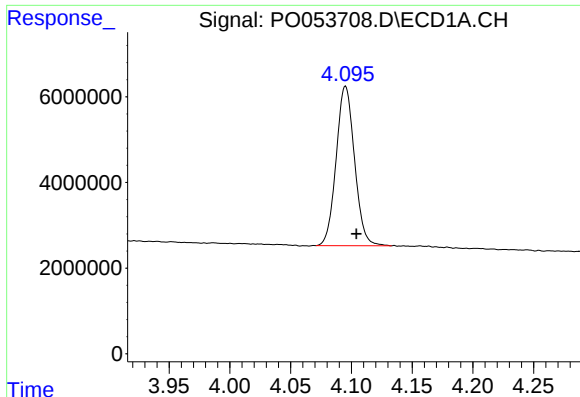

#1 Tetrachloro-m-xylene


R.T.: 4.095 min
Delta R.T.: -0.009 min
Response: 39271483
Conc: 20.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-006-ABCD

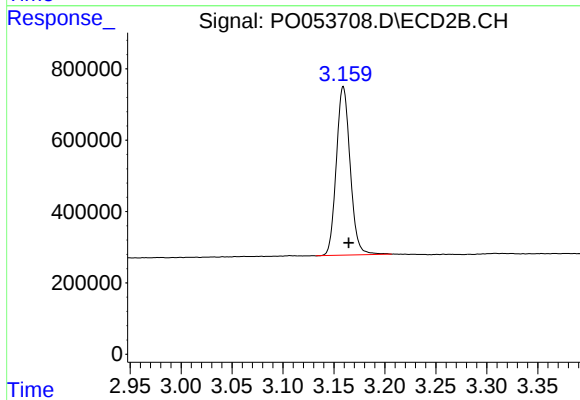


#1 Tetrachloro-m-xylene

R.T.: 3.159 min
Delta R.T.: -0.005 min
Response: 4472282
Conc: 18.65 ng/ml

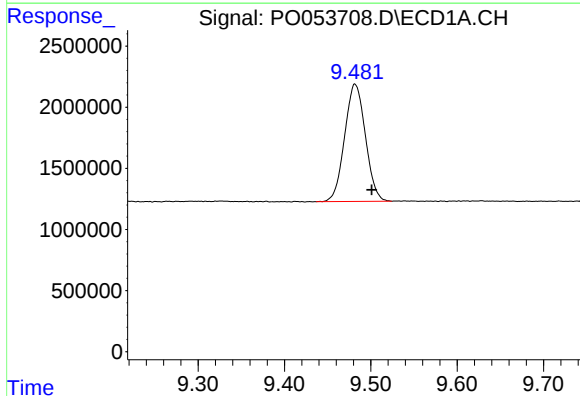

#2 Decachlorobiphenyl

R.T.: 9.481 min
Delta R.T.: -0.019 min
Response: 16039380
Conc: 16.46 ng/ml

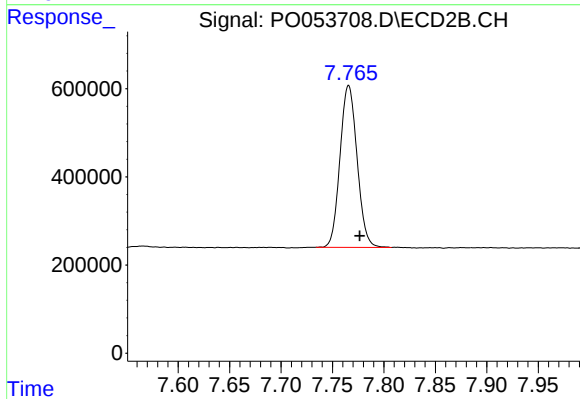

#2 Decachlorobiphenyl

R.T.: 7.766 min
Delta R.T.: -0.011 min
Response: 4246998
Conc: 17.01 ng/ml