

Data Path : P:\HPCHEM1\ECD_0\Data\P0020518\
Data File : P0042091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2018 18:43
Operator : SM/UA
Sample : J1432-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
A277000

Manual Integrations
APPROVED

ugo
2/4/2018 1:23:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 19:23:22 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.190	3.361	1535764	247713	7.957m	0.853m#
2) SA Decachlor...	9.516	8.167	427729	1466727	1.820m	4.101m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0020518\
Data File : P0042091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2018 18:43
Operator : SM/UA
Sample : J1432-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
A277000


Manual Integrations
APPROVED

ugo
2/4/2018 1:23:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 19:23:22 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

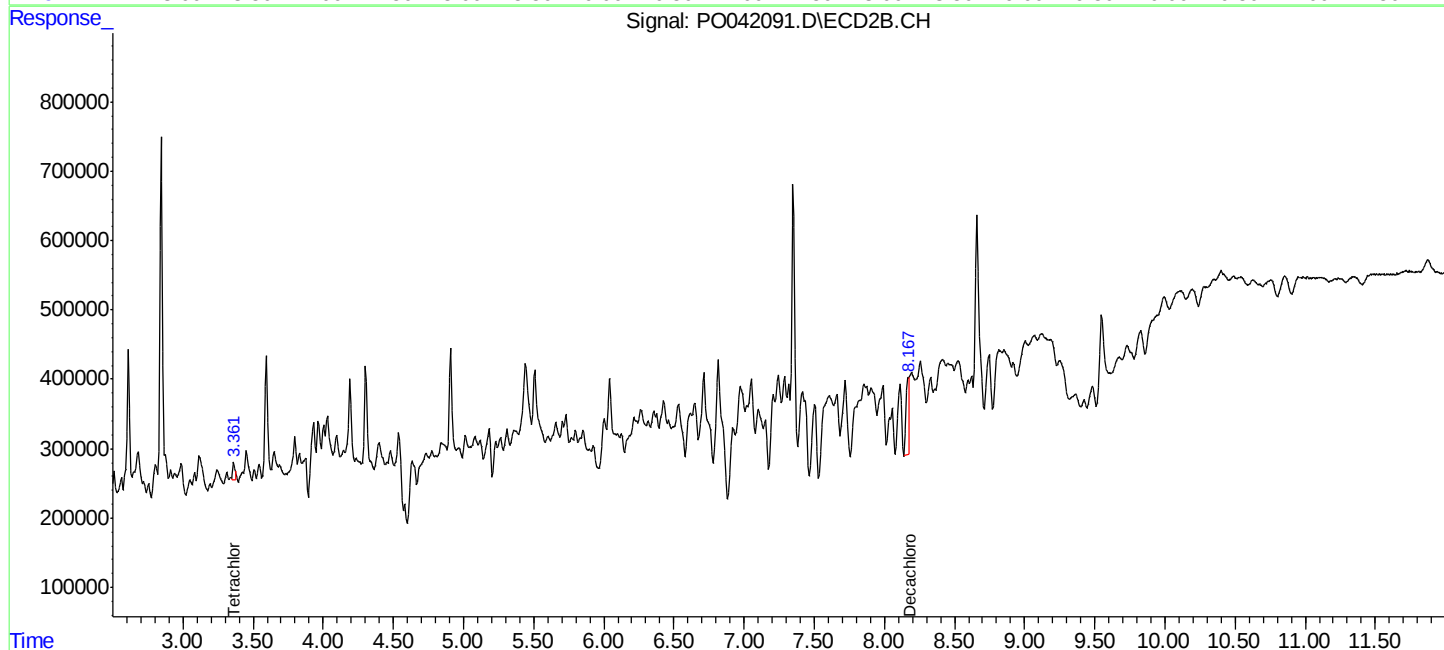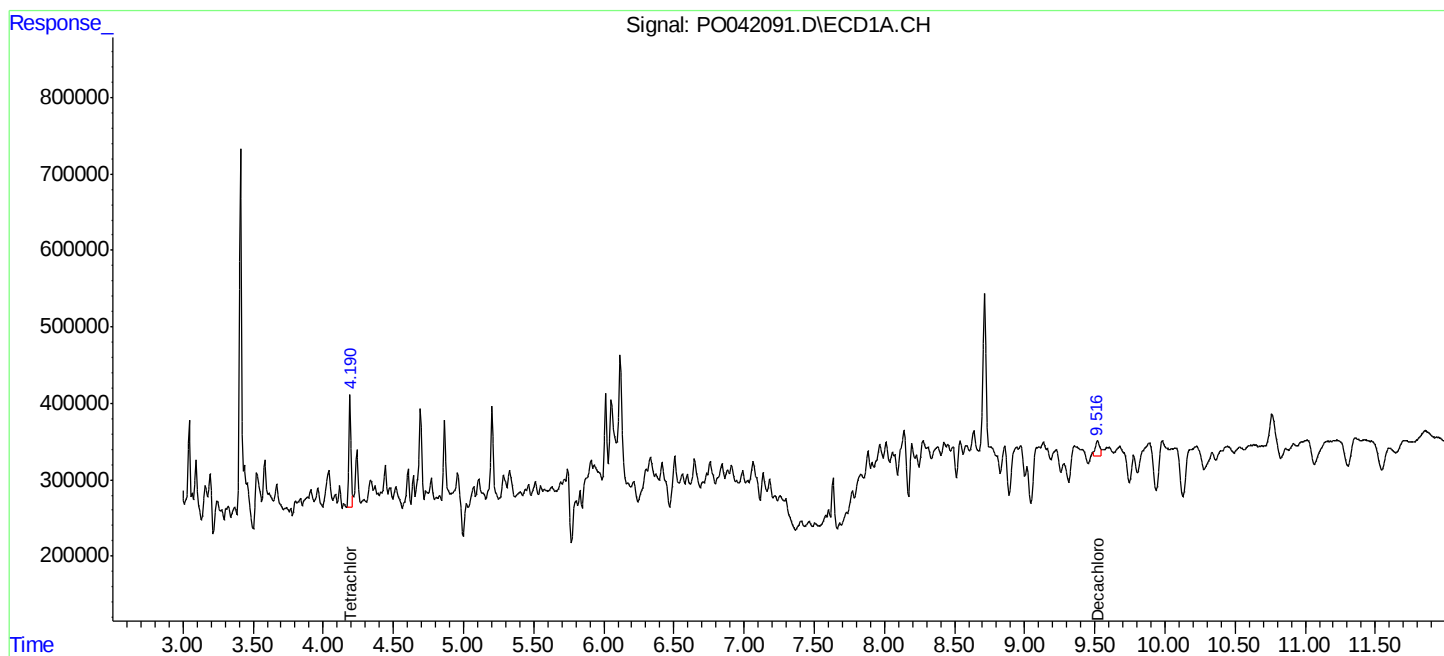

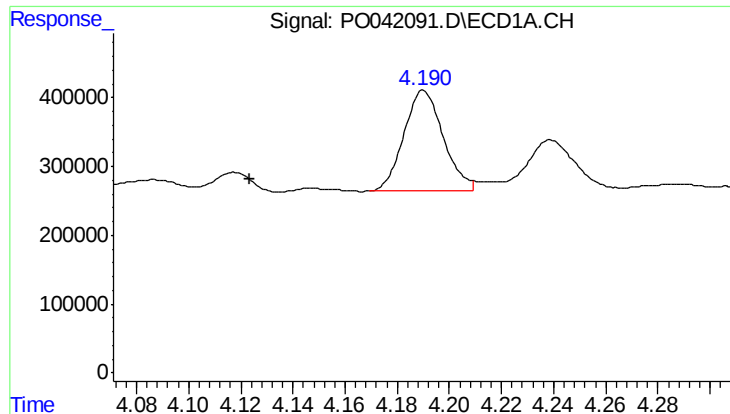


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: 0.066 min
Response: 1535764
Conc: 7.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
A277000


Manual Integrations
APPROVED

ugo
2/4/2018 1:23:05 PM

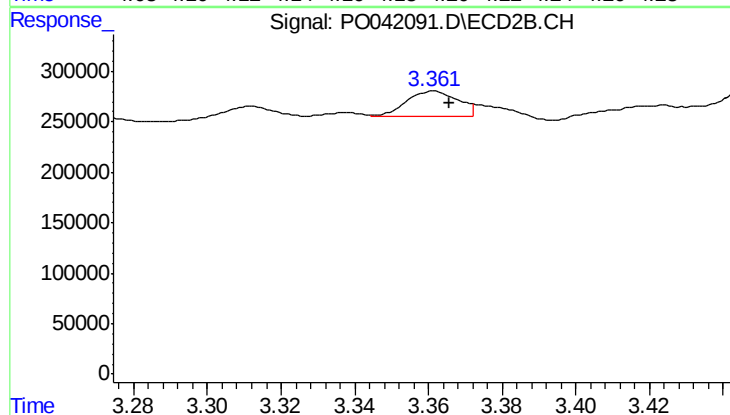


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: -0.005 min
Response: 247713
Conc: 0.85 ng/ml m

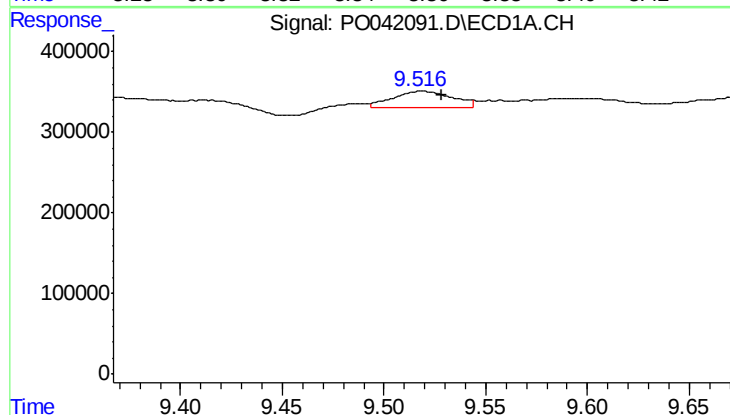

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.012 min
Response: 427729
Conc: 1.82 ng/ml m

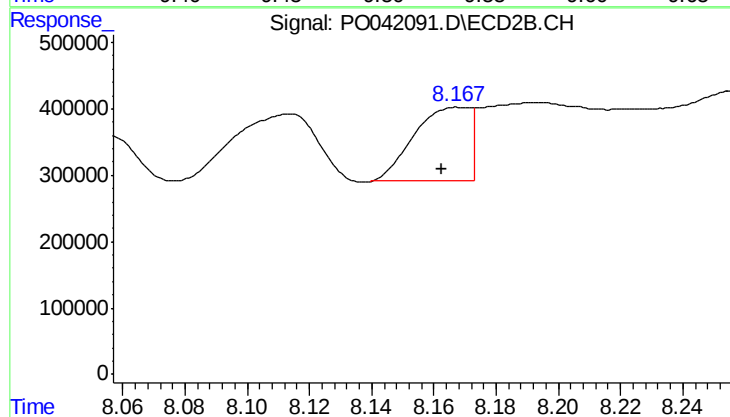

#2 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: 0.005 min
Response: 1466727
Conc: 4.10 ng/ml m