

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020619\
 Data File : P0053746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2019 13:17
 Operator : SM/SJ
 Sample : K1362-01MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:35:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.093	3.157	42571115	5386690	21.842	22.458
2)	SA Decachlor...	9.471	7.759	19064621	5002113	19.561	20.032
Target Compounds							
3)	L1 AR-1016-1	5.252	4.147	12538135	3582255	278.458	407.169 #
4)	L1 AR-1016-2	5.252	4.147	12538135	3582255	186.057	253.749 #
5)	L1 AR-1016-3	5.311	4.304	9684647	1911897	244.022	242.247
6)	L1 AR-1016-4	5.410	4.347	7926658	1424517	249.071	272.408
7)	L1 AR-1016-5	5.692	4.537	7156518	1789088	255.076	246.101
8)	L2 AR-1221-1	0.000	3.427	0	287801	N.D.	114.994 #
9)	L2 AR-1221-2	4.388	3.427	1716175	287801	143.395	161.317
10)	L2 AR-1221-3	4.462	3.493	6557754	1123057	166.496	178.343
11)	L3 AR-1232-1	4.462	3.493	6557754	1123057	204.193	209.727
12)	L3 AR-1232-2	4.971	4.147	8999469	3582255	591.533	564.066
13)	L3 AR-1232-3	5.252	4.304	12538135	1911897	427.943	541.798 #
14)	L3 AR-1232-4	5.410	4.383	7926658	1707031	559.968	667.013
15)	L3 AR-1232-5	5.493	4.537	6039642	1789088	753.747	569.020
16)	L4 AR-1242-1	5.252	4.147	12538135	3582255	346.812	482.487 #
17)	L4 AR-1242-2	5.252	4.147	12538135	3582255	237.334	312.612 #
18)	L4 AR-1242-3	5.311	4.304	9684647	1911897	303.221	310.193
19)	L4 AR-1242-4	5.410	4.383	7926658	1707031	306.434	320.243
20)	L4 AR-1242-5	0.000	4.858	0	1408528	N.D.	191.707 #
21)	L5 AR-1248-1	5.252	4.147	12538135	3582255	458.182	625.119 #
22)	L5 AR-1248-2	5.493	4.347	6039642	1424517	183.316	187.789
23)	L5 AR-1248-3	5.692	4.383	7156518	1707031	186.927	217.872
24)	L5 AR-1248-4	6.058	4.537	4080118	1789088	97.214	180.195 #
25)	L5 AR-1248-5	0.000	4.858	0	1408528	N.D.	136.030 #
26)	L6 AR-1254-1	6.058	4.858	4080118	1408528	97.041	86.485
27)	L6 AR-1254-2	6.270	4.998	4961305	1335105	76.011	96.800 #
28)	L6 AR-1254-3	6.634	5.381	2464081	2591982	35.991	118.580 #
29)	L6 AR-1254-4	6.912	5.589	1585224	255250	31.103	17.983 #
30)	L6 AR-1254-5	7.355	5.976	1910553	4346945	39.915	232.711 #
31)	L7 AR-1260-1	6.788	5.489	10275532	3583824	210.807	235.361
32)	L7 AR-1260-2	7.041	5.672	12589289	3963762	202.580	213.776
33)	L7 AR-1260-3	7.392	5.808	8351873	3582780	213.510	209.584
34)	L7 AR-1260-4	7.616	6.253	8755922	2449455	202.629	222.428
35)	L7 AR-1260-5	7.921	6.494	18392649	5709294	202.051	209.661
36)	L8 AR-1262-1	7.392	6.011	8351873	2861207	121.725	144.472
37)	L8 AR-1262-2	7.921	6.494	18392649	5709294	152.653	168.112
38)	L8 AR-1262-3	8.216	6.757	7356984	1512620	298.326	116.353 #
39)	L8 AR-1262-4	8.260	6.820	6995909	4349322	112.859	177.696 #
40)	L8 AR-1262-5	8.852	7.304	4775754	1321951	113.073	118.258
41)	L9 AR-1268-1	8.216	6.757	7356984	1512620	49.653	39.174

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020619\
 Data File : P0053746.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2019 13:17
 Operator : SM/SJ
 Sample : K1362-01MS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:35:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.260	6.820	6995909	4349322	49.847	118.938 #
44) L9	AR-1268-4	8.852	7.304	4775754	1321951	100.458	106.148
45) L9	AR-1268-5	9.199	7.559	1587445	482906	4.234	5.148



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020619\
Data File : P0053746.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2019 13:17
Operator : SM/SJ
Sample : K1362-01MS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:35:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

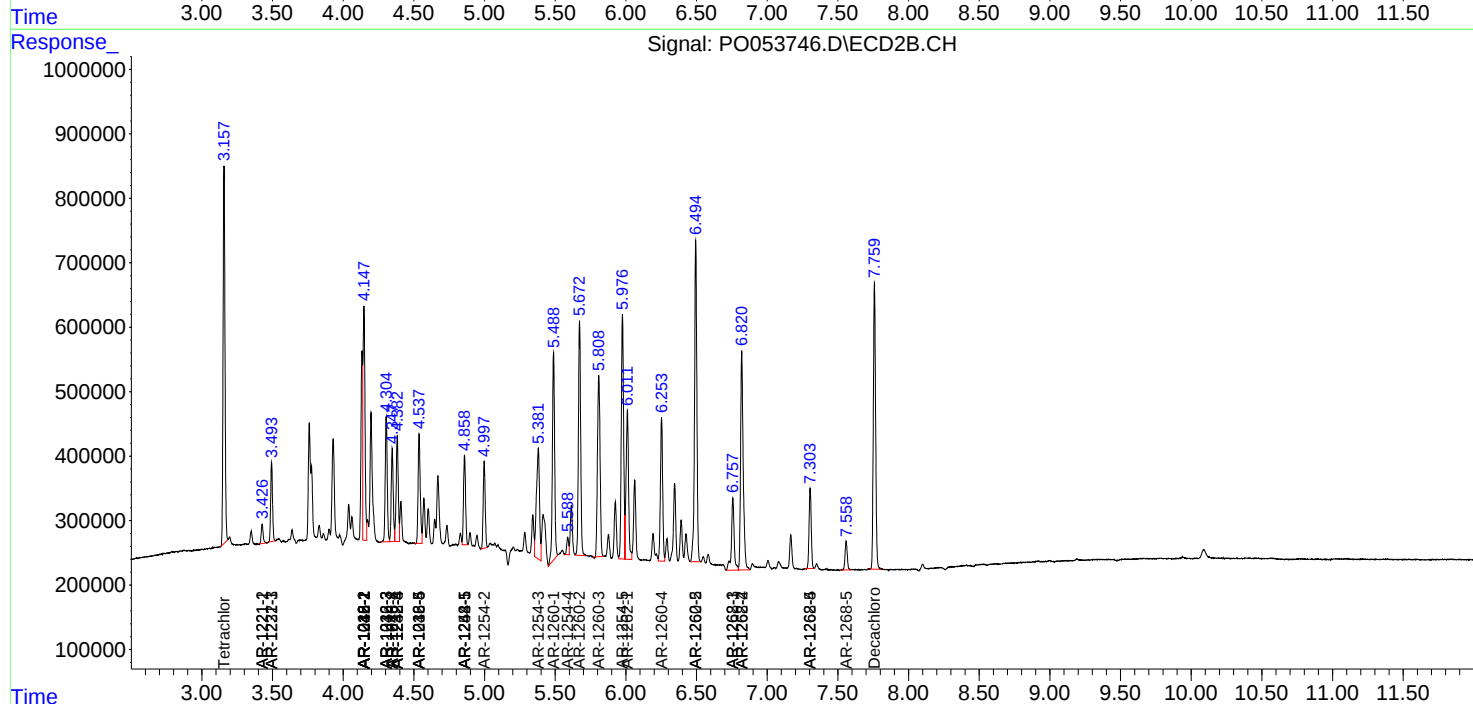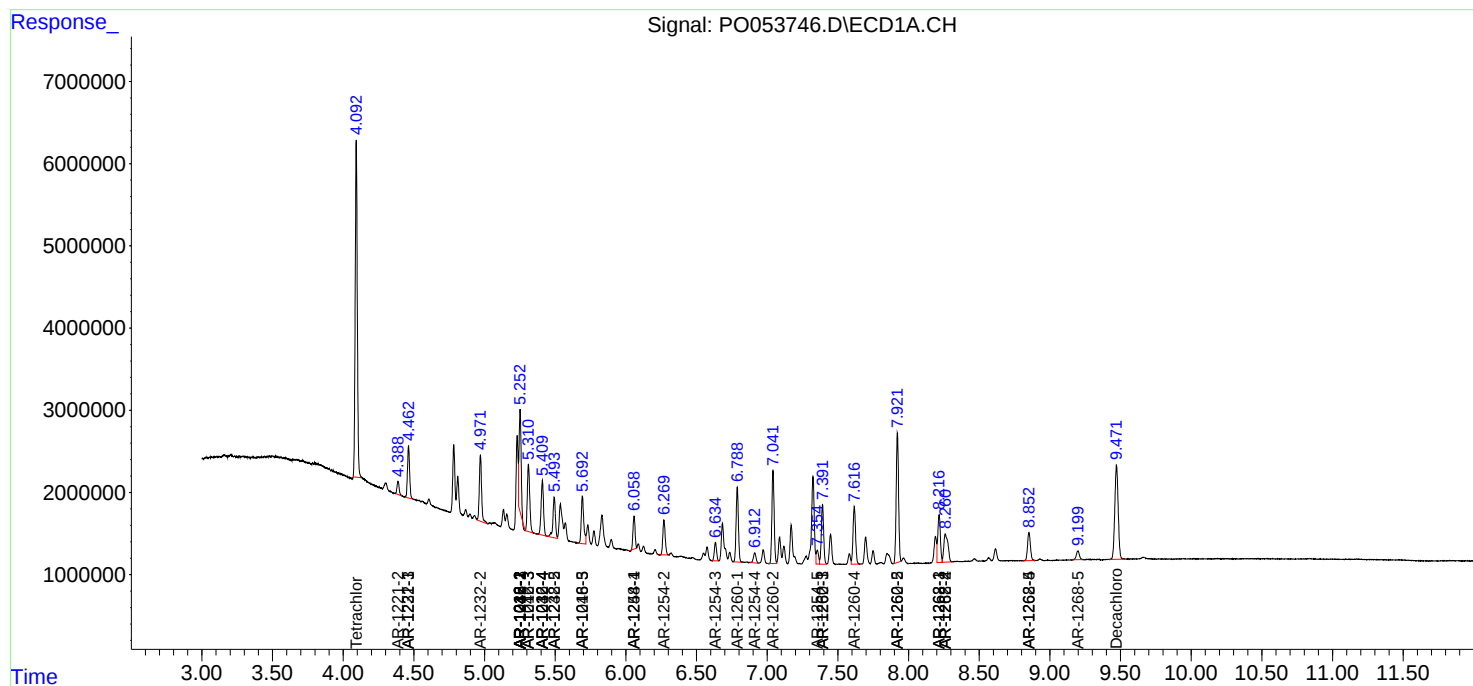


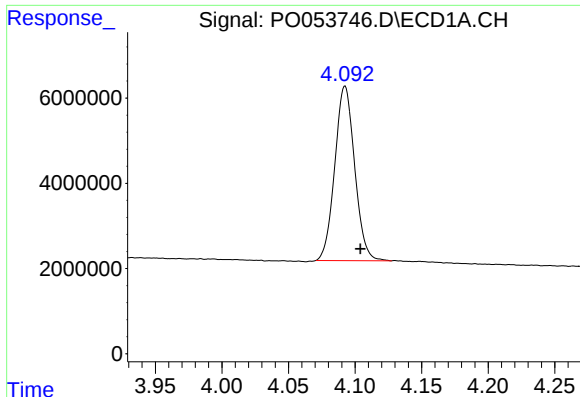

#1 Tetrachloro-m-xylene


R.T.: 4.093 min
Delta R.T.: -0.011 min
Response: 42571115
Conc: 21.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

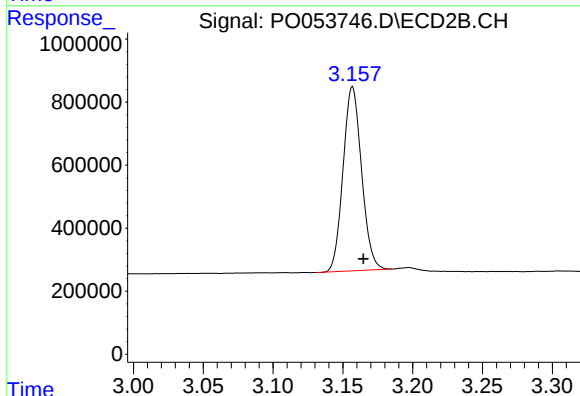


#1 Tetrachloro-m-xylene

R.T.: 3.157 min
Delta R.T.: -0.008 min
Response: 5386690
Conc: 22.46 ng/ml

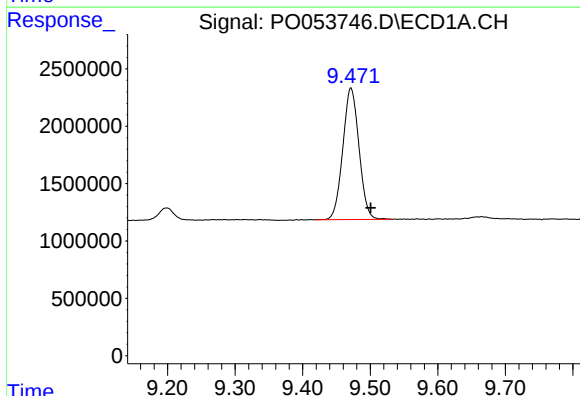


#2 Decachlorobiphenyl

R.T.: 9.471 min
Delta R.T.: -0.029 min
Response: 19064621
Conc: 19.56 ng/ml

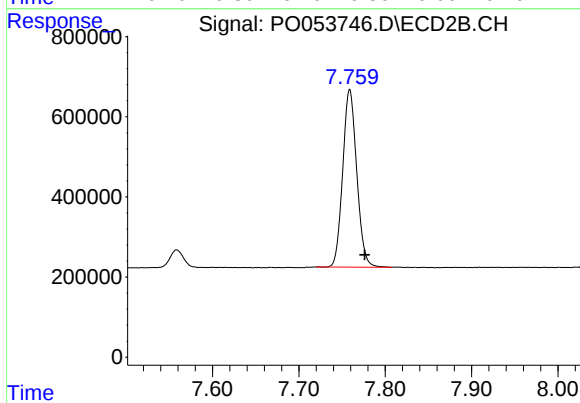

#2 Decachlorobiphenyl


R.T.: 7.759 min
Delta R.T.: -0.017 min
Response: 5002113
Conc: 20.03 ng/ml

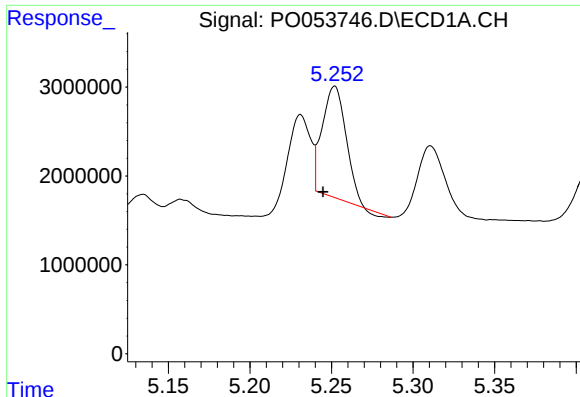

#3 AR-1016-1


R.T.: 5.252 min
Delta R.T.: 0.007 min
Response: 12538135
Conc: 278.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

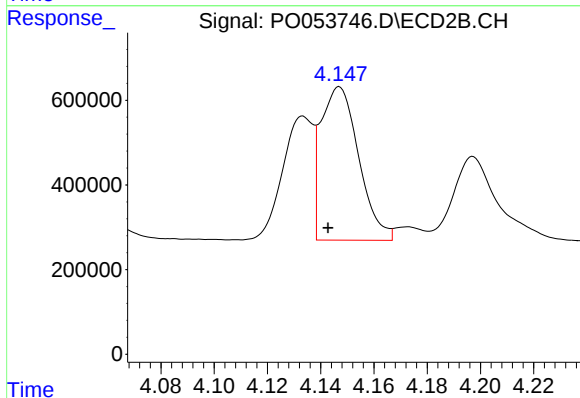


#3 AR-1016-1

R.T.: 4.147 min
Delta R.T.: 0.004 min
Response: 3582255
Conc: 407.17 ng/ml

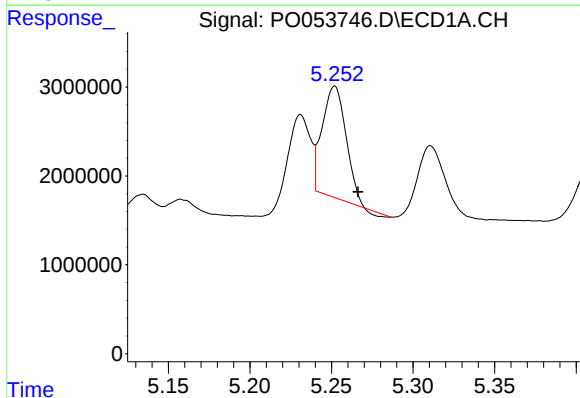


#4 AR-1016-2

R.T.: 5.252 min
Delta R.T.: -0.014 min
Response: 12538135
Conc: 186.06 ng/ml

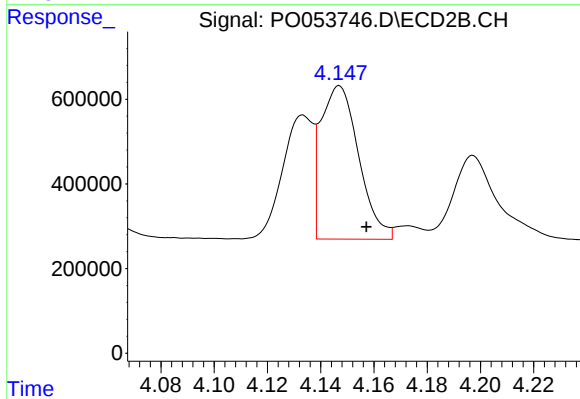

#4 AR-1016-2


R.T.: 4.147 min
Delta R.T.: -0.010 min
Response: 3582255
Conc: 253.75 ng/ml

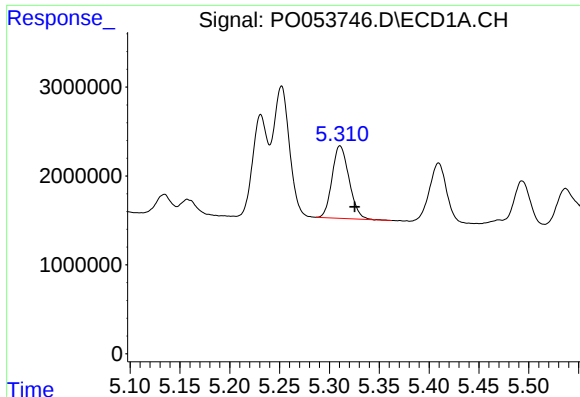

#5 AR-1016-3


R.T.: 5.311 min
Delta R.T.: -0.015 min
Response: 9684647
Conc: 244.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

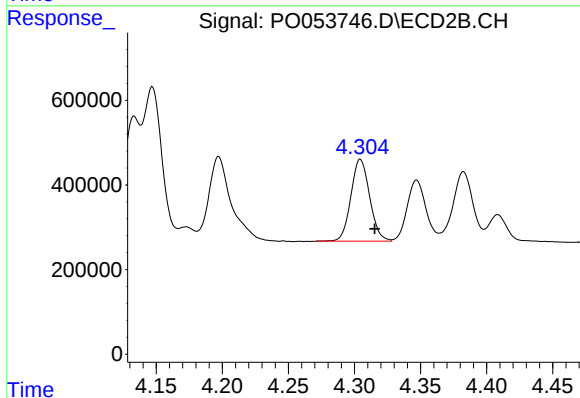


#5 AR-1016-3

R.T.: 4.304 min
Delta R.T.: -0.011 min
Response: 1911897
Conc: 242.25 ng/ml

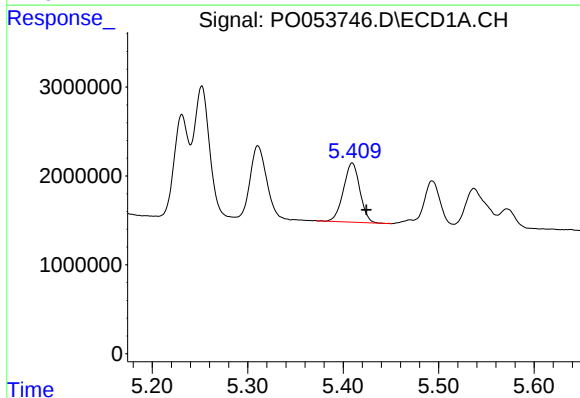


#6 AR-1016-4

R.T.: 5.410 min
Delta R.T.: -0.015 min
Response: 7926658
Conc: 249.07 ng/ml

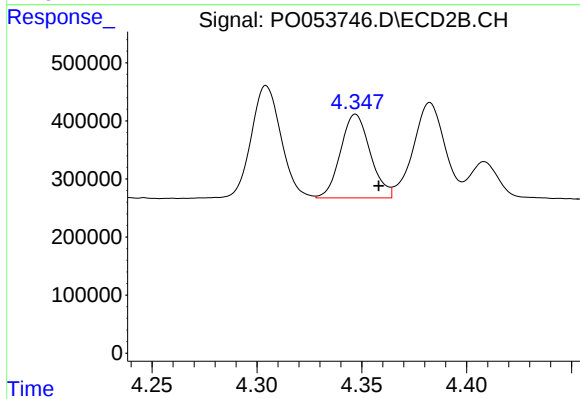

#6 AR-1016-4


R.T.: 4.347 min
Delta R.T.: -0.011 min
Response: 1424517
Conc: 272.41 ng/ml

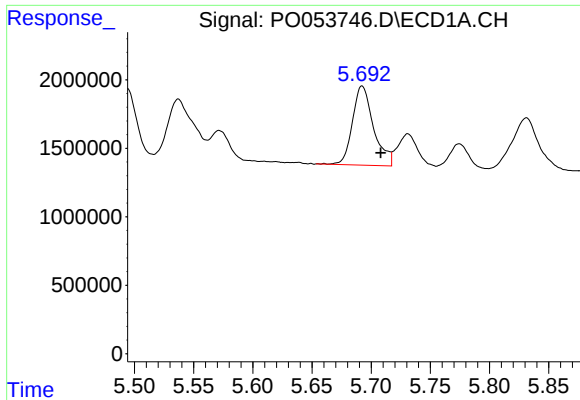

#7 AR-1016-5


R.T.: 5.692 min
Delta R.T.: -0.016 min
Response: 7156518
Conc: 255.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

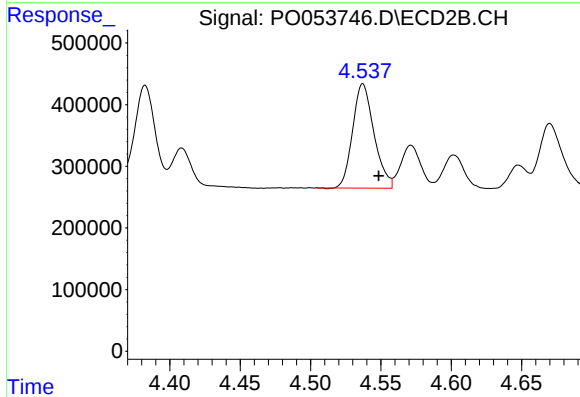


#7 AR-1016-5

R.T.: 4.537 min
Delta R.T.: -0.011 min
Response: 1789088
Conc: 246.10 ng/ml

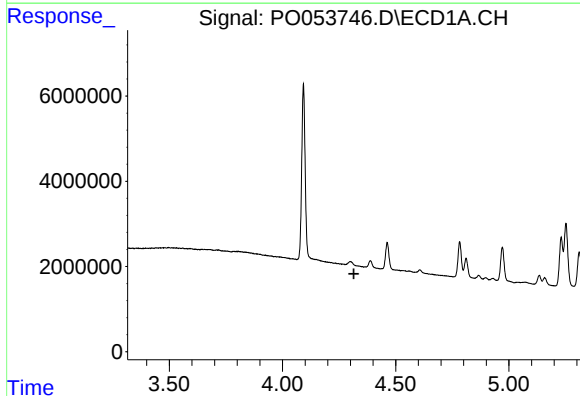


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.315 min
Response: 0
Conc: N.D.

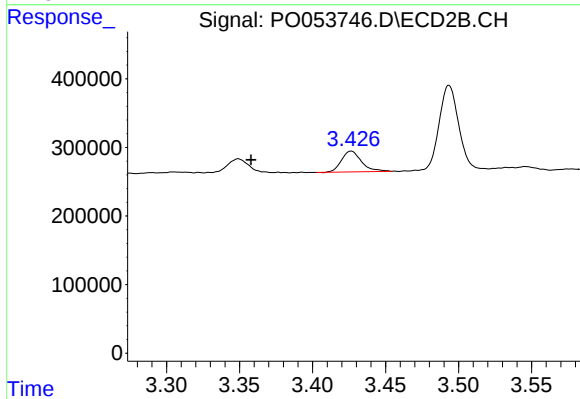

#8 AR-1221-1


R.T.: 3.427 min
Delta R.T.: 0.069 min
Response: 287801
Conc: 114.99 ng/ml

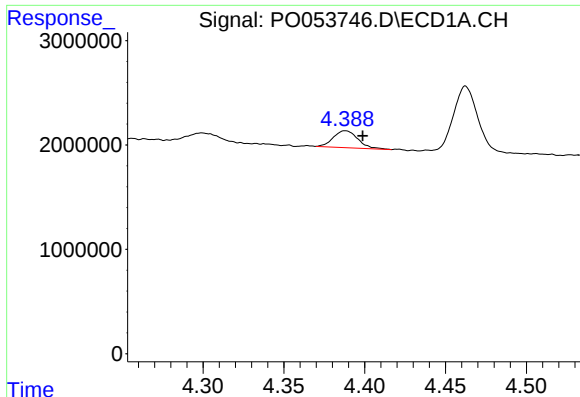

#9 AR-1221-2


R.T.: 4.388 min
Delta R.T.: -0.011 min
Response: 1716175
Conc: 143.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

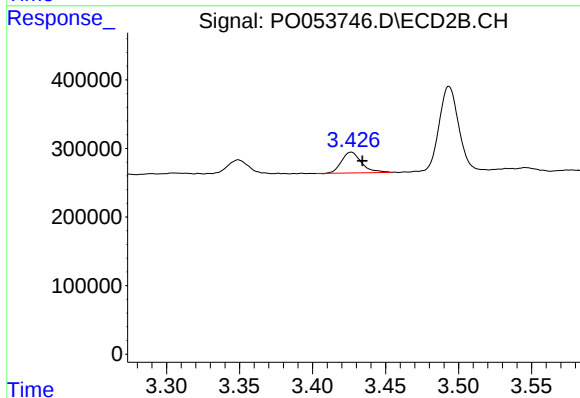


#9 AR-1221-2

R.T.: 3.427 min
Delta R.T.: -0.008 min
Response: 287801
Conc: 161.32 ng/ml

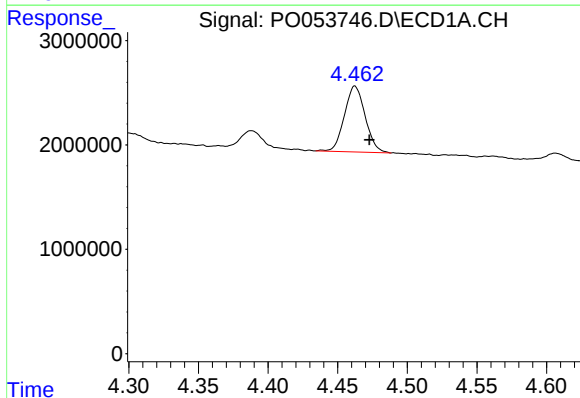


#10 AR-1221-3

R.T.: 4.462 min
Delta R.T.: -0.011 min
Response: 6557754
Conc: 166.50 ng/ml

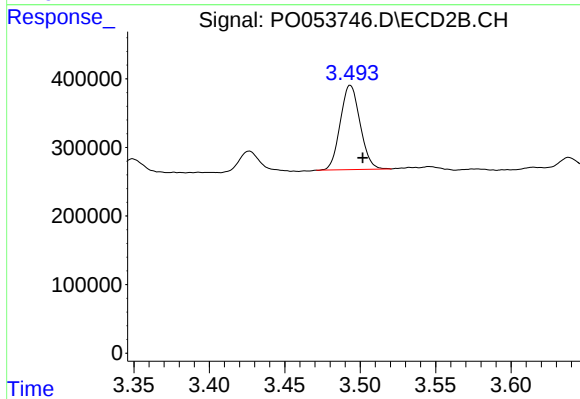

#10 AR-1221-3


R.T.: 3.493 min
Delta R.T.: -0.008 min
Response: 1123057
Conc: 178.34 ng/ml

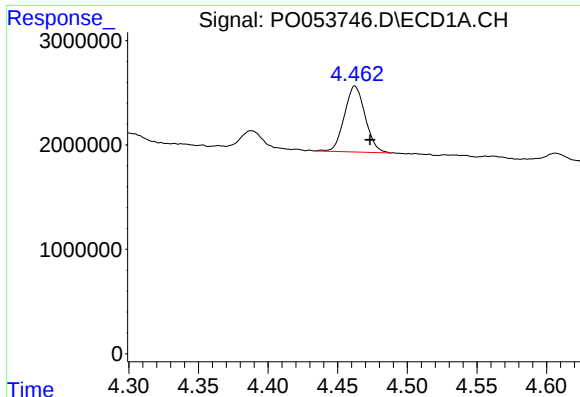

#11 AR-1232-1


R.T.: 4.462 min
Delta R.T.: -0.011 min
Response: 6557754
Conc: 204.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

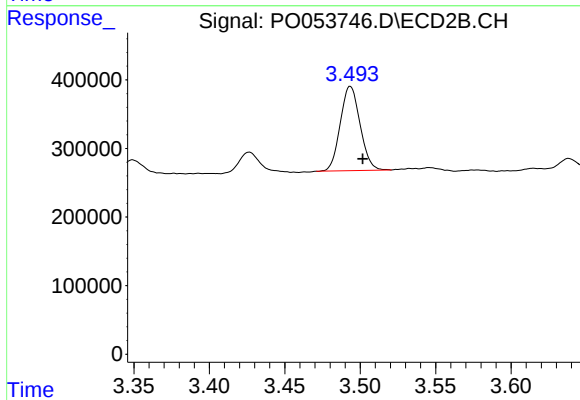


#11 AR-1232-1

R.T.: 3.493 min
Delta R.T.: -0.008 min
Response: 1123057
Conc: 209.73 ng/ml

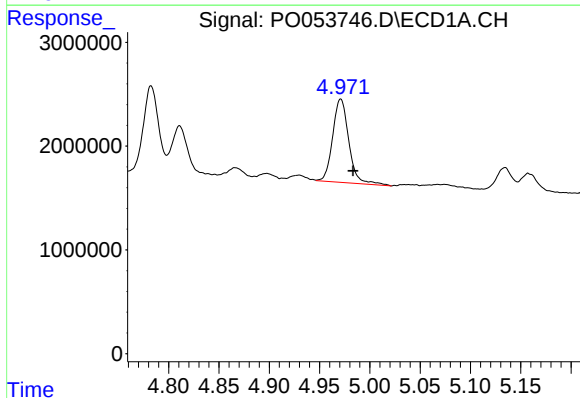


#12 AR-1232-2

R.T.: 4.971 min
Delta R.T.: -0.012 min
Response: 8999469
Conc: 591.53 ng/ml

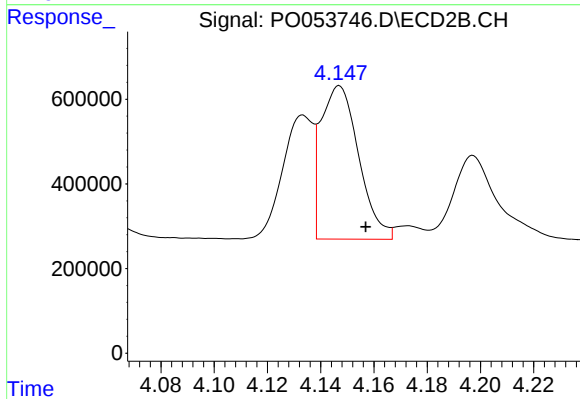

#12 AR-1232-2


R.T.: 4.147 min
Delta R.T.: -0.010 min
Response: 3582255
Conc: 564.07 ng/ml

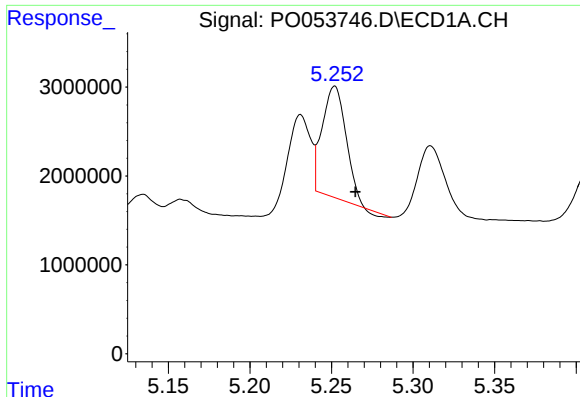

#13 AR-1232-3


R.T.: 5.252 min
Delta R.T.: -0.013 min
Response: 12538135
Conc: 427.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

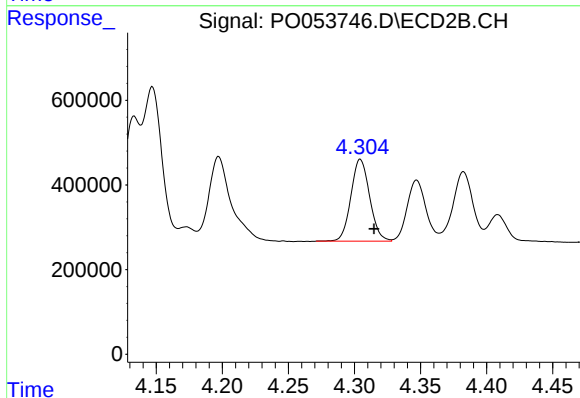


#13 AR-1232-3

R.T.: 4.304 min
Delta R.T.: -0.010 min
Response: 1911897
Conc: 541.80 ng/ml

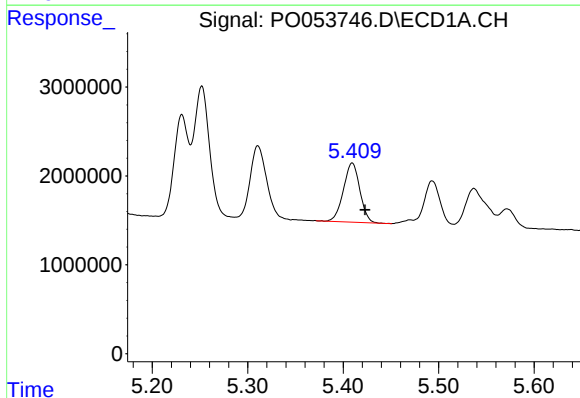


#14 AR-1232-4

R.T.: 5.410 min
Delta R.T.: -0.013 min
Response: 7926658
Conc: 559.97 ng/ml

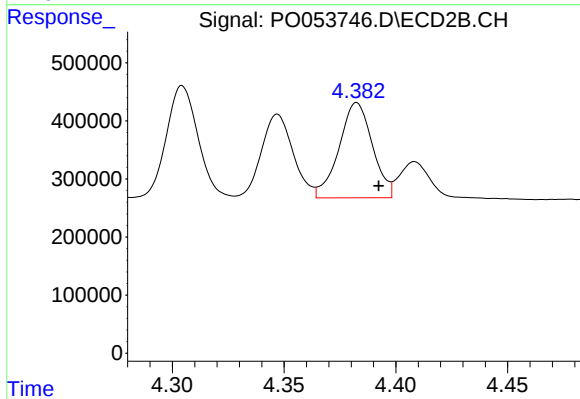

#14 AR-1232-4


R.T.: 4.383 min
Delta R.T.: -0.010 min
Response: 1707031
Conc: 667.01 ng/ml

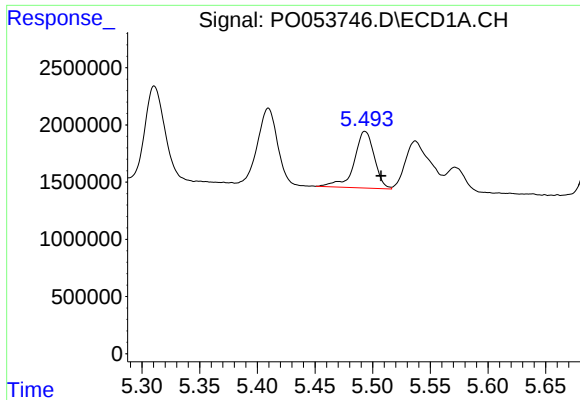

#15 AR-1232-5


R.T.: 5.493 min
Delta R.T.: -0.014 min
Response: 6039642
Conc: 753.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

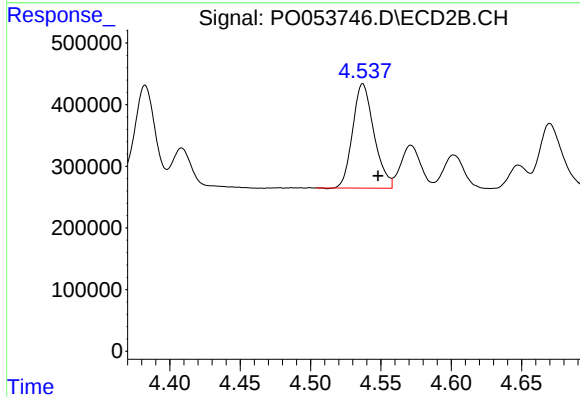


#15 AR-1232-5

R.T.: 4.537 min
Delta R.T.: -0.011 min
Response: 1789088
Conc: 569.02 ng/ml

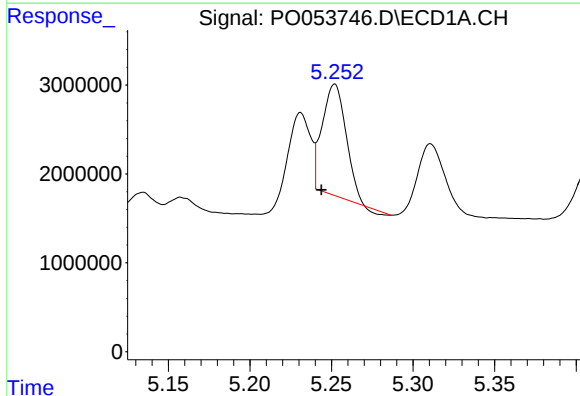


#16 AR-1242-1

R.T.: 5.252 min
Delta R.T.: 0.008 min
Response: 12538135
Conc: 346.81 ng/ml

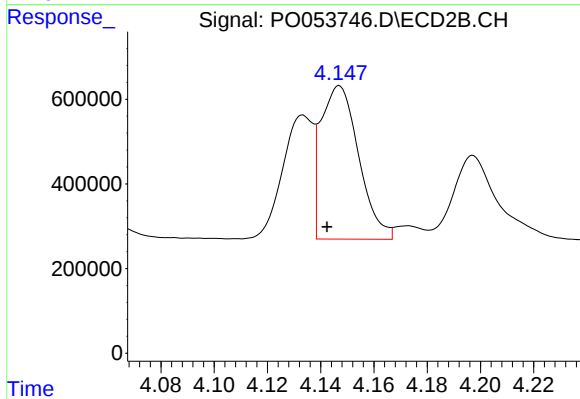

#16 AR-1242-1


R.T.: 4.147 min
Delta R.T.: 0.005 min
Response: 3582255
Conc: 482.49 ng/ml

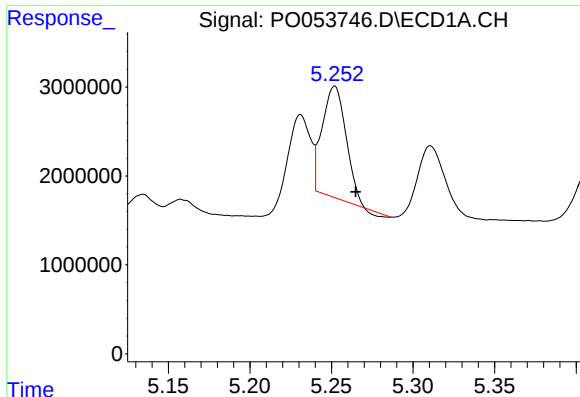

#17 AR-1242-2


R.T.: 5.252 min
Delta R.T.: -0.013 min
Response: 12538135
Conc: 237.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

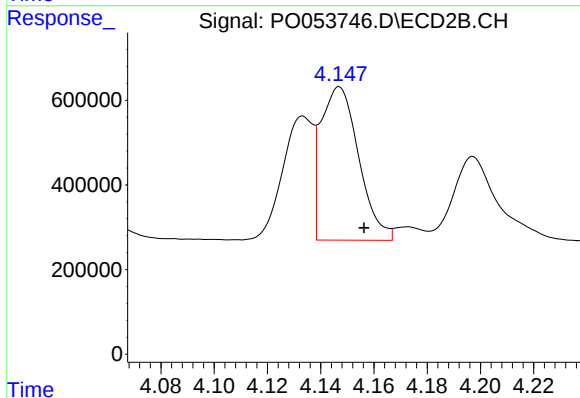


#17 AR-1242-2

R.T.: 4.147 min
Delta R.T.: -0.009 min
Response: 3582255
Conc: 312.61 ng/ml

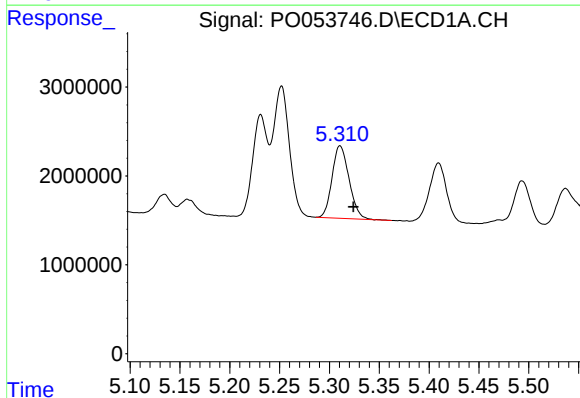


#18 AR-1242-3

R.T.: 5.311 min
Delta R.T.: -0.014 min
Response: 9684647
Conc: 303.22 ng/ml

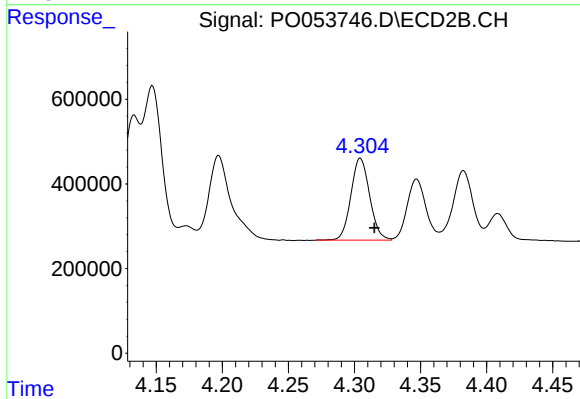

#18 AR-1242-3


R.T.: 4.304 min
Delta R.T.: -0.011 min
Response: 1911897
Conc: 310.19 ng/ml

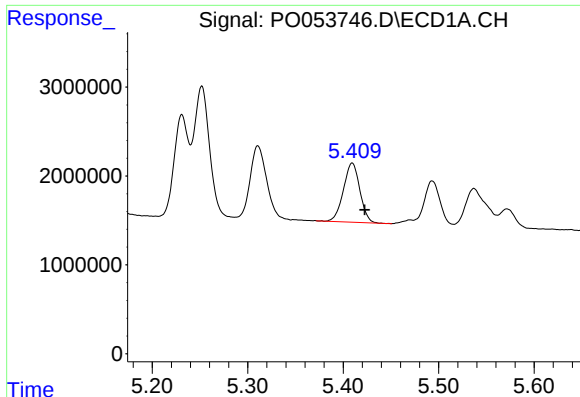

#19 AR-1242-4


R.T.: 5.410 min
Delta R.T.: -0.013 min
Response: 7926658
Conc: 306.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

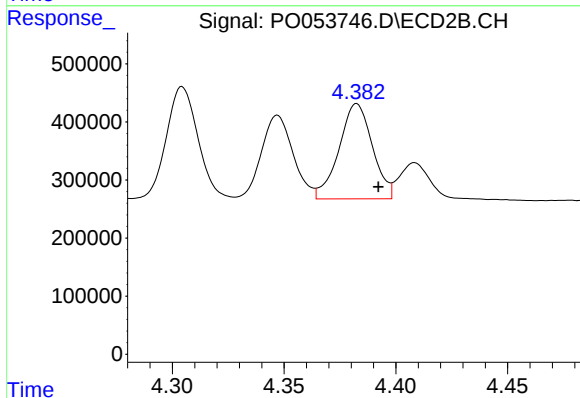


#19 AR-1242-4

R.T.: 4.383 min
Delta R.T.: -0.010 min
Response: 1707031
Conc: 320.24 ng/ml

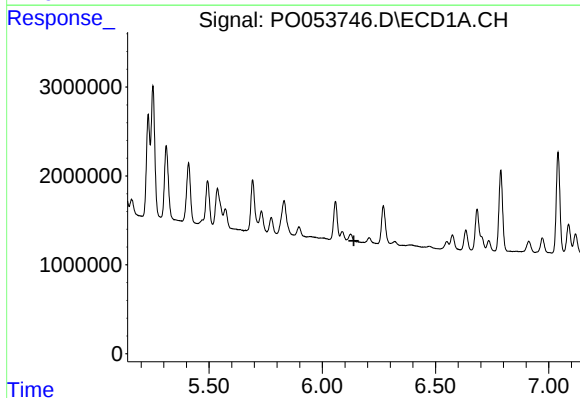


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

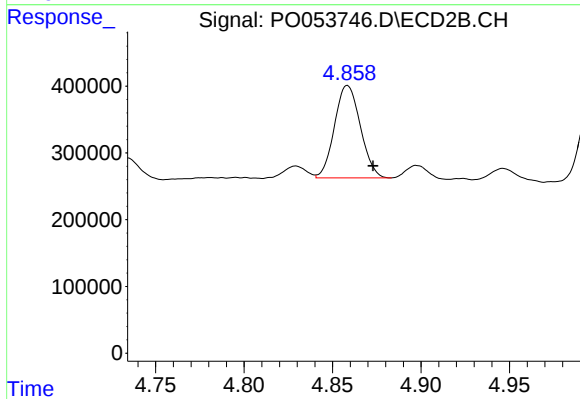

#20 AR-1242-5


R.T.: 4.858 min
Delta R.T.: -0.015 min
Response: 1408528
Conc: 191.71 ng/ml

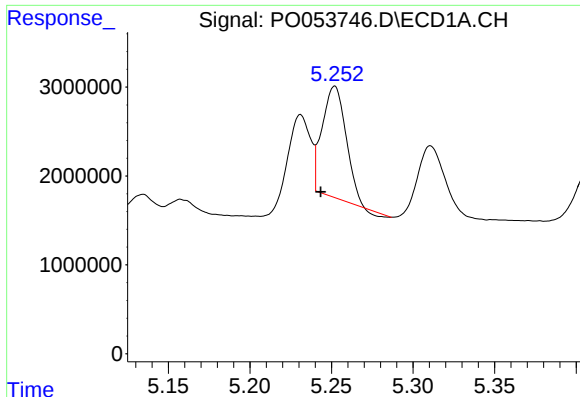

#21 AR-1248-1


R.T.: 5.252 min
Delta R.T.: 0.009 min
Response: 12538135
Conc: 458.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

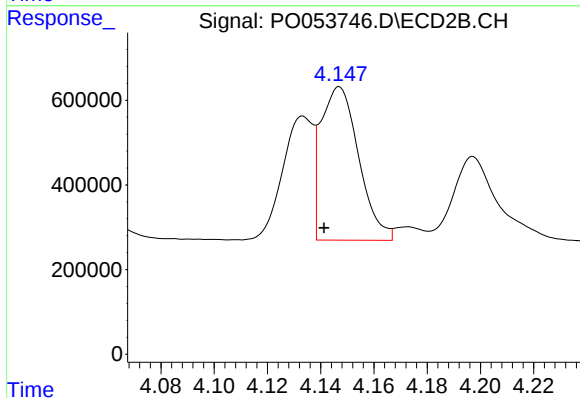


#21 AR-1248-1

R.T.: 4.147 min
Delta R.T.: 0.006 min
Response: 3582255
Conc: 625.12 ng/ml

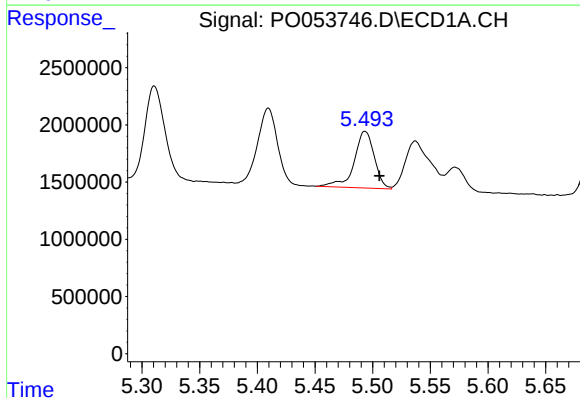


#22 AR-1248-2

R.T.: 5.493 min
Delta R.T.: -0.013 min
Response: 6039642
Conc: 183.32 ng/ml

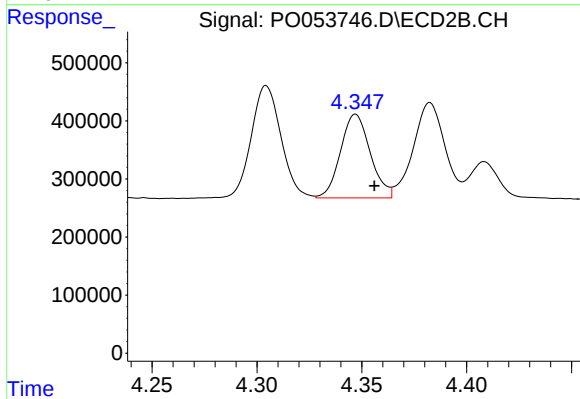

#22 AR-1248-2


R.T.: 4.347 min
Delta R.T.: -0.009 min
Response: 1424517
Conc: 187.79 ng/ml

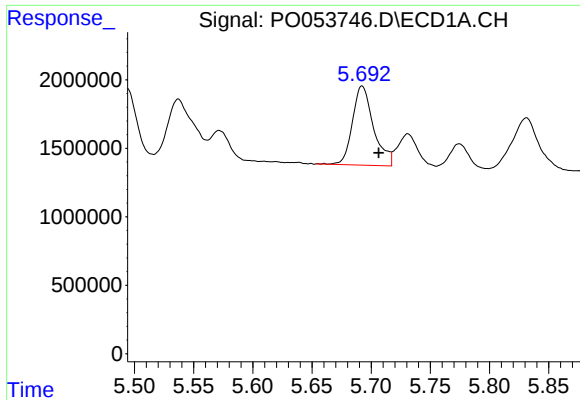

#23 AR-1248-3


R.T.: 5.692 min
Delta R.T.: -0.014 min
Response: 7156518
Conc: 186.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

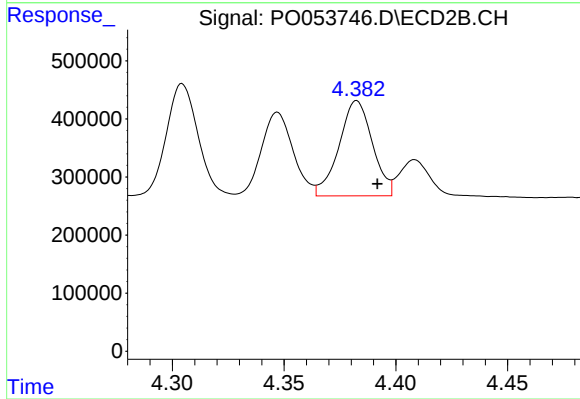


#23 AR-1248-3

R.T.: 4.383 min
Delta R.T.: -0.009 min
Response: 1707031
Conc: 217.87 ng/ml

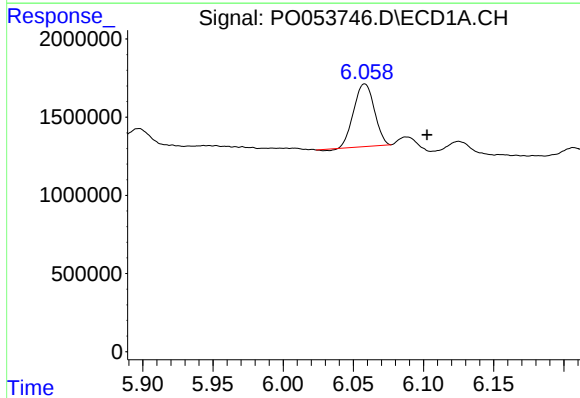


#24 AR-1248-4

R.T.: 6.058 min
Delta R.T.: -0.044 min
Response: 4080118
Conc: 97.21 ng/ml

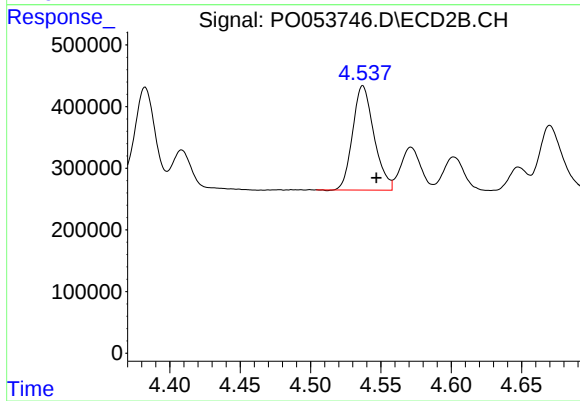

#24 AR-1248-4


R.T.: 4.537 min
Delta R.T.: -0.010 min
Response: 1789088
Conc: 180.20 ng/ml

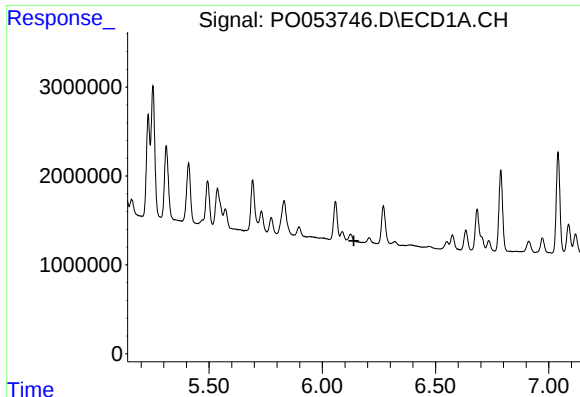

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

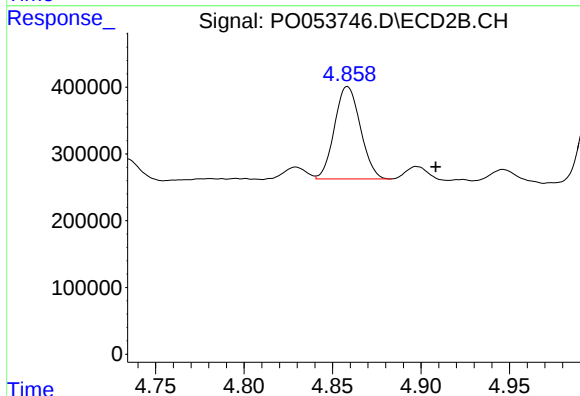


#25 AR-1248-5

R.T.: 4.858 min
Delta R.T.: -0.050 min
Response: 1408528
Conc: 136.03 ng/ml

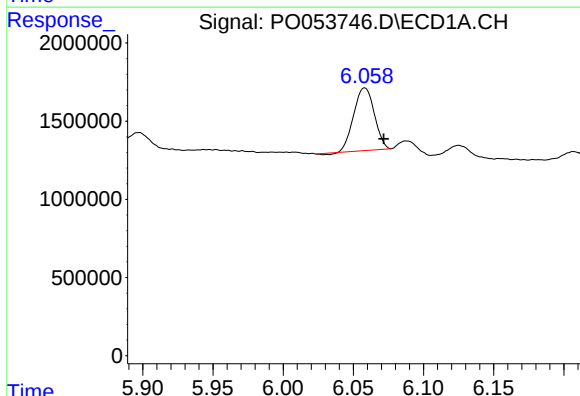


#26 AR-1254-1

R.T.: 6.058 min
Delta R.T.: -0.013 min
Response: 4080118
Conc: 97.04 ng/ml

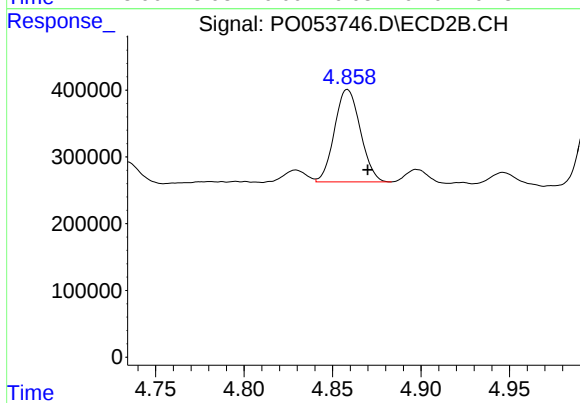

#26 AR-1254-1


R.T.: 4.858 min
Delta R.T.: -0.011 min
Response: 1408528
Conc: 86.48 ng/ml

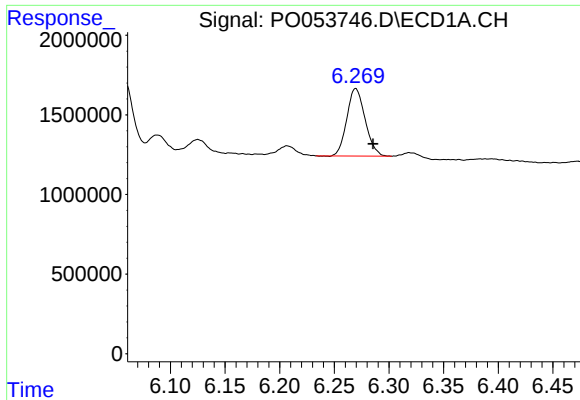

#27 AR-1254-2


R.T.: 6.270 min
Delta R.T.: -0.016 min
Response: 4961305
Conc: 76.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

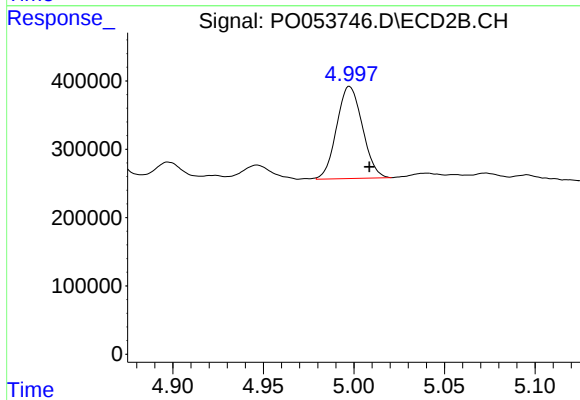


#27 AR-1254-2

R.T.: 4.998 min
Delta R.T.: -0.011 min
Response: 1335105
Conc: 96.80 ng/ml

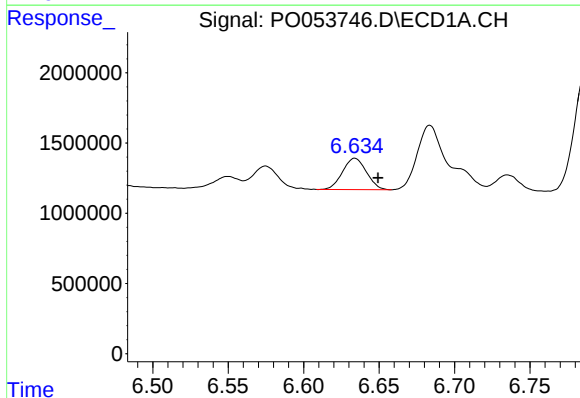


#28 AR-1254-3

R.T.: 6.634 min
Delta R.T.: -0.015 min
Response: 2464081
Conc: 35.99 ng/ml

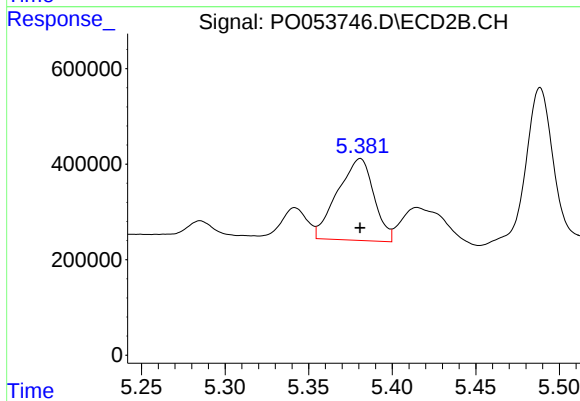

#28 AR-1254-3


R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 2591982
Conc: 118.58 ng/ml

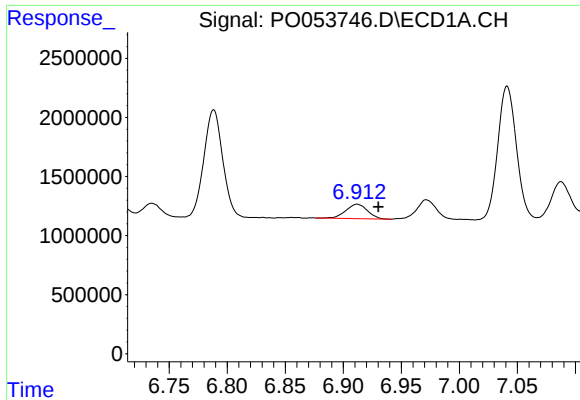

#29 AR-1254-4


R.T.: 6.912 min
Delta R.T.: -0.018 min
Response: 1585224
Conc: 31.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

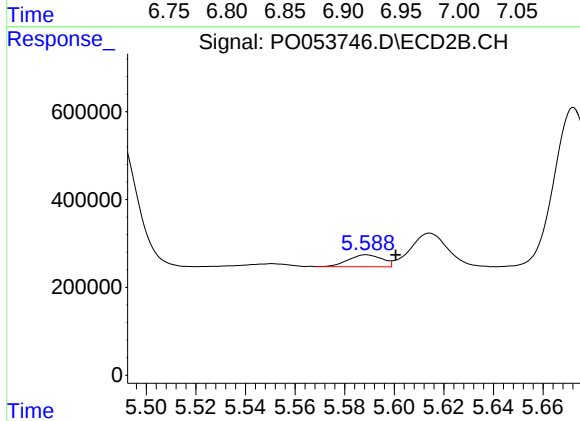


#29 AR-1254-4

R.T.: 5.589 min
Delta R.T.: -0.012 min
Response: 255250
Conc: 17.98 ng/ml

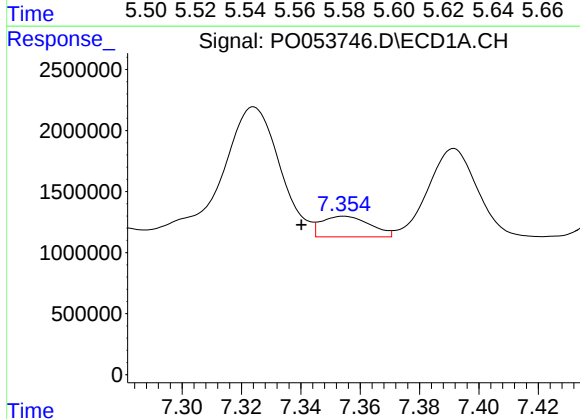


#30 AR-1254-5

R.T.: 7.355 min
Delta R.T.: 0.014 min
Response: 1910553
Conc: 39.92 ng/ml

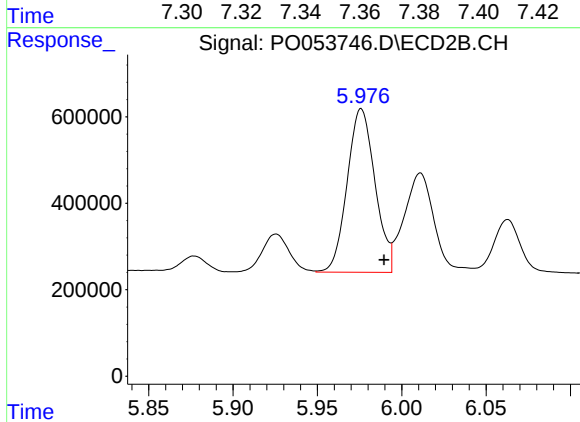

#30 AR-1254-5


R.T.: 5.976 min
Delta R.T.: -0.013 min
Response: 4346945
Conc: 232.71 ng/ml

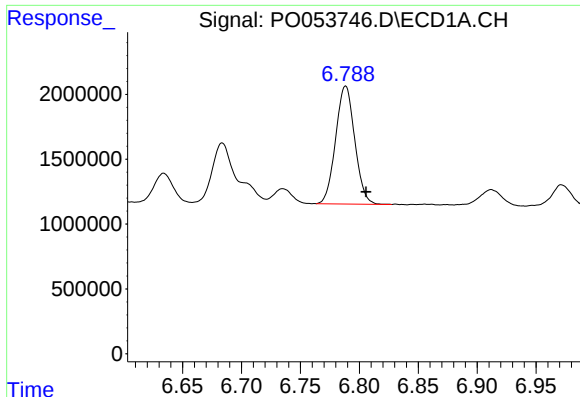

#31 AR-1260-1


R.T.: 6.788 min
Delta R.T.: -0.017 min
Response: 10275532
Conc: 210.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

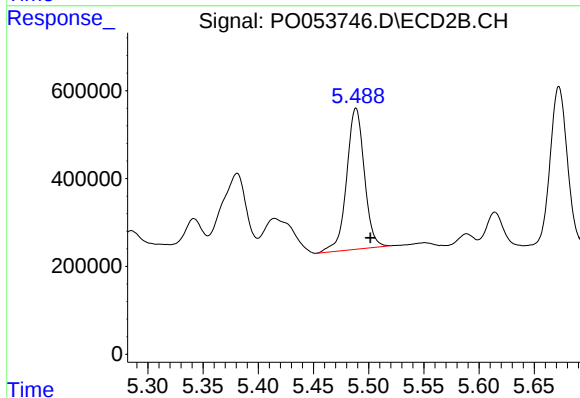


#31 AR-1260-1

R.T.: 5.489 min
Delta R.T.: -0.013 min
Response: 3583824
Conc: 235.36 ng/ml

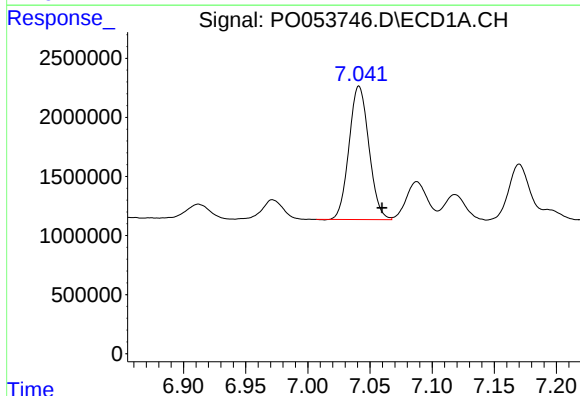


#32 AR-1260-2

R.T.: 7.041 min
Delta R.T.: -0.018 min
Response: 12589289
Conc: 202.58 ng/ml

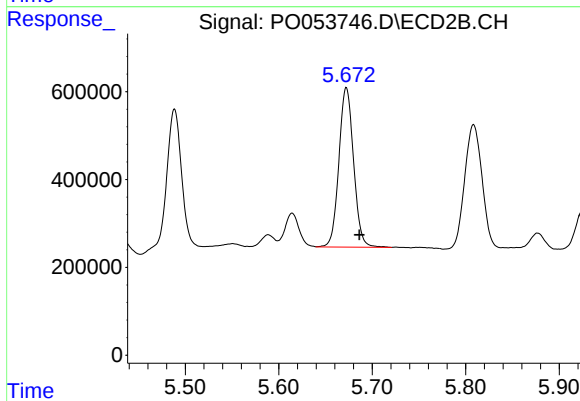

#32 AR-1260-2


R.T.: 5.672 min
Delta R.T.: -0.014 min
Response: 3963762
Conc: 213.78 ng/ml

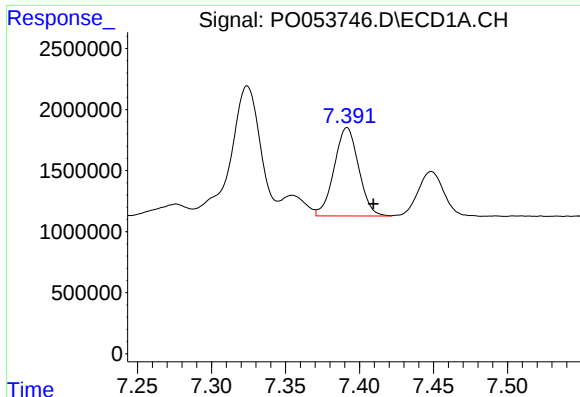

#33 AR-1260-3


R.T.: 7.392 min
Delta R.T.: -0.018 min
Response: 8351873
Conc: 213.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

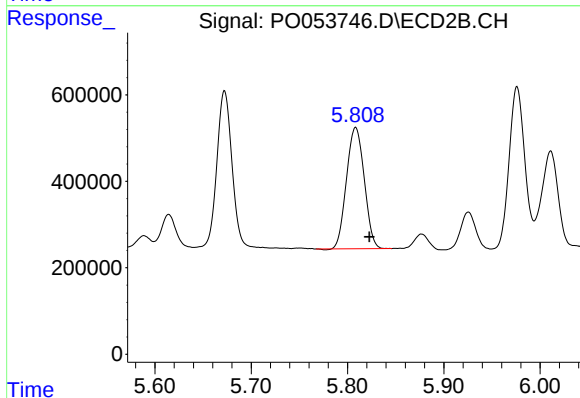


#33 AR-1260-3

R.T.: 5.808 min
Delta R.T.: -0.014 min
Response: 3582780
Conc: 209.58 ng/ml

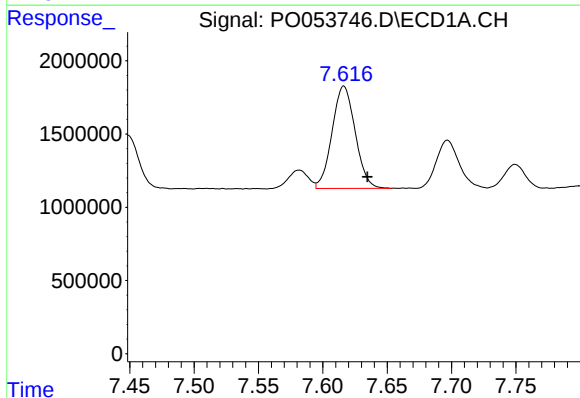


#34 AR-1260-4

R.T.: 7.616 min
Delta R.T.: -0.018 min
Response: 8755922
Conc: 202.63 ng/ml

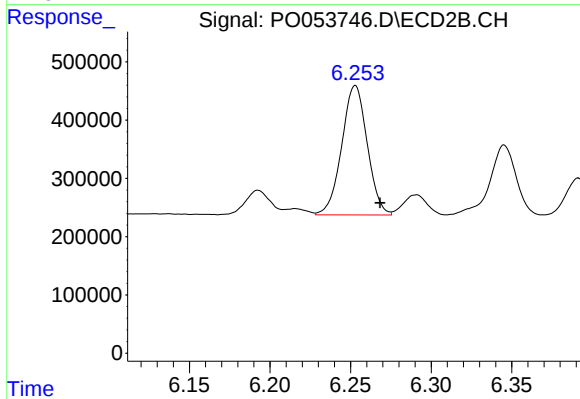

#34 AR-1260-4


R.T.: 6.253 min
Delta R.T.: -0.015 min
Response: 2449455
Conc: 222.43 ng/ml

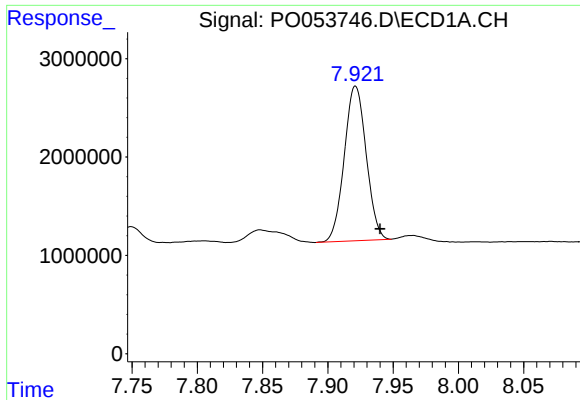

#35 AR-1260-5


R.T.: 7.921 min
Delta R.T.: -0.019 min
Response: 18392649
Conc: 202.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

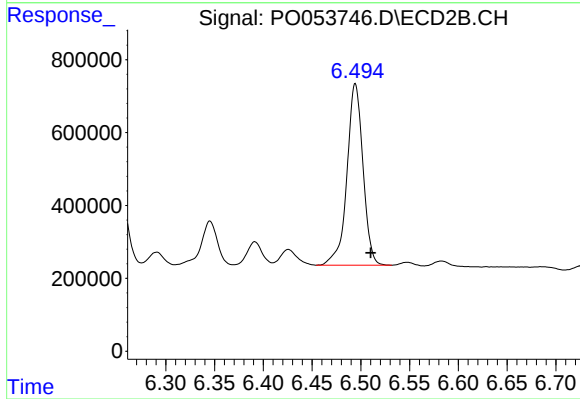


#35 AR-1260-5

R.T.: 6.494 min
Delta R.T.: -0.016 min
Response: 5709294
Conc: 209.66 ng/ml

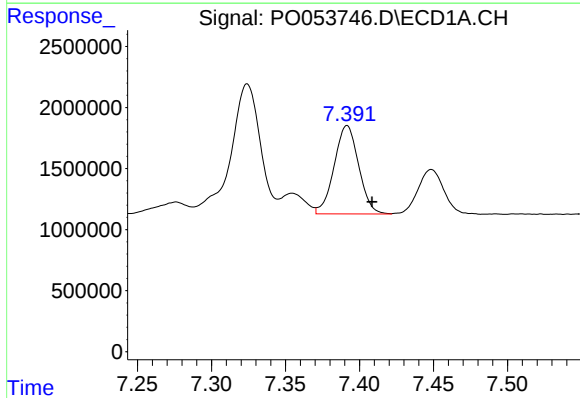


#36 AR-1262-1

R.T.: 7.392 min
Delta R.T.: -0.017 min
Response: 8351873
Conc: 121.72 ng/ml

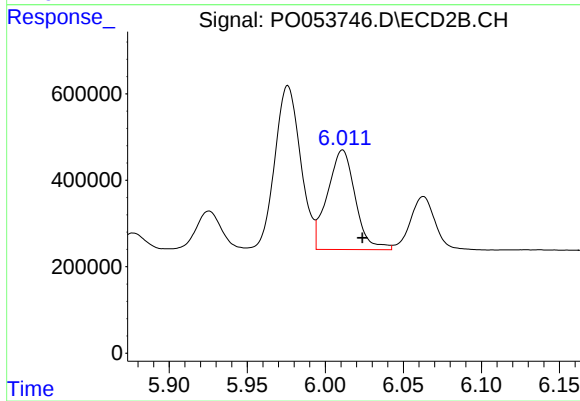

#36 AR-1262-1


R.T.: 6.011 min
Delta R.T.: -0.013 min
Response: 2861207
Conc: 144.47 ng/ml

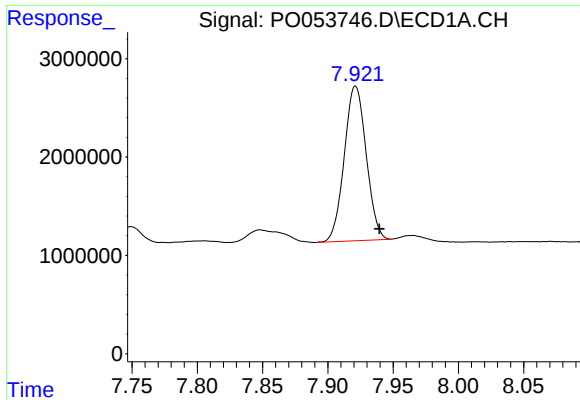

#37 AR-1262-2


R.T.: 7.921 min
Delta R.T.: -0.018 min
Response: 18392649
Conc: 152.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

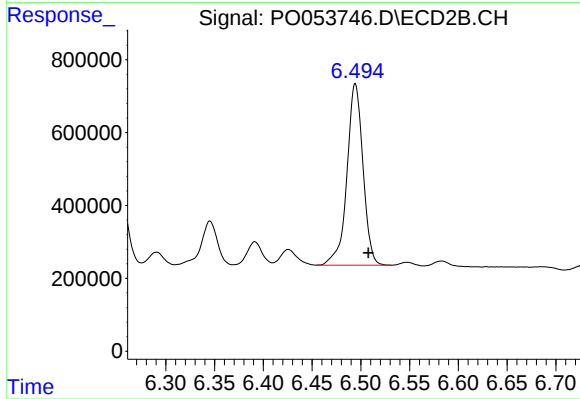


#37 AR-1262-2

R.T.: 6.494 min
Delta R.T.: -0.013 min
Response: 5709294
Conc: 168.11 ng/ml

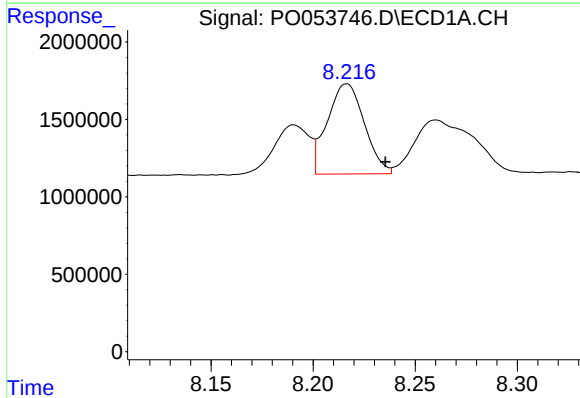


#38 AR-1262-3

R.T.: 8.216 min
Delta R.T.: -0.019 min
Response: 7356984
Conc: 298.33 ng/ml

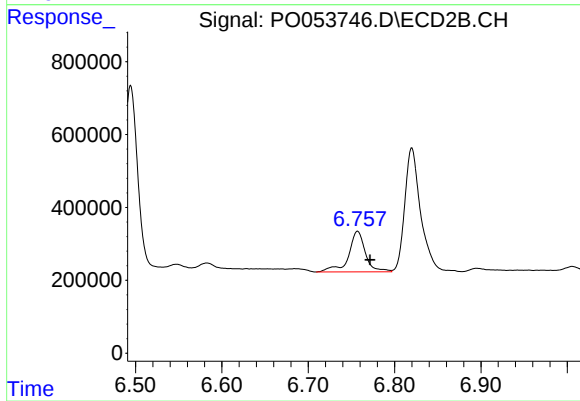

#38 AR-1262-3


R.T.: 6.757 min
Delta R.T.: -0.014 min
Response: 1512620
Conc: 116.35 ng/ml

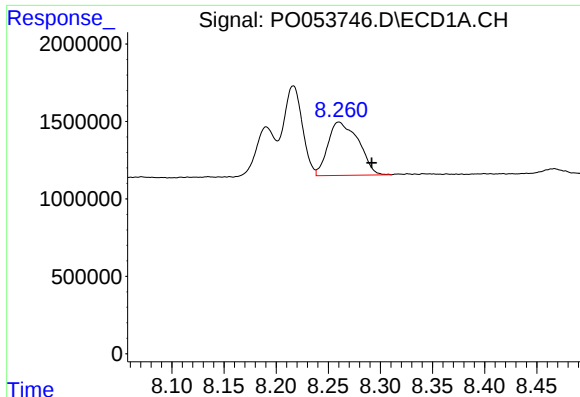

#39 AR-1262-4


R.T.: 8.260 min
Delta R.T.: -0.032 min
Response: 6995909
Conc: 112.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

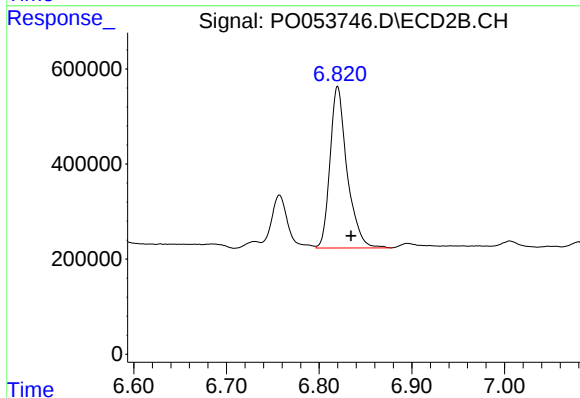


#39 AR-1262-4

R.T.: 6.820 min
Delta R.T.: -0.014 min
Response: 4349322
Conc: 177.70 ng/ml

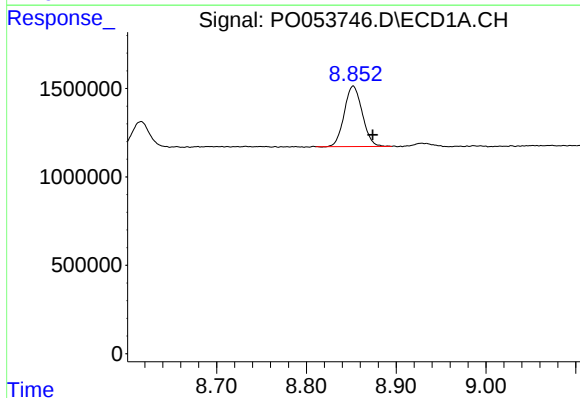


#40 AR-1262-5

R.T.: 8.852 min
Delta R.T.: -0.022 min
Response: 4775754
Conc: 113.07 ng/ml

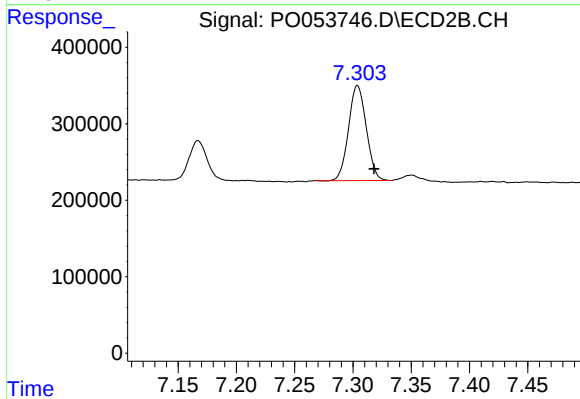

#40 AR-1262-5


R.T.: 7.304 min
Delta R.T.: -0.014 min
Response: 1321951
Conc: 118.26 ng/ml

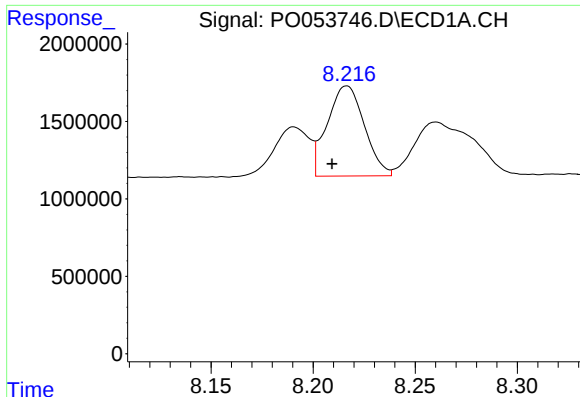

#41 AR-1268-1


R.T.: 8.216 min
Delta R.T.: 0.007 min
Response: 7356984
Conc: 49.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

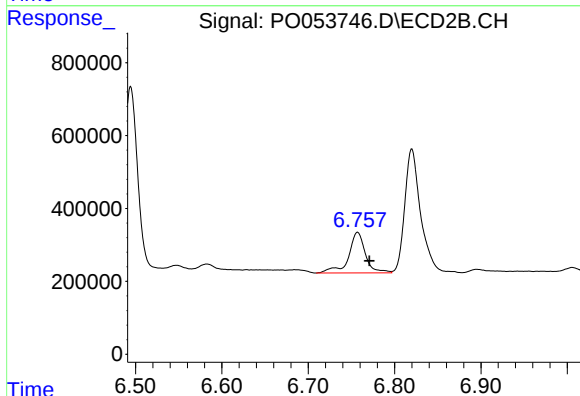


#41 AR-1268-1

R.T.: 6.757 min
Delta R.T.: -0.013 min
Response: 1512620
Conc: 39.17 ng/ml

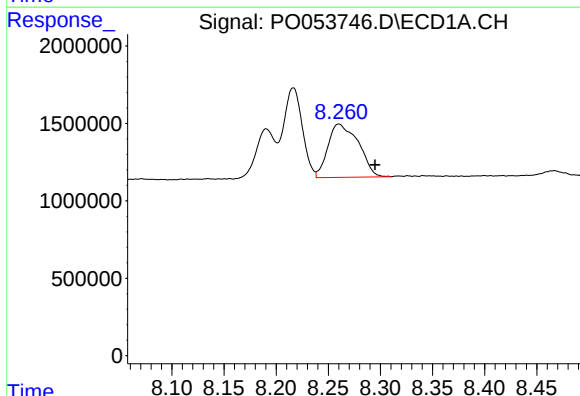


#42 AR-1268-2

R.T.: 8.260 min
Delta R.T.: -0.035 min
Response: 6995909
Conc: 49.85 ng/ml

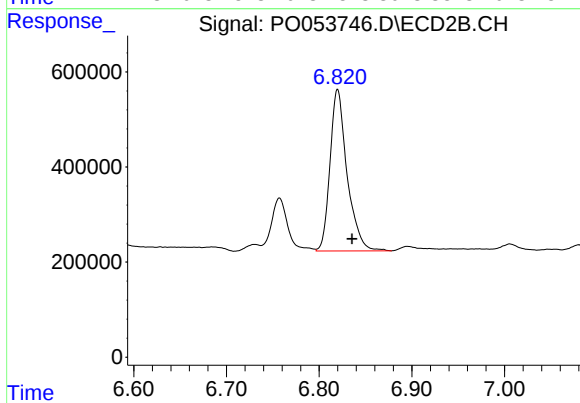

#42 AR-1268-2


R.T.: 6.820 min
Delta R.T.: -0.016 min
Response: 4349322
Conc: 118.94 ng/ml

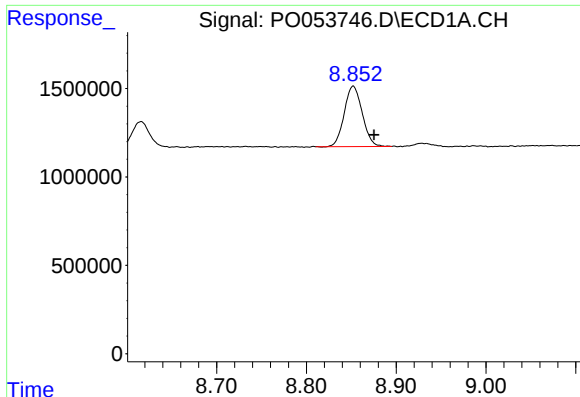

#44 AR-1268-4


R.T.: 8.852 min
Delta R.T.: -0.023 min
Response: 4775754
Conc: 100.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

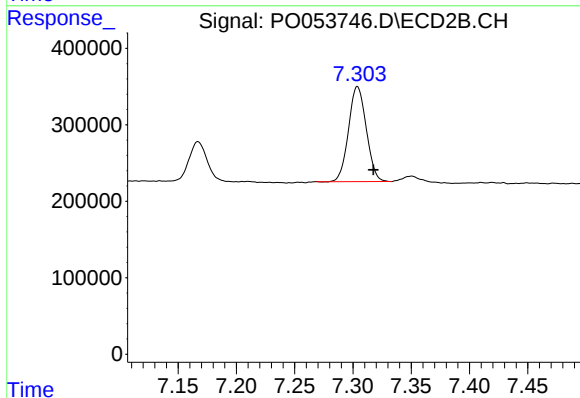


#44 AR-1268-4

R.T.: 7.304 min
Delta R.T.: -0.014 min
Response: 1321951
Conc: 106.15 ng/ml

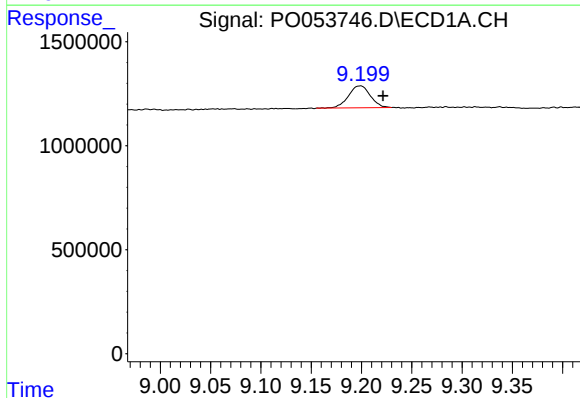

#45 AR-1268-5

R.T.: 9.199 min
Delta R.T.: -0.023 min
Response: 1587445
Conc: 4.23 ng/ml

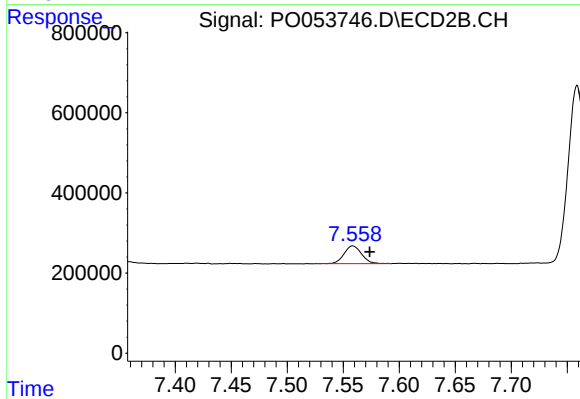

#45 AR-1268-5

R.T.: 7.559 min
Delta R.T.: -0.015 min
Response: 482906
Conc: 5.15 ng/ml