

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
 Data File : P0053740.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2019 11:05
 Operator : SM/SJ
 Sample : K1376-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-01

Manual Integrations
 APPROVED

Sohil
 2/8/2019 5:15:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:32:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.093	3.159	3380074	519593	1.734	2.166m
2) SA Decachlor...	9.472	7.761	1785373	525104	1.832	2.103

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
Data File : P0053740.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2019 11:05
Operator : SM/SJ
Sample : K1376-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-01


Manual Integrations
APPROVED

Sohil
2/8/2019 5:15:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:32:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

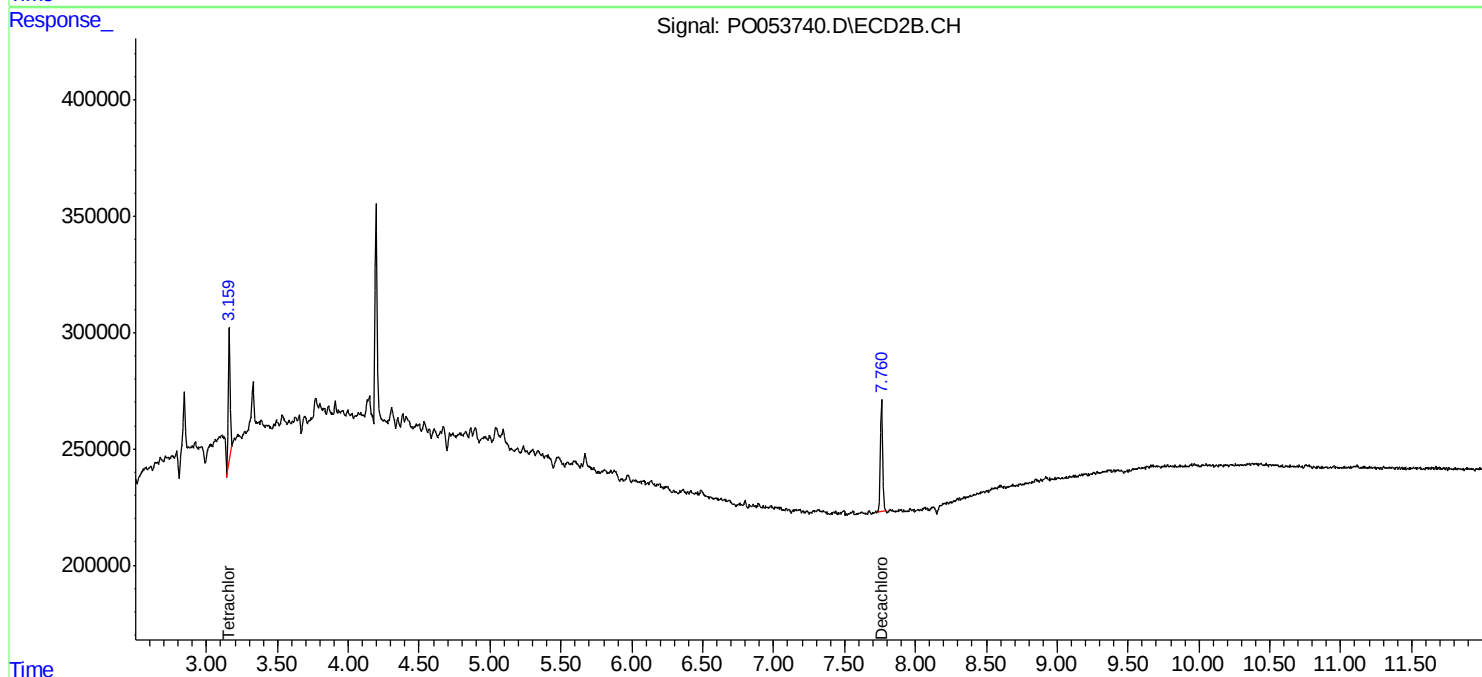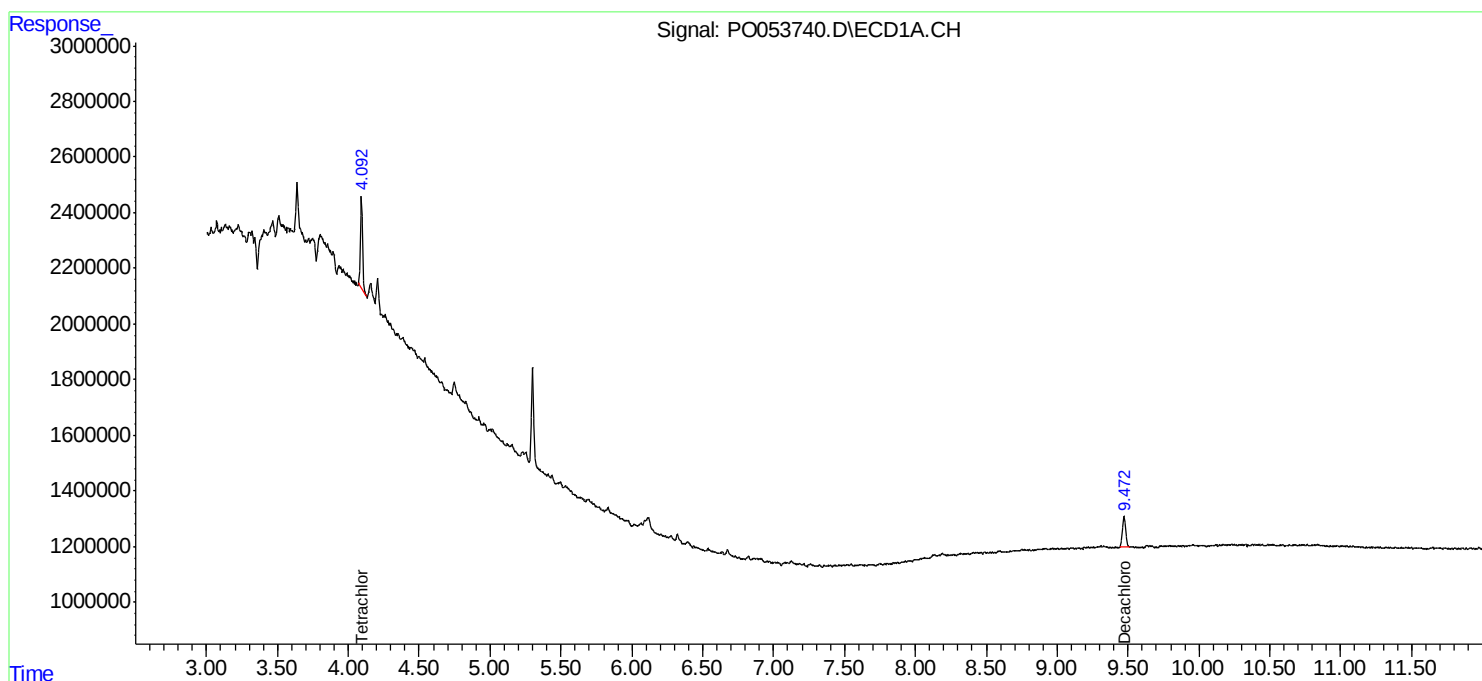

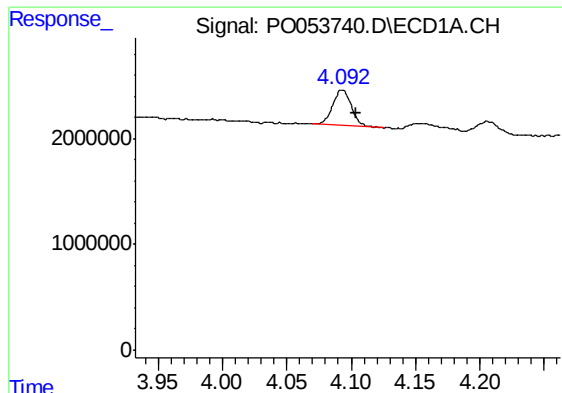


#1 Tetrachloro-m-xylene

R.T.: 4.093 min
Delta R.T.: -0.011 min
Response: 3380074
Conc: 1.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-01


Manual Integrations
APPROVED

Sohil
2/8/2019 5:15:33 PM

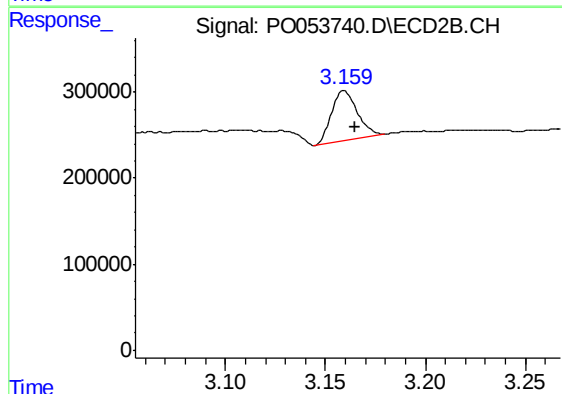


#1 Tetrachloro-m-xylene

R.T.: 3.159 min
Delta R.T.: -0.006 min
Response: 519593
Conc: 2.17 ng/ml m

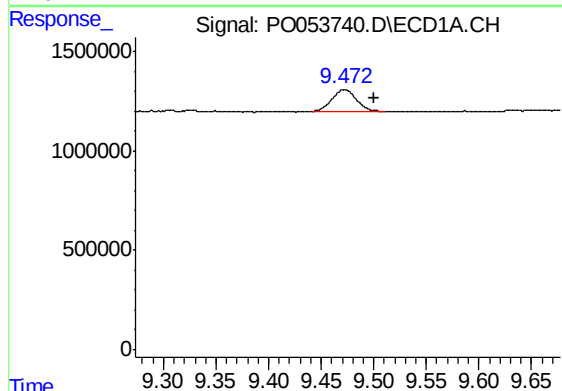

#2 Decachlorobiphenyl

R.T.: 9.472 min
Delta R.T.: -0.029 min
Response: 1785373
Conc: 1.83 ng/ml

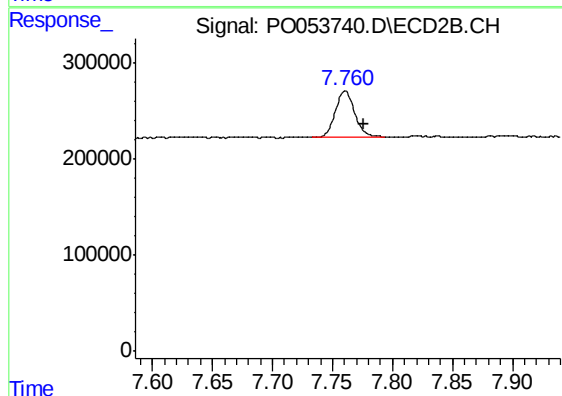

#2 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: -0.016 min
Response: 525104
Conc: 2.10 ng/ml