

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
 Data File : P0053756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2019 16:51
 Operator : SM/SJ
 Sample : K1350-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-03-020419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:41:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.099	3.160	36933461	5319360	18.949	22.178
2)	SA Decachlor...	9.479	7.763	16164603	3558232	16.585	14.250

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
Data File : P0053756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2019 16:51
Operator : SM/SJ
Sample : K1350-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EO-03-020419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:41:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

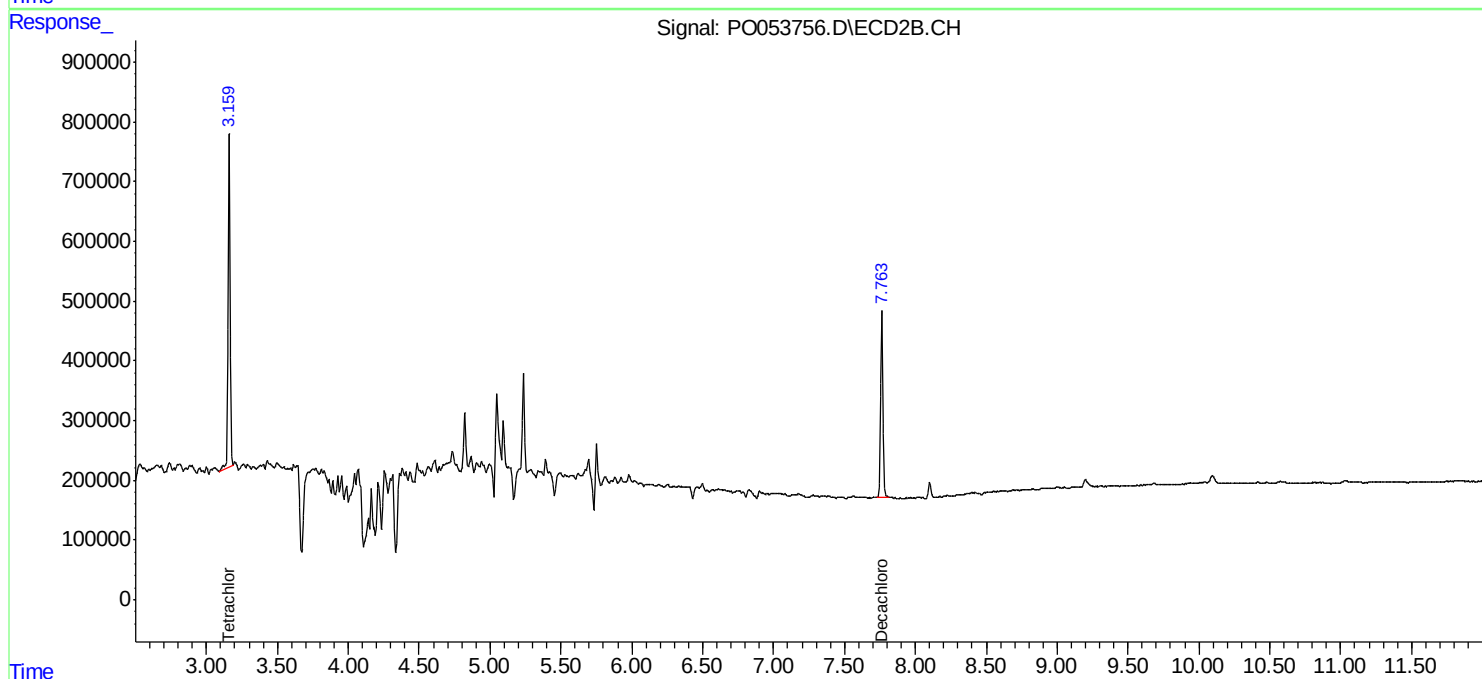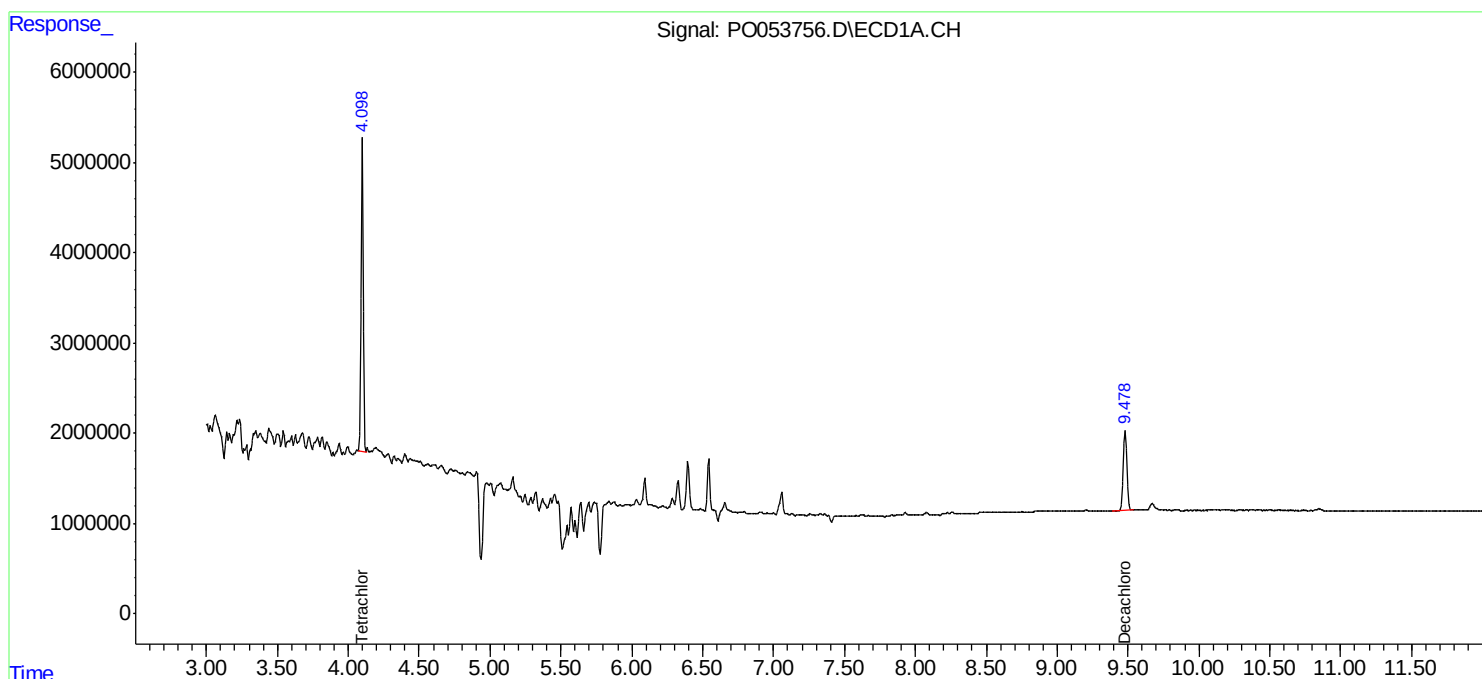


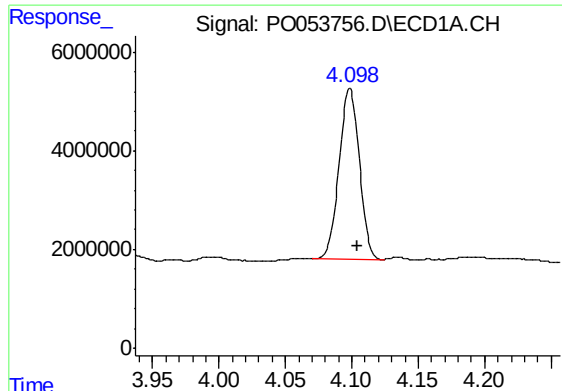

#1 Tetrachloro-m-xylene


R.T.: 4.099 min
Delta R.T.: -0.005 min
Response: 36933461
Conc: 18.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-03-020419-A

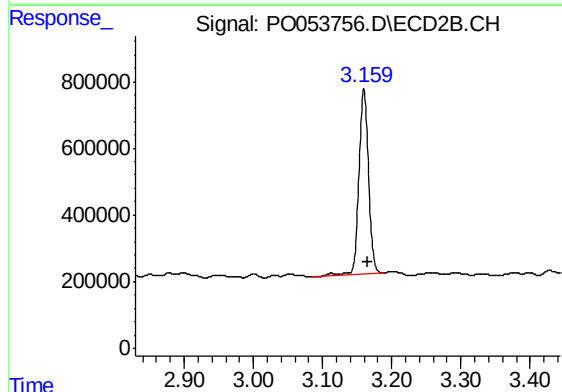


#1 Tetrachloro-m-xylene

R.T.: 3.160 min
Delta R.T.: -0.005 min
Response: 5319360
Conc: 22.18 ng/ml

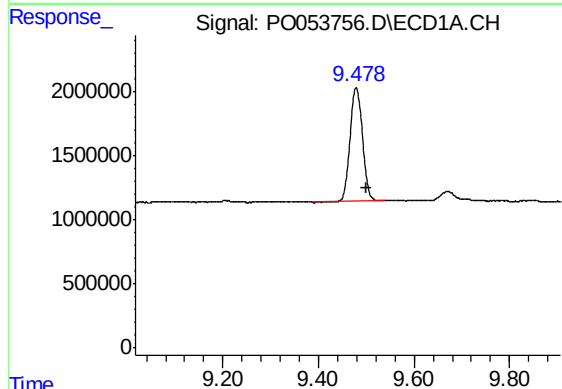

#2 Decachlorobiphenyl

R.T.: 9.479 min
Delta R.T.: -0.022 min
Response: 16164603
Conc: 16.59 ng/ml

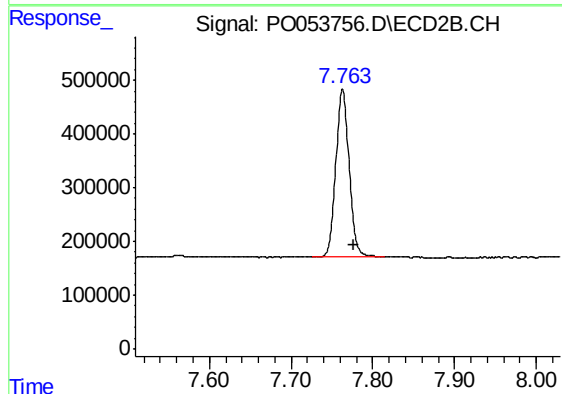

#2 Decachlorobiphenyl

R.T.: 7.763 min
Delta R.T.: -0.013 min
Response: 3558232
Conc: 14.25 ng/ml