

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
 Data File : P0053761.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Feb 2019 18:15
 Operator : SM/SJ
 Sample : K1346-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-020419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 23:44:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.094	3.161	40124117	6370640	20.586	26.561 #
2) SA Decachlor...	9.473	7.761	13041435	2742945	13.381	10.985

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_O\Data\po020619\
Data File : P0053761.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Feb 2019 18:15
Operator : SM/SJ
Sample : K1346-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-020419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 23:44:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

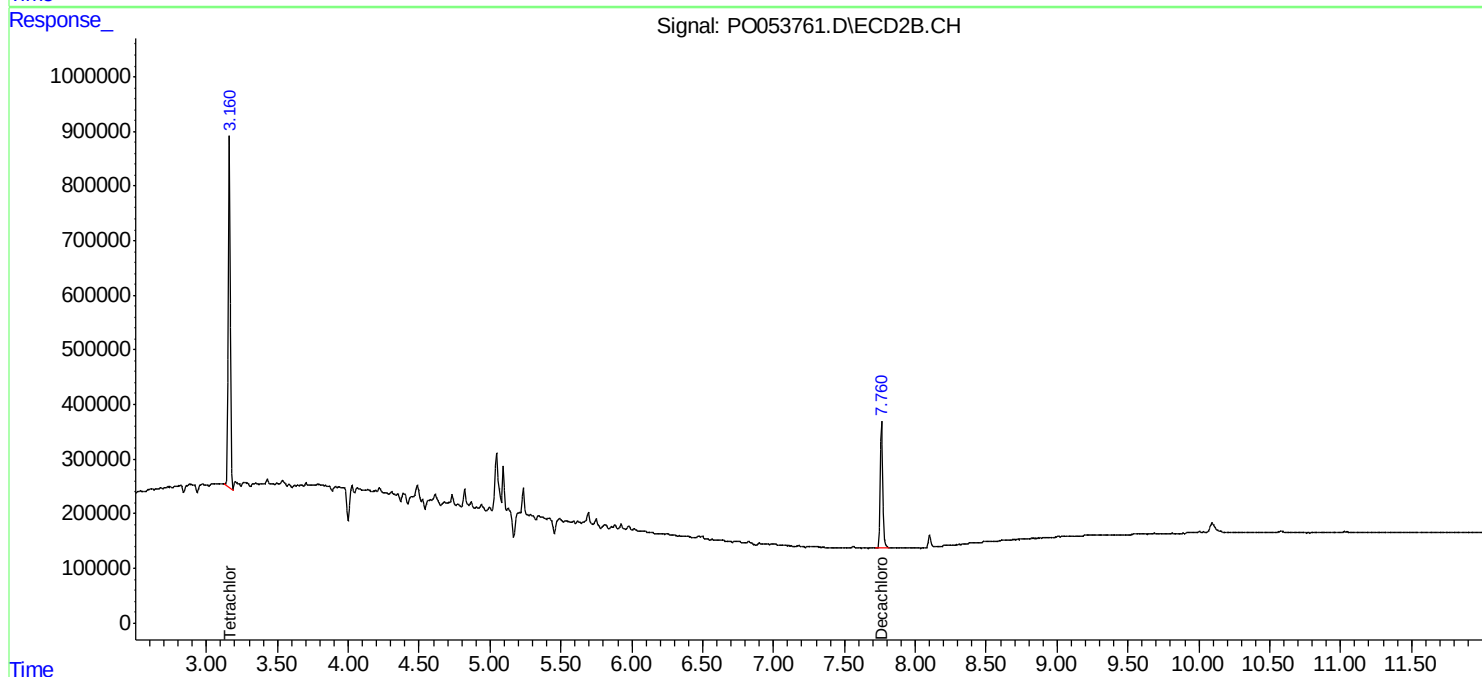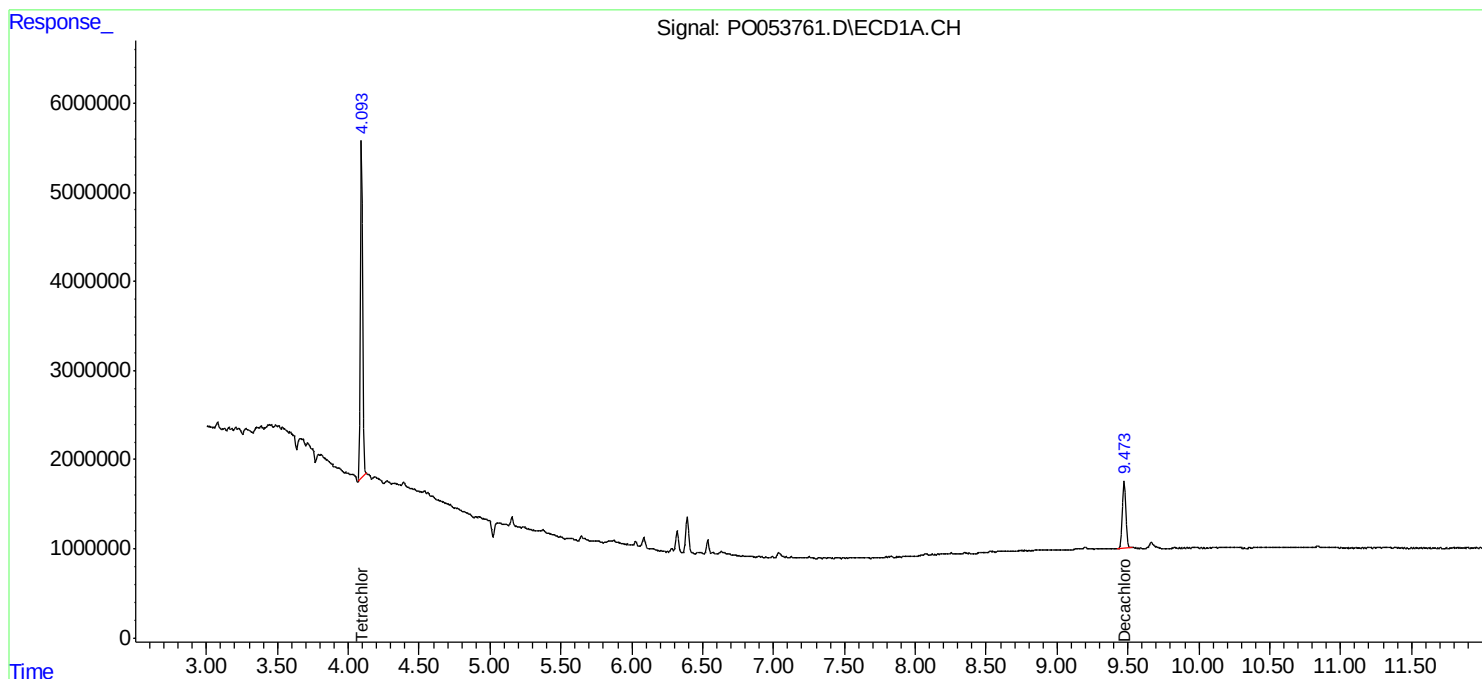


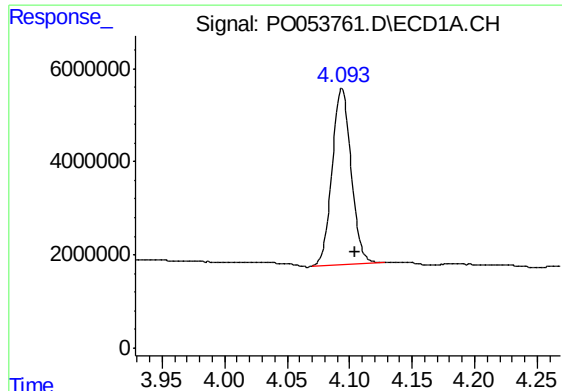

#1 Tetrachloro-m-xylene


R.T.: 4.094 min
Delta R.T.: -0.010 min
Response: 40124117
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-020419-A

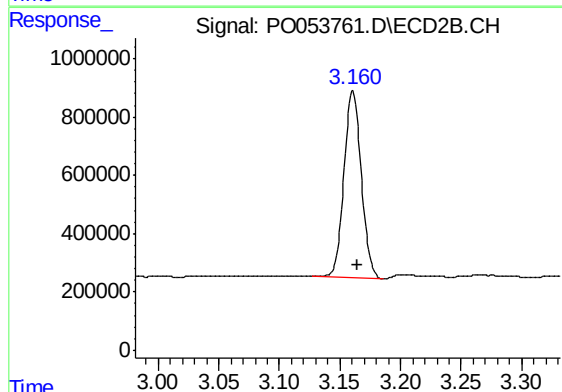


#1 Tetrachloro-m-xylene

R.T.: 3.161 min
Delta R.T.: -0.004 min
Response: 6370640
Conc: 26.56 ng/ml

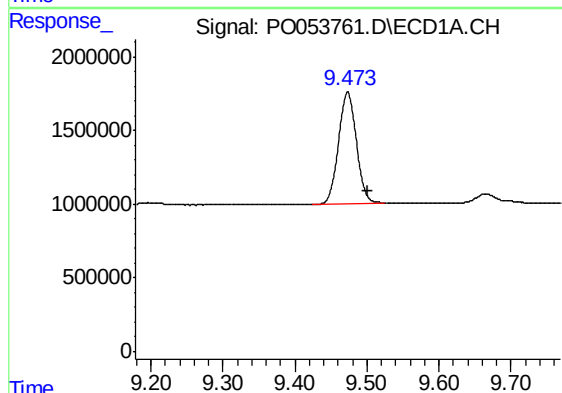

#2 Decachlorobiphenyl

R.T.: 9.473 min
Delta R.T.: -0.027 min
Response: 13041435
Conc: 13.38 ng/ml

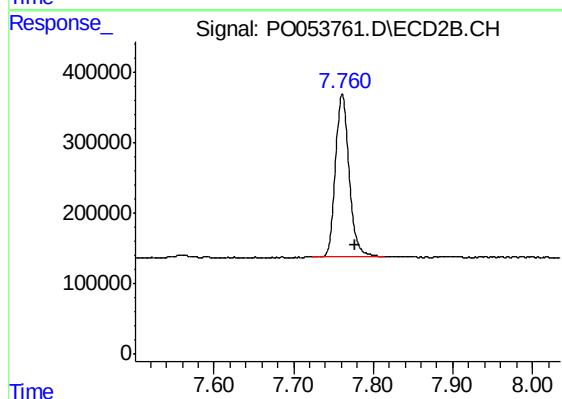

#2 Decachlorobiphenyl

R.T.: 7.761 min
Delta R.T.: -0.015 min
Response: 2742945
Conc: 10.98 ng/ml