

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020820\
 Data File : P0066379.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Feb 2020 19:24
 Operator : DD\AJ
 Sample : L1431-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-209

Manual Integrations
 APPROVED

mohammad
 2/11/2020 3:48:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 23:27:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 06 18:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.143	3.421	702150	970905	24.892m	24.724
2) SA Decachlor...	9.636	8.318	765742	968316	18.542	16.643

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020820\
Data File : PO066379.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Feb 2020 19:24
Operator : DD\AJ
Sample : L1431-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-209


Manual Integrations
APPROVED

mohammad
2/11/2020 3:48:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 23:27:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

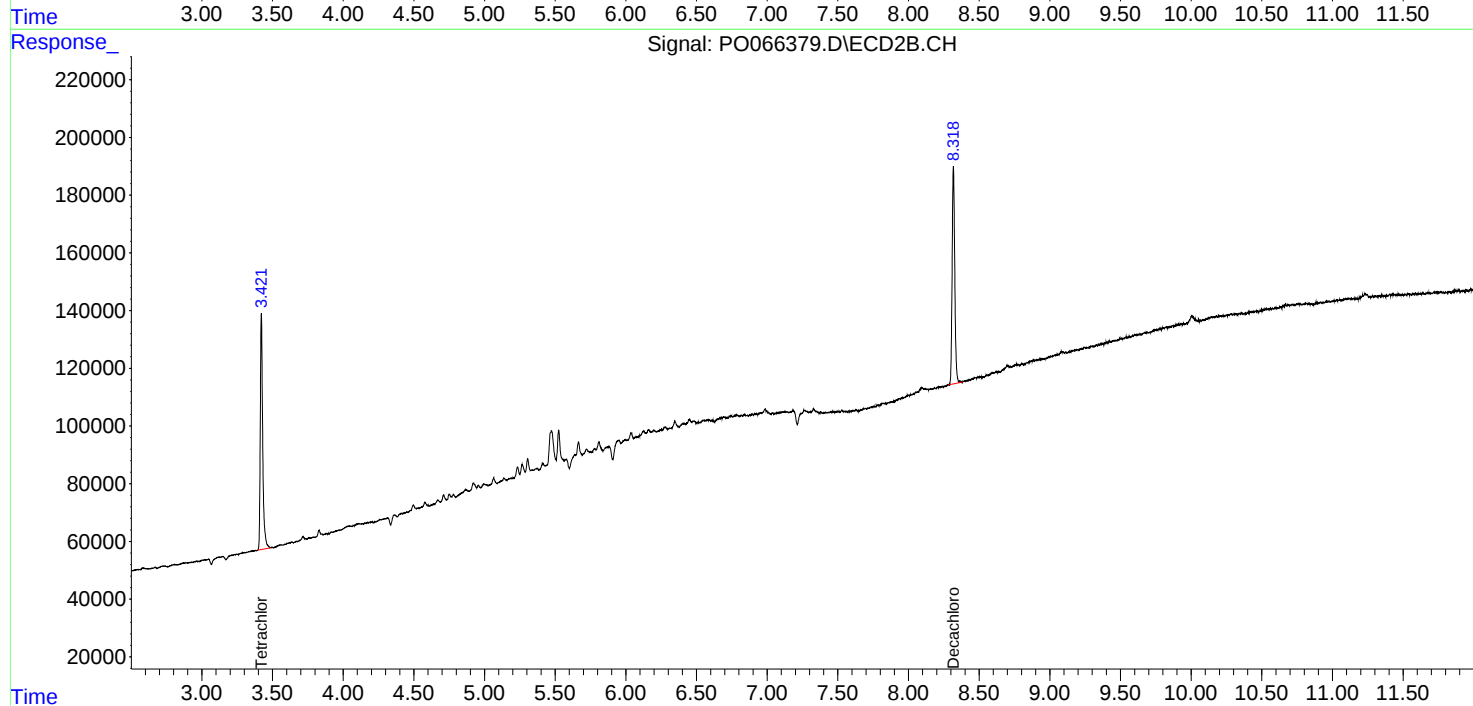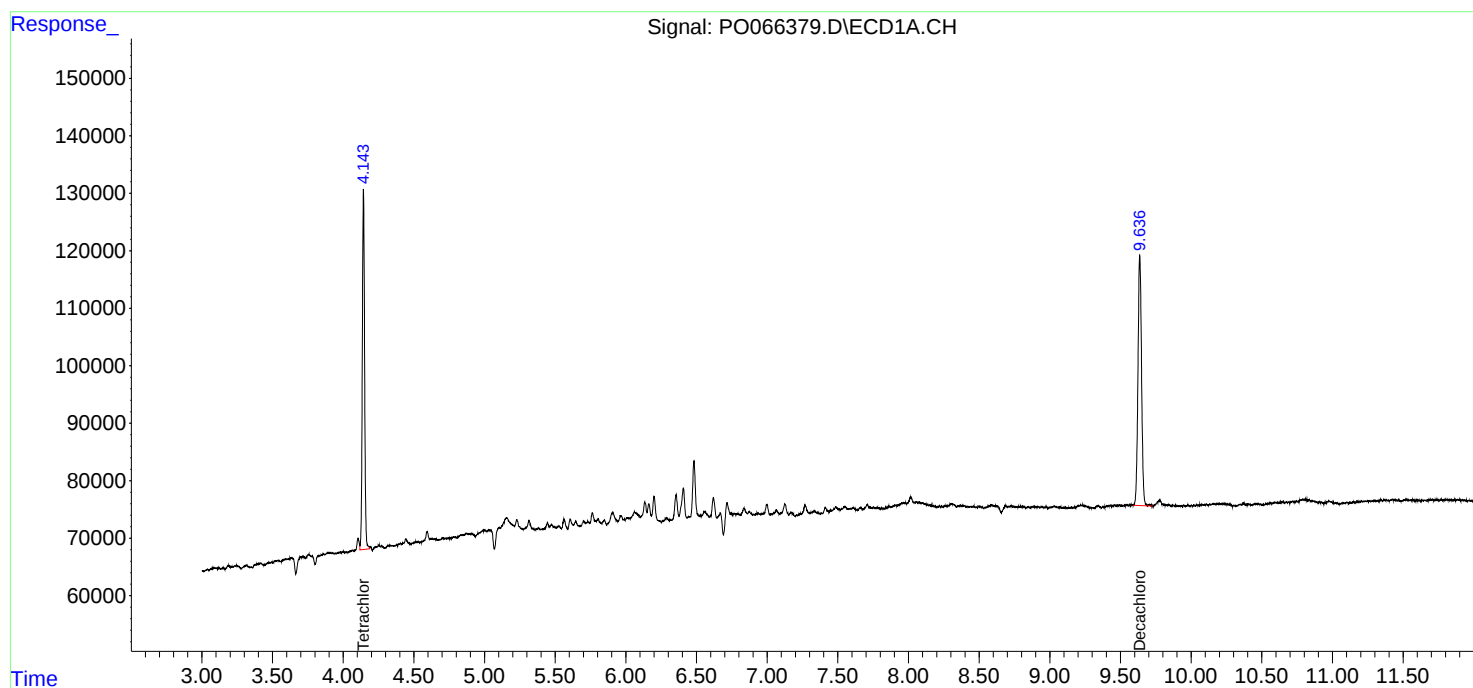

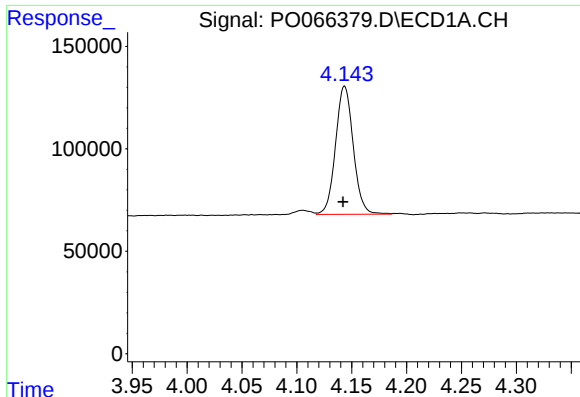


#1 Tetrachloro-m-xylene

R.T.: 4.143 min
Delta R.T.: 0.001 min
Response: 702150
Conc: 24.89 ng/ml m

Instrument :
ECD_O
ClientSampleId :
VNJ-209


Manual Integrations
APPROVED

mohammad
2/11/2020 3:48:13 PM

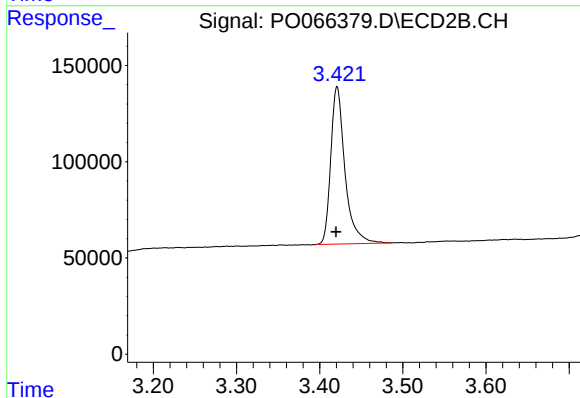


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.002 min
Response: 970905
Conc: 24.72 ng/ml

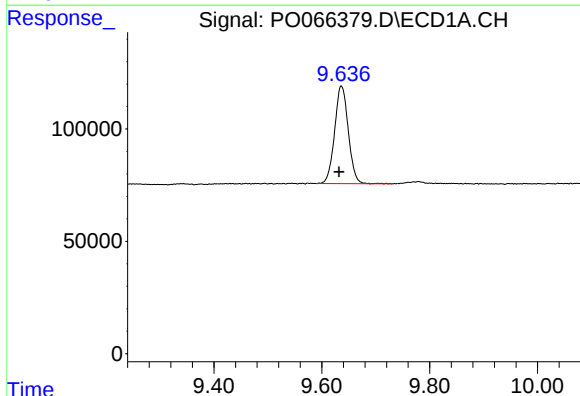

#2 Decachlorobiphenyl

R.T.: 9.636 min
Delta R.T.: 0.004 min
Response: 765742
Conc: 18.54 ng/ml

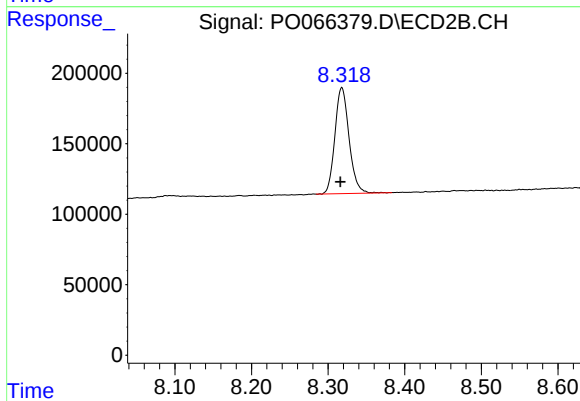

#2 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: 0.002 min
Response: 968316
Conc: 16.64 ng/ml