

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020820\
Data File : P0066383.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Feb 2020 20:31
Operator : DD\AJ
Sample : L1429-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
STORM-DRAIN-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 23:29:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.144	3.421	701179	938321	24.858	23.894
2) SA Decachlor...	9.638	8.319	1022988	1337568	24.772	22.989

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020820\
Data File : P0066383.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Feb 2020 20:31
Operator : DD\AJ
Sample : L1429-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
STORM-DRAIN-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 23:29:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

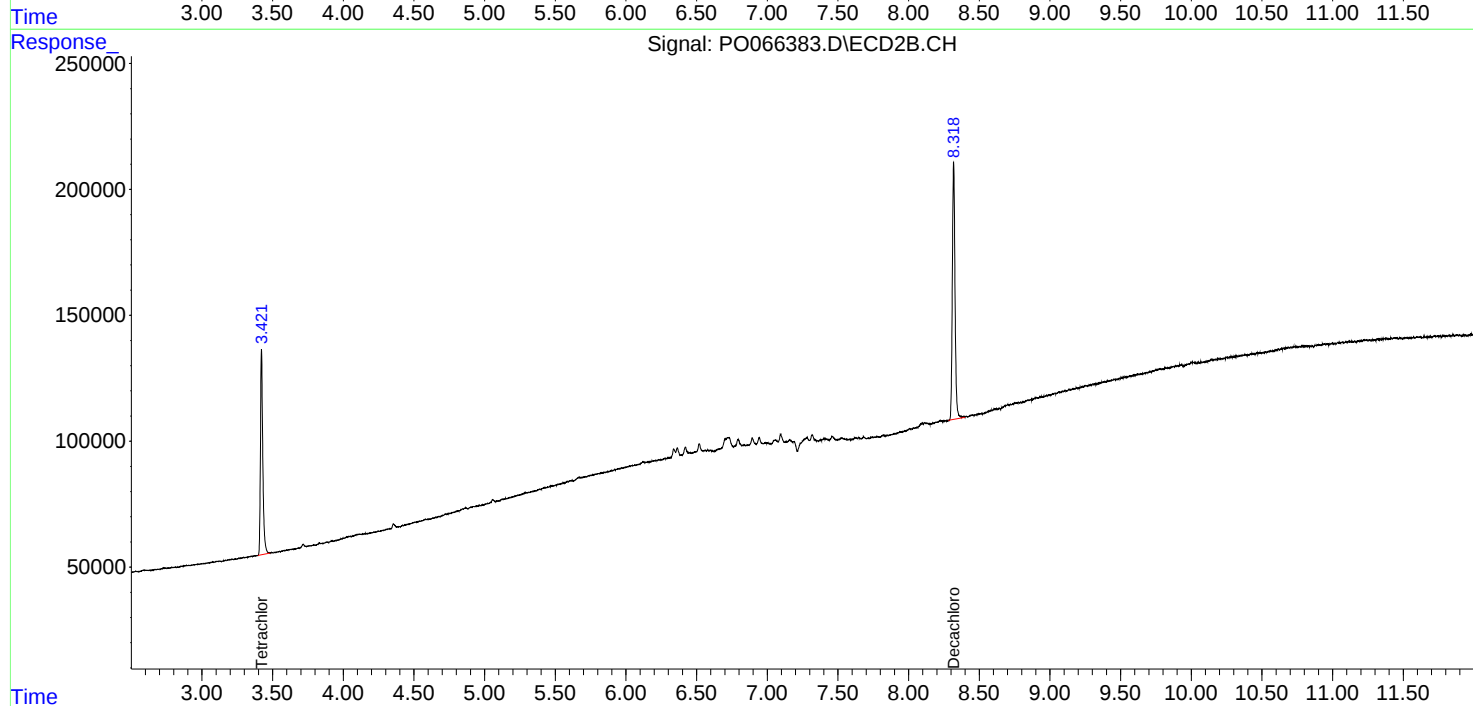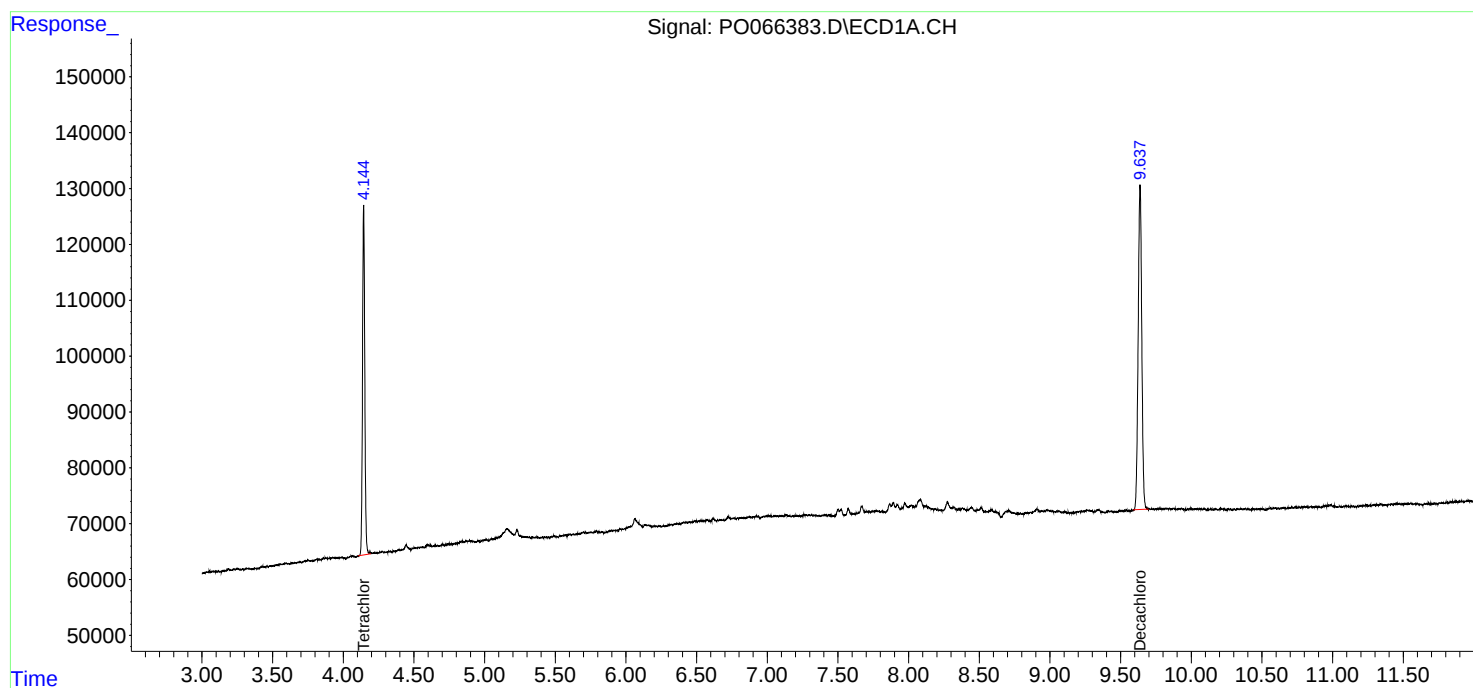


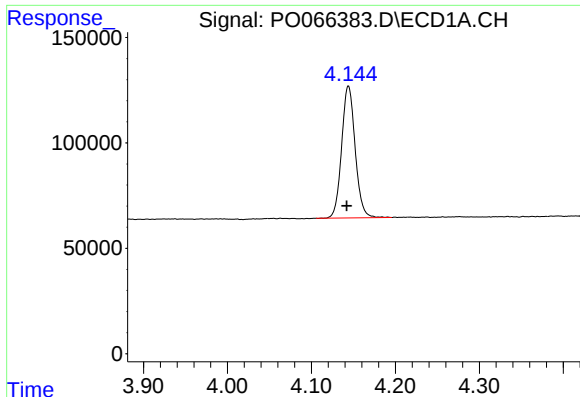

#1 Tetrachloro-m-xylene


R.T.: 4.144 min
Delta R.T.: 0.002 min
Response: 701179
Conc: 24.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
STORM-DRAIN-PIPE

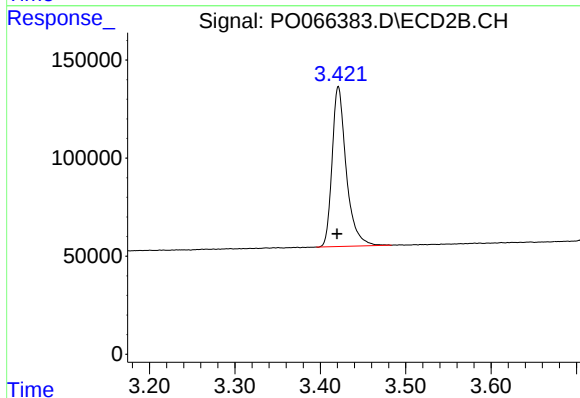


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.002 min
Response: 938321
Conc: 23.89 ng/ml

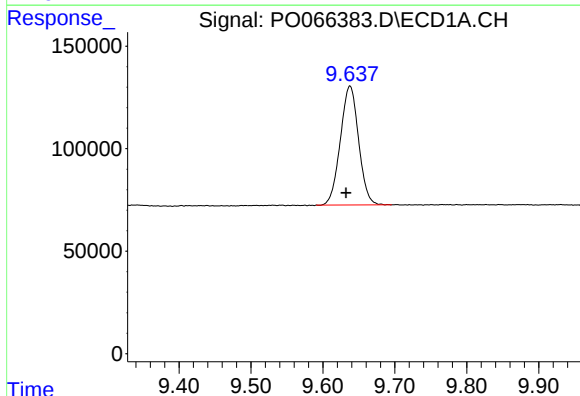

#2 Decachlorobiphenyl

R.T.: 9.638 min
Delta R.T.: 0.005 min
Response: 1022988
Conc: 24.77 ng/ml

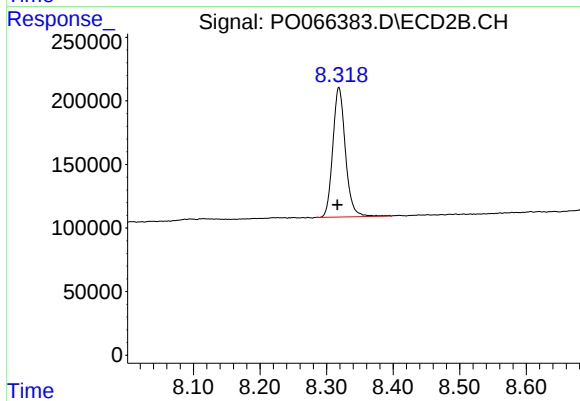

#2 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.002 min
Response: 1337568
Conc: 22.99 ng/ml