

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020820\
 Data File : P0066395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Feb 2020 3:36
 Operator : DD\AJ
 Sample : L1419-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 51067

Manual Integrations
 APPROVED

mohammad
 2/11/2020 3:48:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 04:25:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 06 18:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.144	3.421	653315	1008775	23.161	25.688m
2) SA Decachlor...	9.632	8.315	301240	418826	7.295	7.198

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020820\
Data File : P0066395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Feb 2020 3:36
Operator : DD\AJ
Sample : L1419-08
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
51067


Manual Integrations
APPROVED

mohammad
2/11/2020 3:48:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 04:25:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

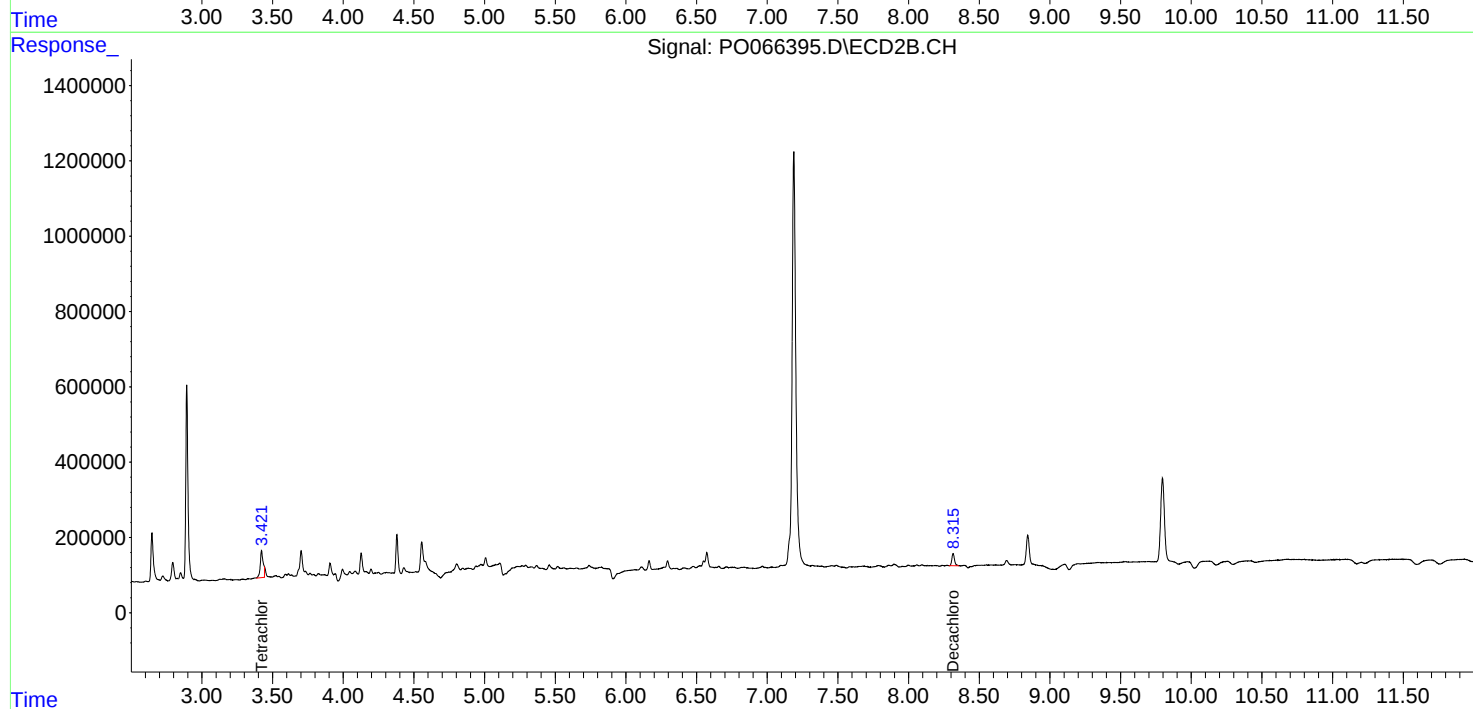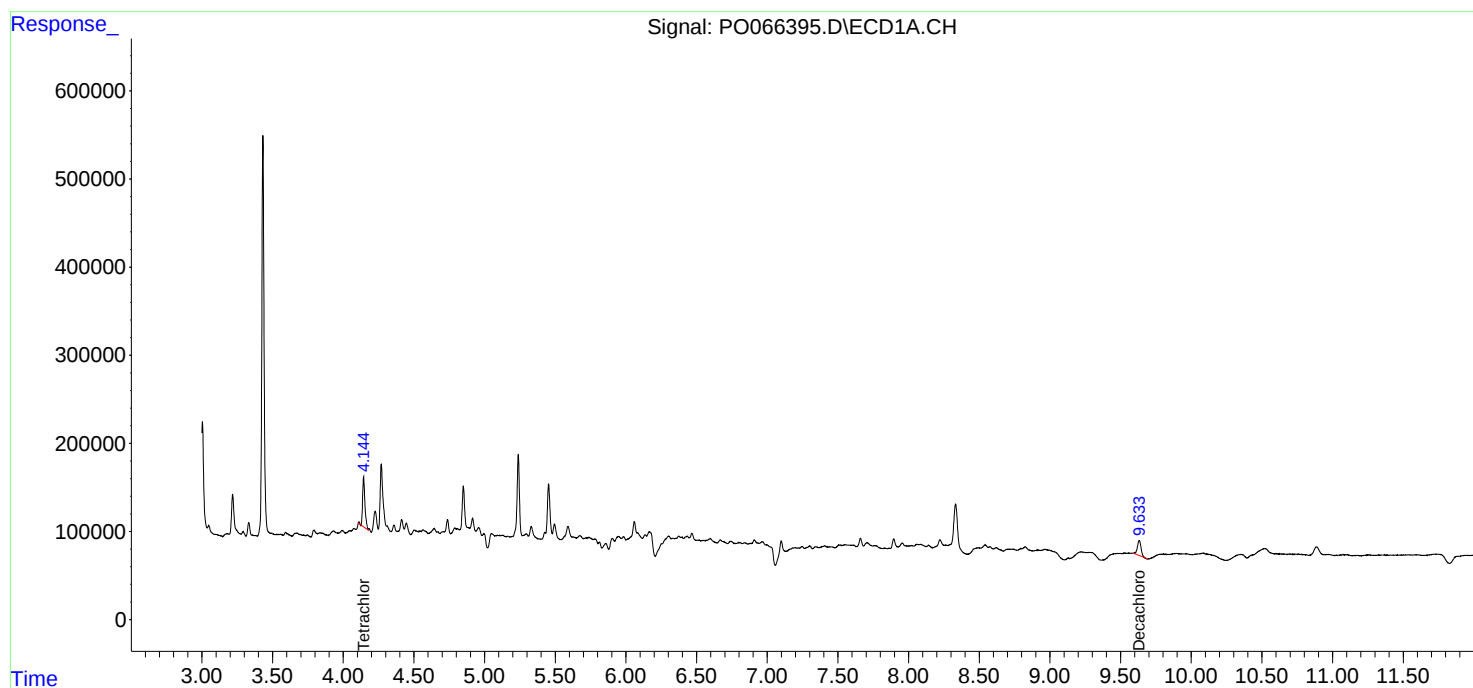

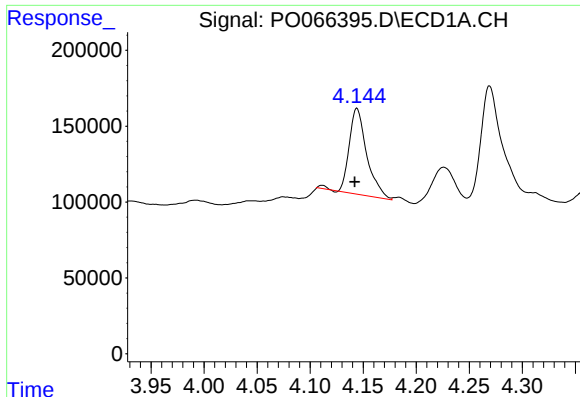


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.002 min
Response: 653315
Conc: 23.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
51067


Manual Integrations
APPROVED

mohammad
2/11/2020 3:48:31 PM

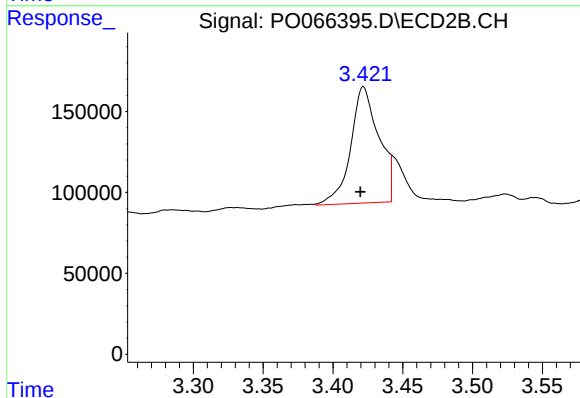


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.002 min
Response: 1008775
Conc: 25.69 ng/ml m

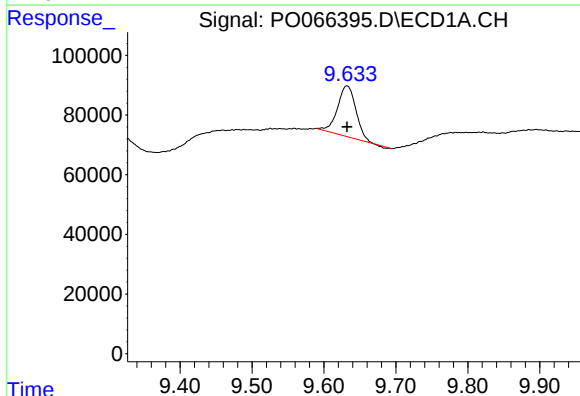

#2 Decachlorobiphenyl

R.T.: 9.632 min
Delta R.T.: 0.000 min
Response: 301240
Conc: 7.29 ng/ml

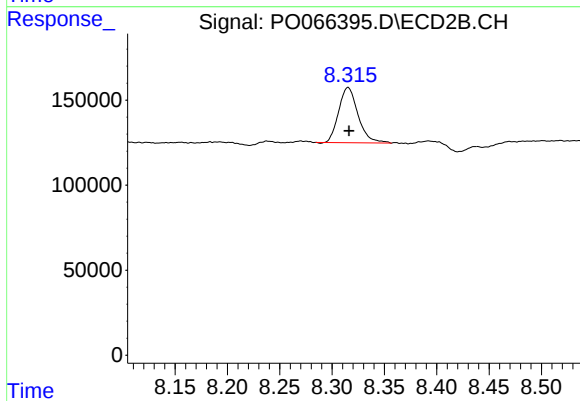

#2 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 418826
Conc: 7.20 ng/ml