

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021219\
 Data File : P0053816.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Feb 2019 18:51
 Operator : SM/SJ
 Sample : K1458-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-2

Manual Integrations
 APPROVED

Sohil
 2/13/2019 2:38:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 00:37:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 11 14:15:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.076	3.147	47571183	4481160	13.383	16.416m
2) SA Decachlor...	9.441	7.740	14058623	2791056	11.196	9.987

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021219\
Data File : P0053816.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2019 18:51
Operator : SM/SJ
Sample : K1458-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-2


Manual Integrations
APPROVED

Sohil
2/13/2019 2:38:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 00:37:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 11 14:15:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

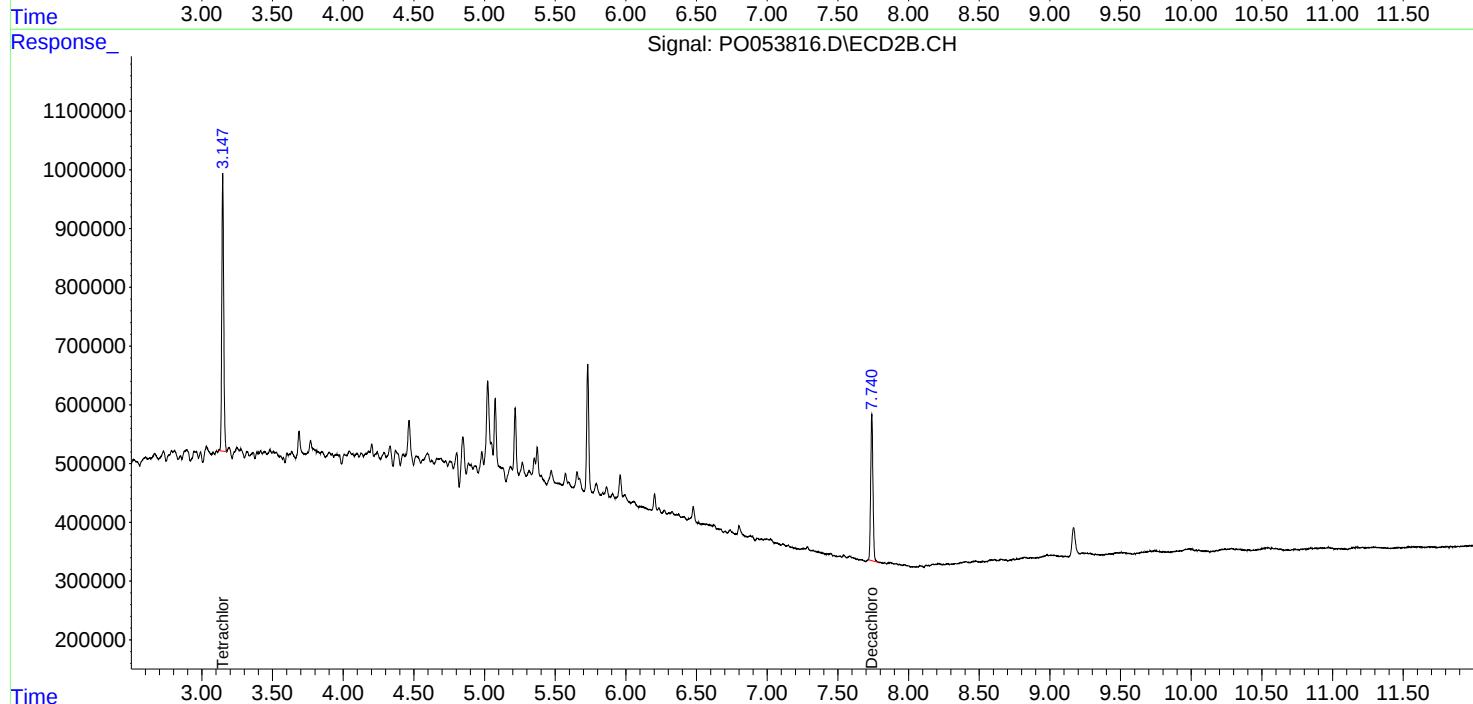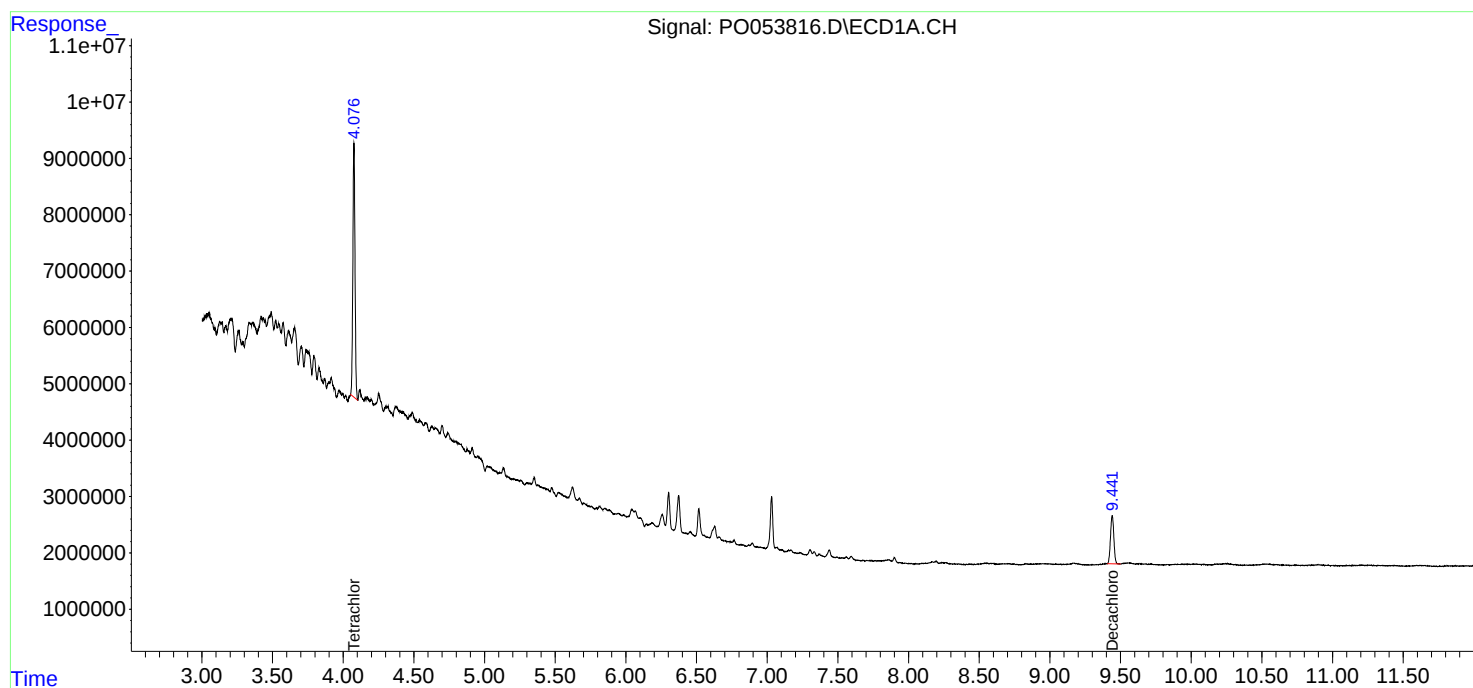

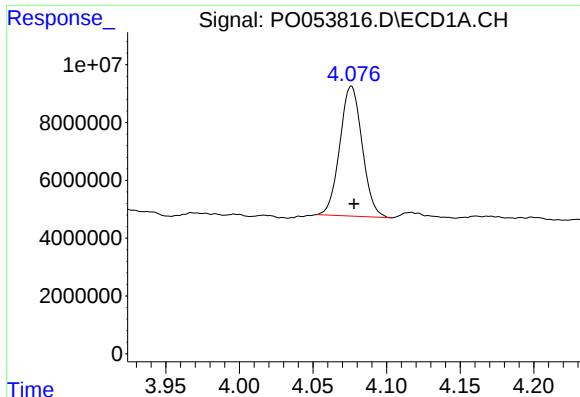


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.002 min
Response: 47571183
Conc: 13.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-2


Manual Integrations
APPROVED

Sohil
2/13/2019 2:38:24 PM

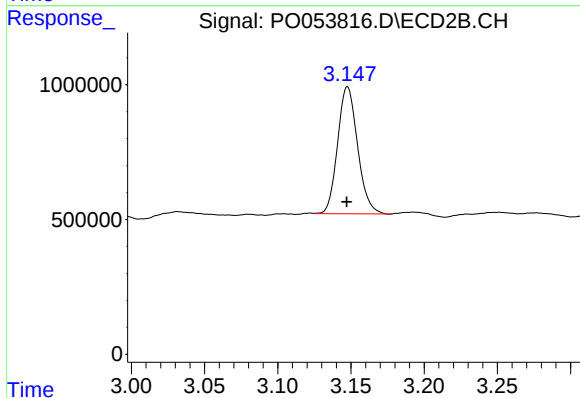


#1 Tetrachloro-m-xylene

R.T.: 3.147 min
Delta R.T.: 0.000 min
Response: 4481160
Conc: 16.42 ng/ml m

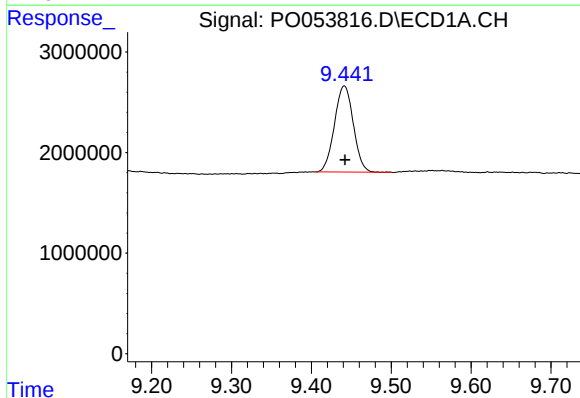

#2 Decachlorobiphenyl

R.T.: 9.441 min
Delta R.T.: 0.000 min
Response: 14058623
Conc: 11.20 ng/ml

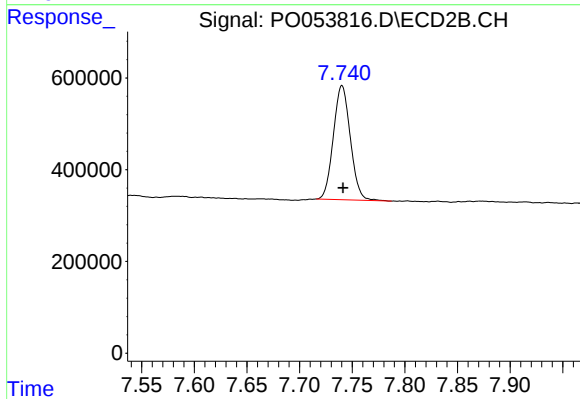

#2 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: -0.001 min
Response: 2791056
Conc: 9.99 ng/ml