

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021220\
Data File : P0066481.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2020 12:42
Operator : DD\AJ
Sample : L1479-03DL 2000X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-021020-SR-02DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 03:39:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021220\
Data File : P0066481.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Feb 2020 12:42
Operator : DD\AJ
Sample : L1479-03DL 2000X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-021020-SR-02DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 03:39:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 06 18:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

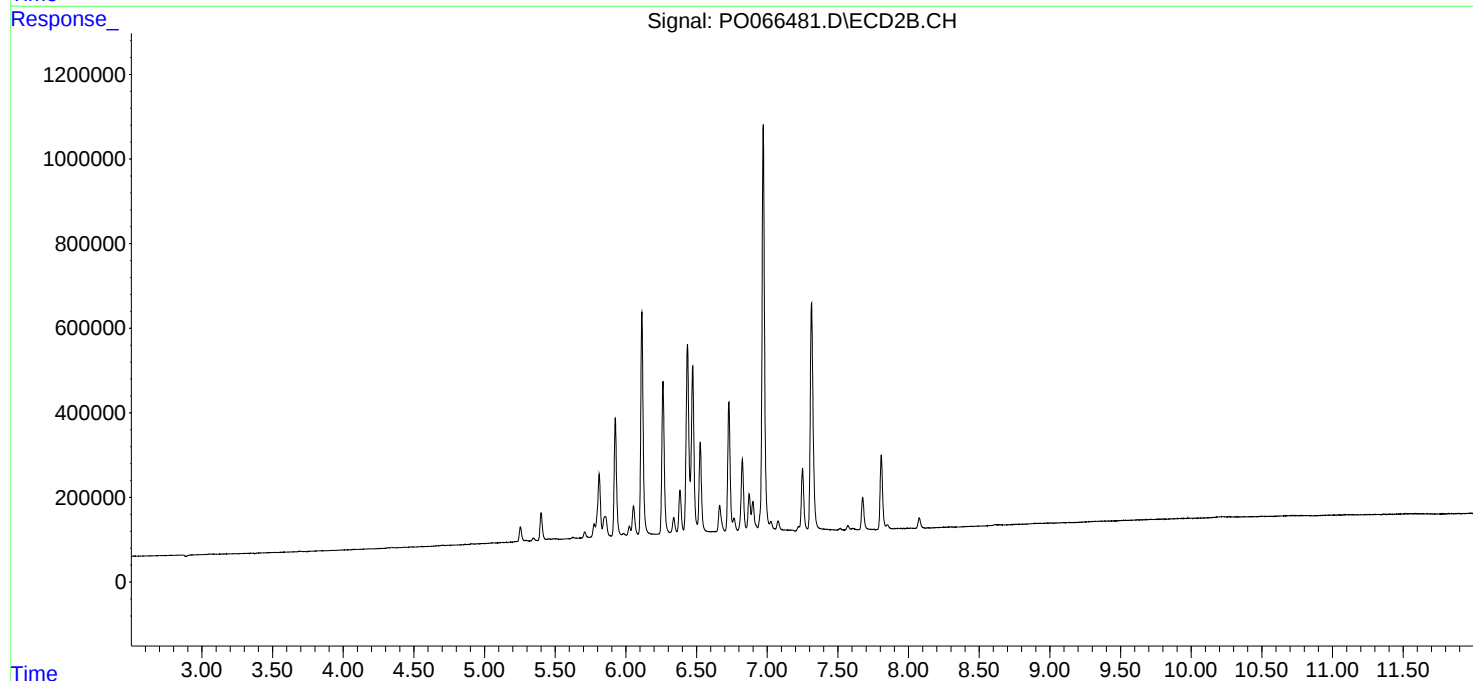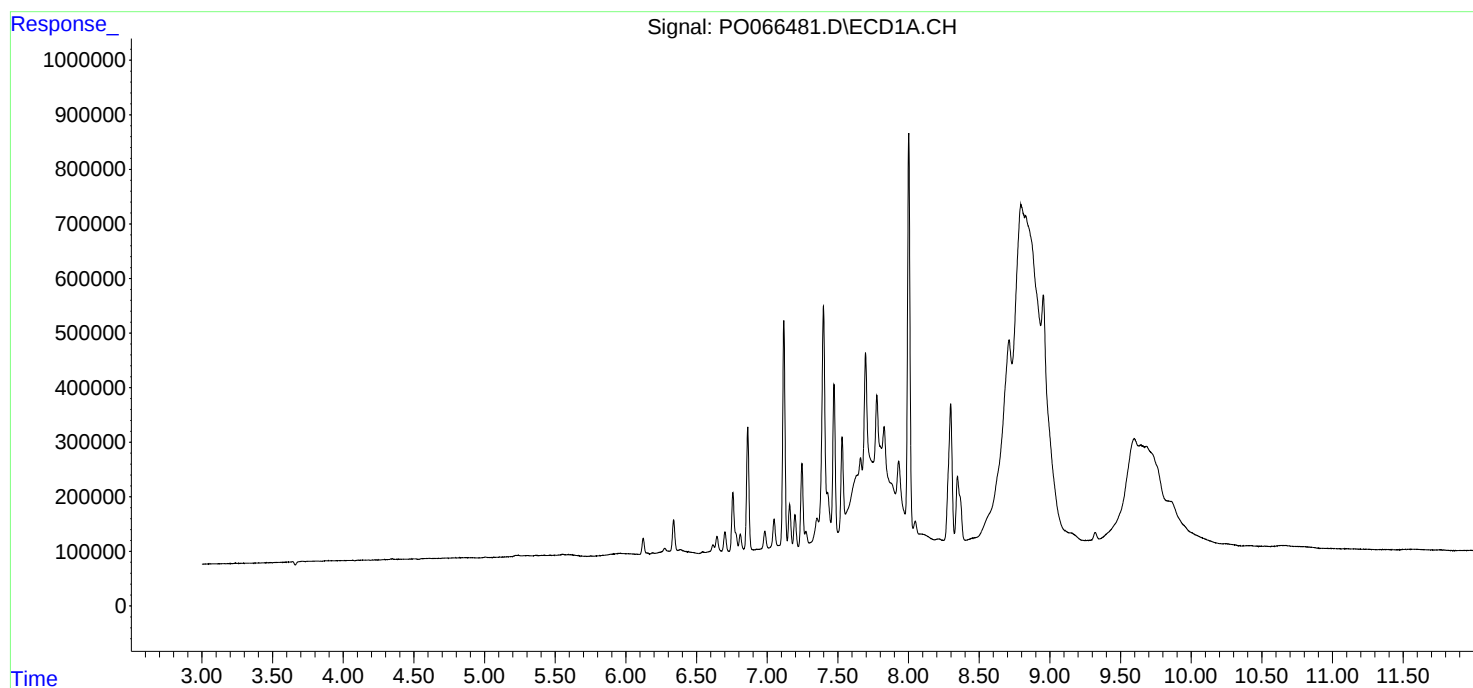


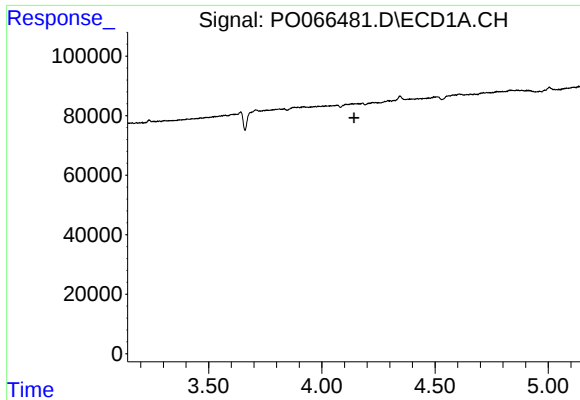

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PCB-021020-SR-02DL

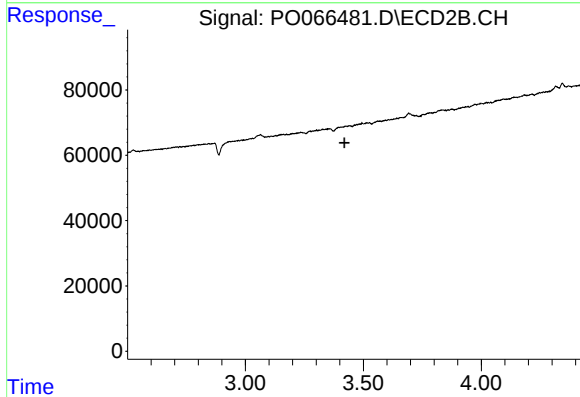


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.420 min
Response: 0
Conc: N.D.

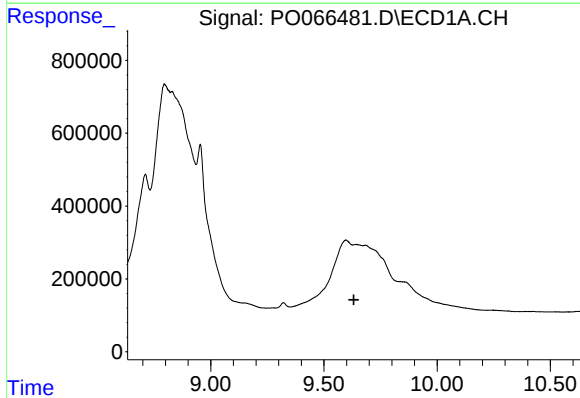

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.632 min
Response: 0
Conc: N.D.

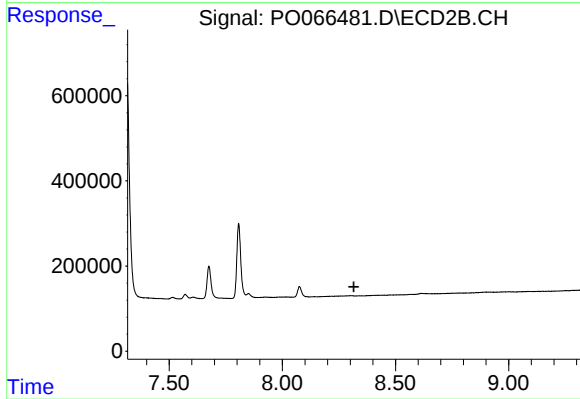

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.316 min
Response: 0
Conc: N.D.