

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021319\
 Data File : P0053858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Feb 2019 17:29
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 13 23:59:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 11 14:15:10 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.072	3.143	88724544	5997987	24.960	21.972
2)	SA Decachlor...	9.434	7.737	27369785	6192924	21.797	22.159

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021319\
Data File : P0053858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Feb 2019 17:29
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 23:59:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 11 14:15:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

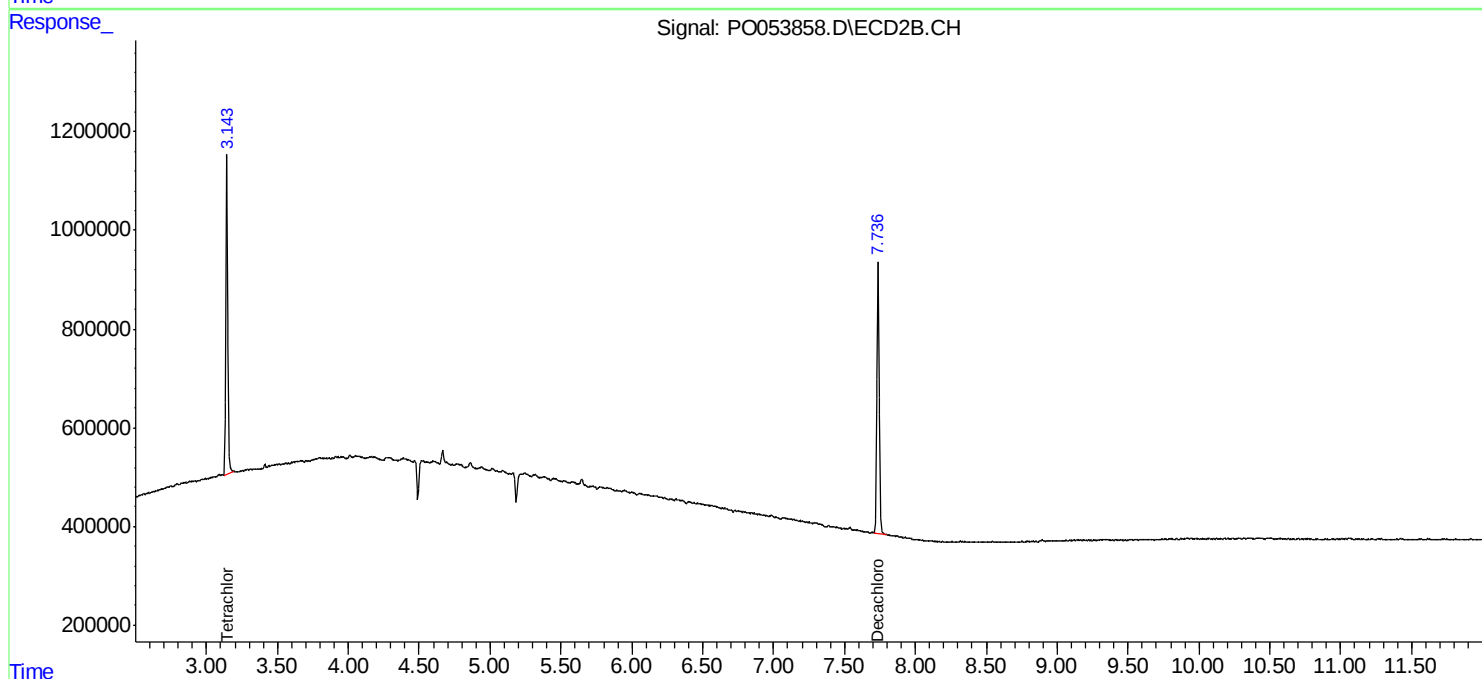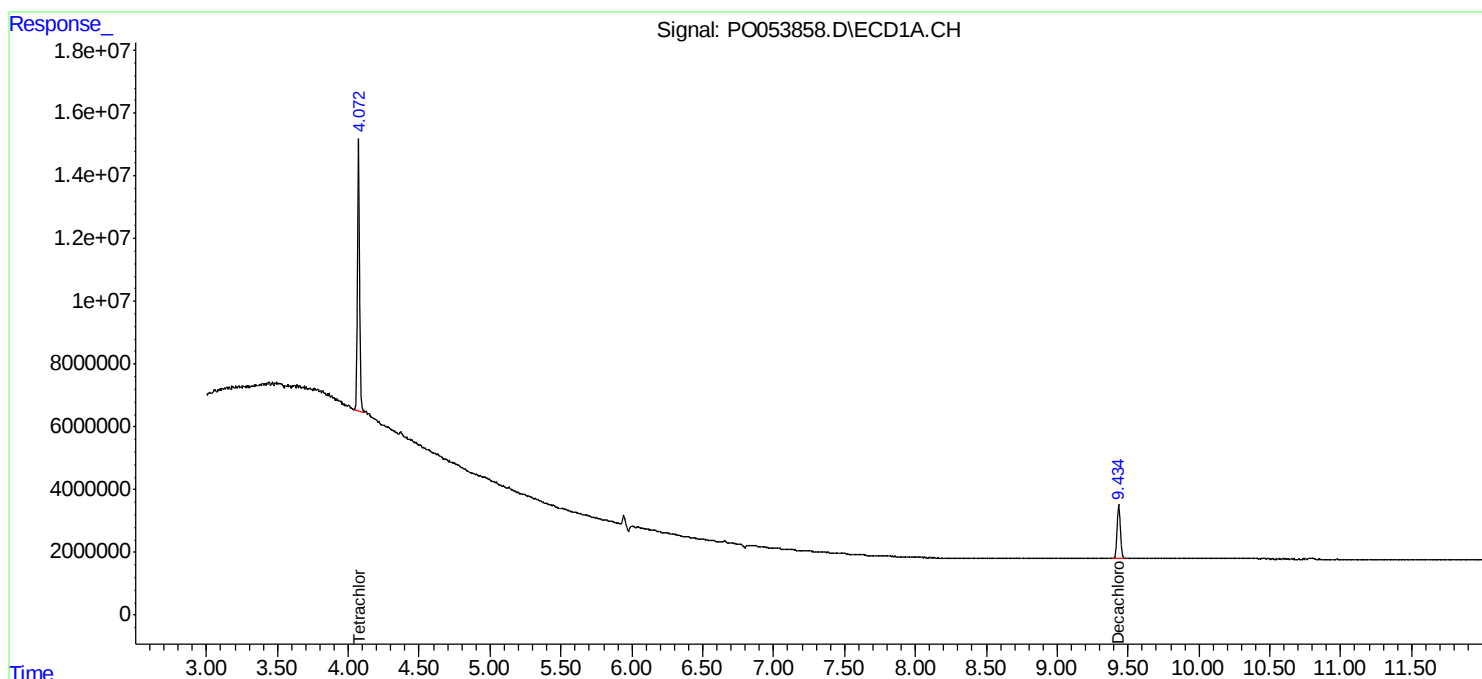


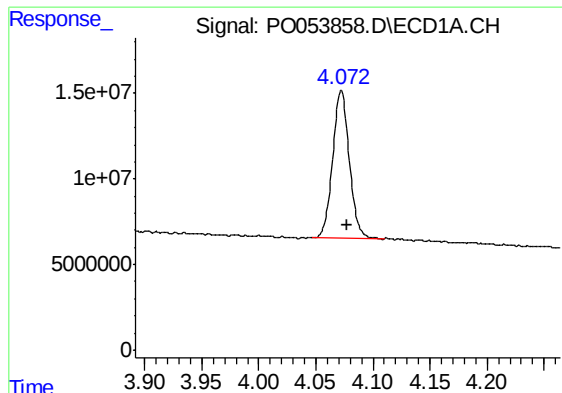

#1 Tetrachloro-m-xylene


R.T.: 4.072 min
Delta R.T.: -0.006 min
Response: 88724544
Conc: 24.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

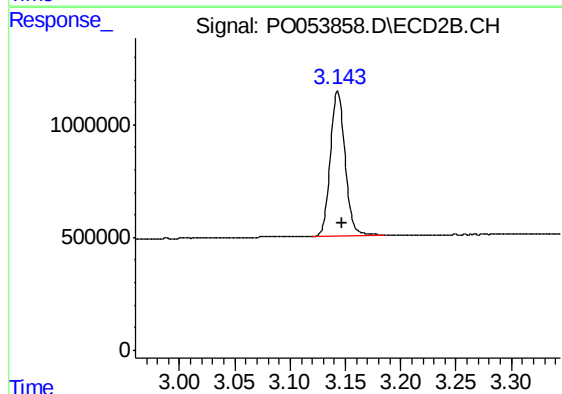


#1 Tetrachloro-m-xylene

R.T.: 3.143 min
Delta R.T.: -0.004 min
Response: 5997987
Conc: 21.97 ng/ml

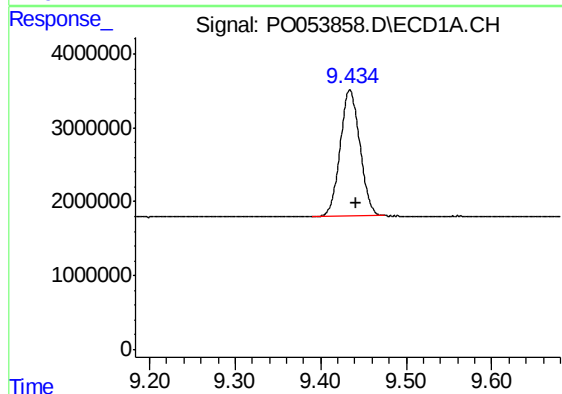

#2 Decachlorobiphenyl

R.T.: 9.434 min
Delta R.T.: -0.008 min
Response: 27369785
Conc: 21.80 ng/ml

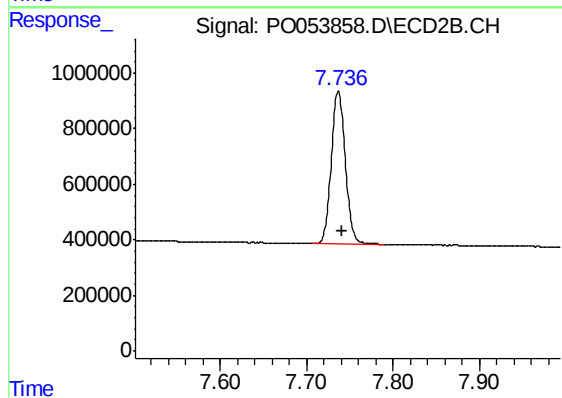

#2 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.005 min
Response: 6192924
Conc: 22.16 ng/ml