

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021319\
Data File : P0053869.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Feb 2019 20:35
Operator : SM/SJ
Sample : K1461-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 23:42:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 11 14:15:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.074	3.144	26664863	2160318	7.501m	7.914m
2) SA Decachlor...	9.436	7.738	5440678	1290351	4.333	4.617

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021319\
Data File : P0053869.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Feb 2019 20:35
Operator : SM/SJ
Sample : K1461-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 13 23:42:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021119.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 11 14:15:10 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

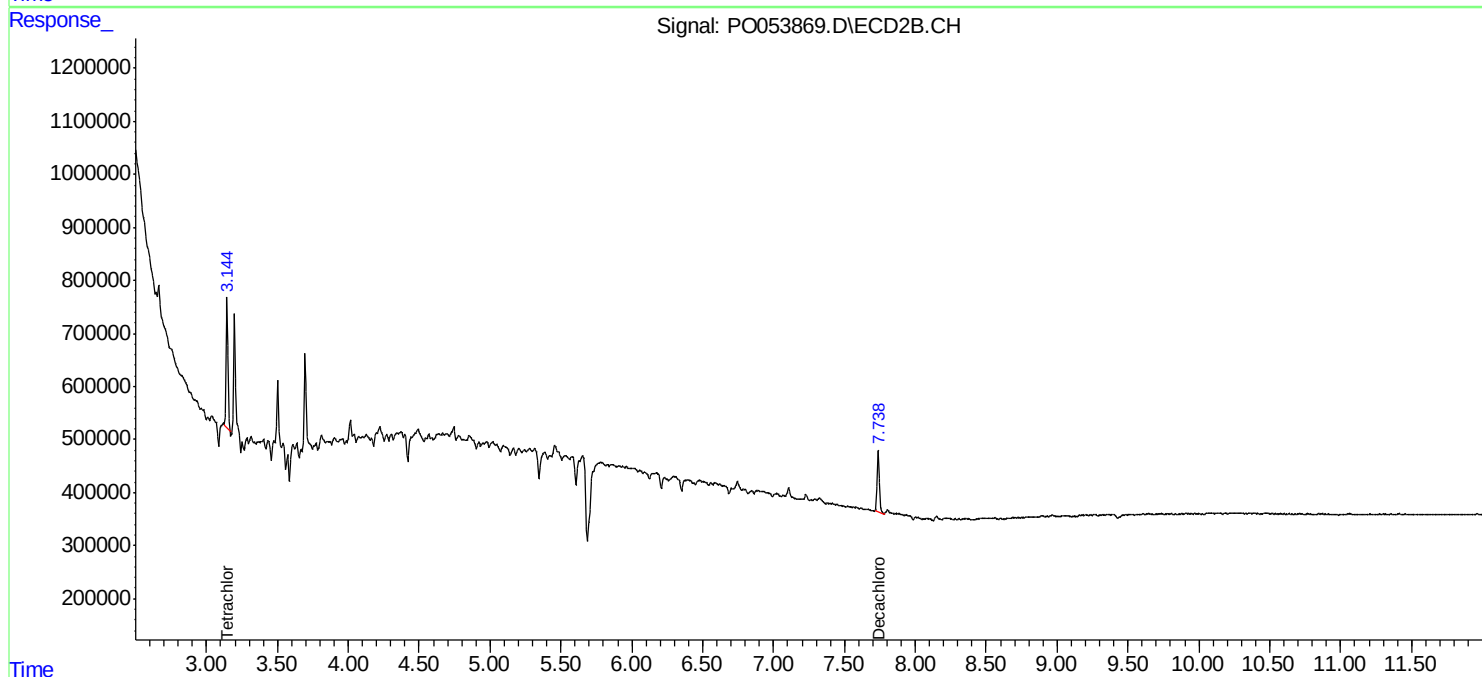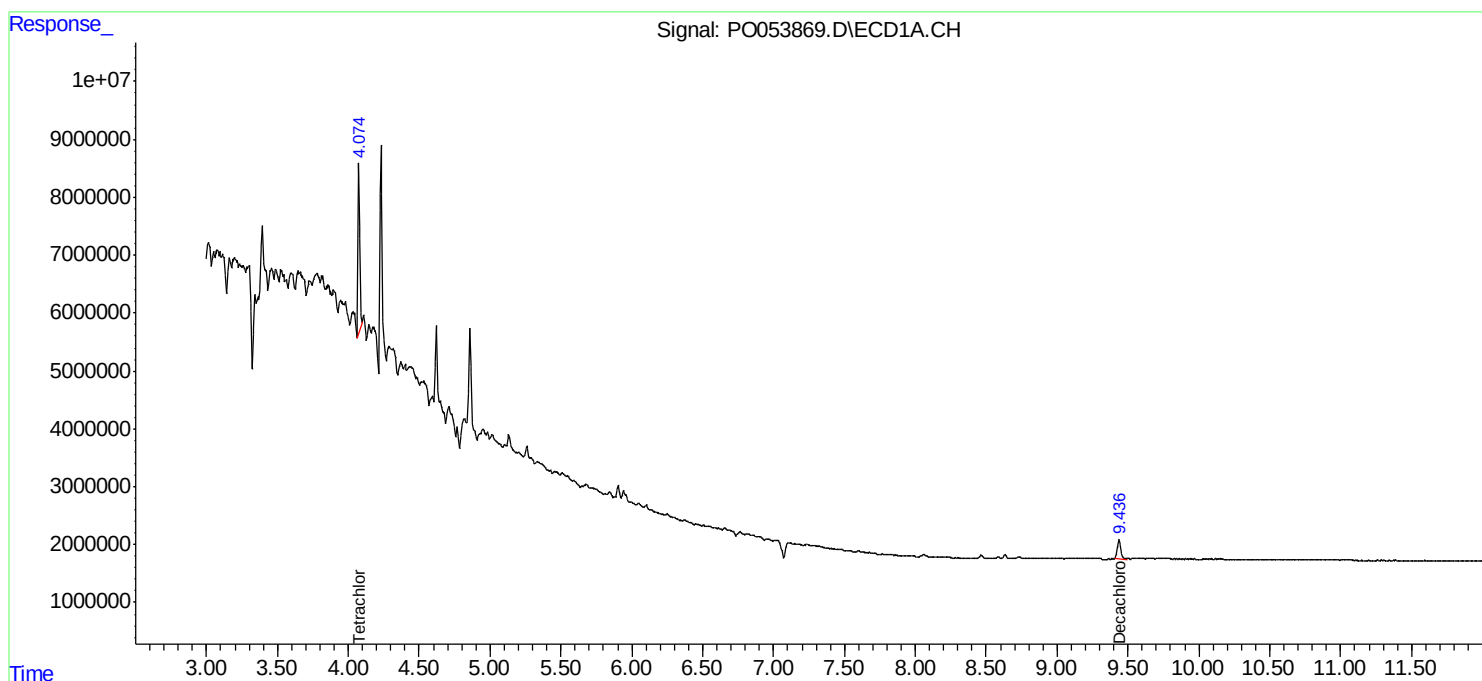


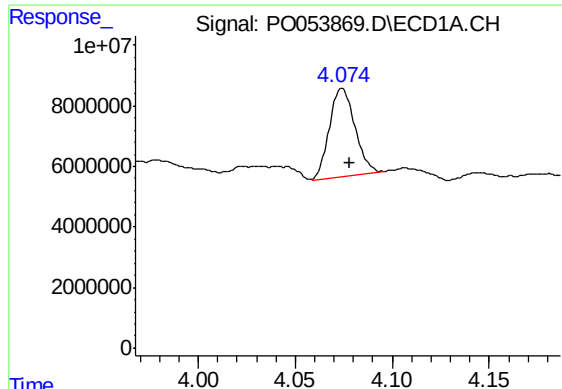

#1 Tetrachloro-m-xylene


R.T.: 4.074 min
Delta R.T.: -0.004 min
Response: 26664863
Conc: 7.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

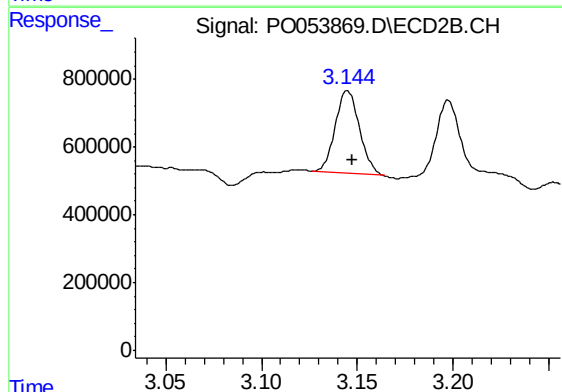


#1 Tetrachloro-m-xylene

R.T.: 3.144 min
Delta R.T.: -0.003 min
Response: 2160318
Conc: 7.91 ng/ml m

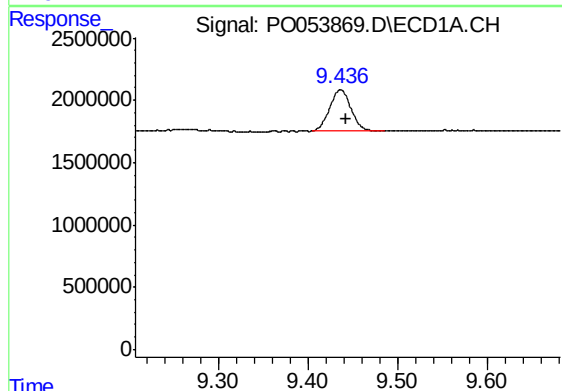

#2 Decachlorobiphenyl

R.T.: 9.436 min
Delta R.T.: -0.006 min
Response: 5440678
Conc: 4.33 ng/ml

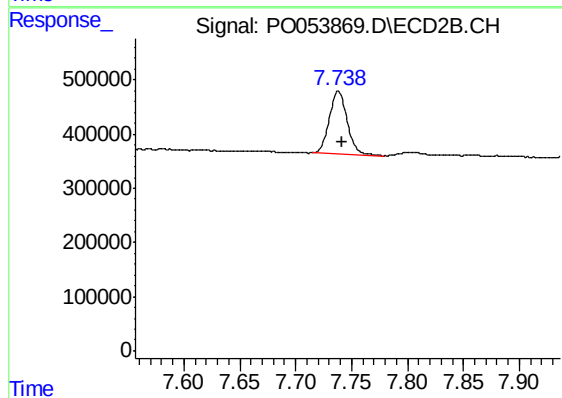

#2 Decachlorobiphenyl

R.T.: 7.738 min
Delta R.T.: -0.003 min
Response: 1290351
Conc: 4.62 ng/ml