

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
 Data File : P0066626.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2020 16:11
 Operator : DD\AJ
 Sample : L1558-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0109-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 06:49:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.129	3.410	684806	874273	20.010	21.702
2) SA Decachlor...	9.606	8.295	785786	1010283	17.135	16.799
Target Compounds						
16) L4 AR-1242-1	5.212	0.000	52107	0	50.644	N.D. #
21) L5 AR-1248-1	5.212	0.000	52107	0	64.563	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
Data File : P0066626.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2020 16:11
Operator : DD\AJ
Sample : L1558-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0109-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 06:49:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

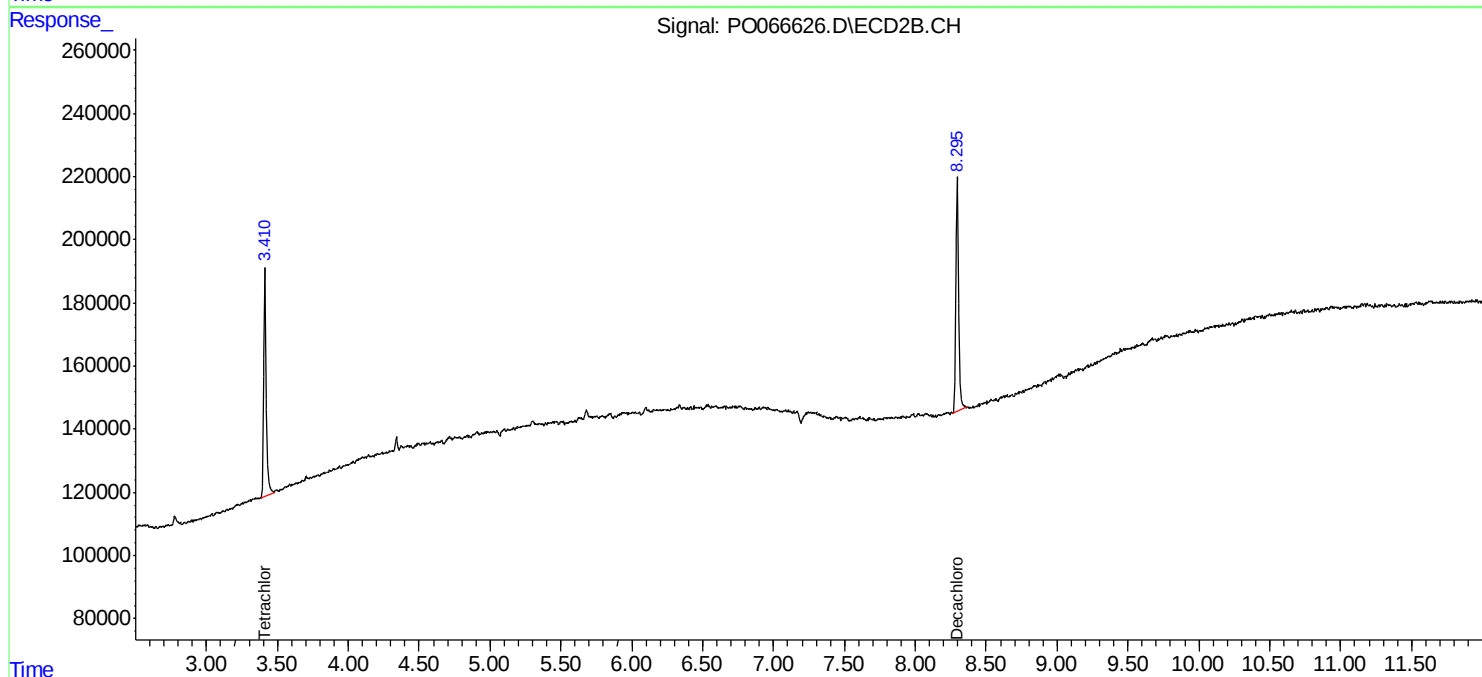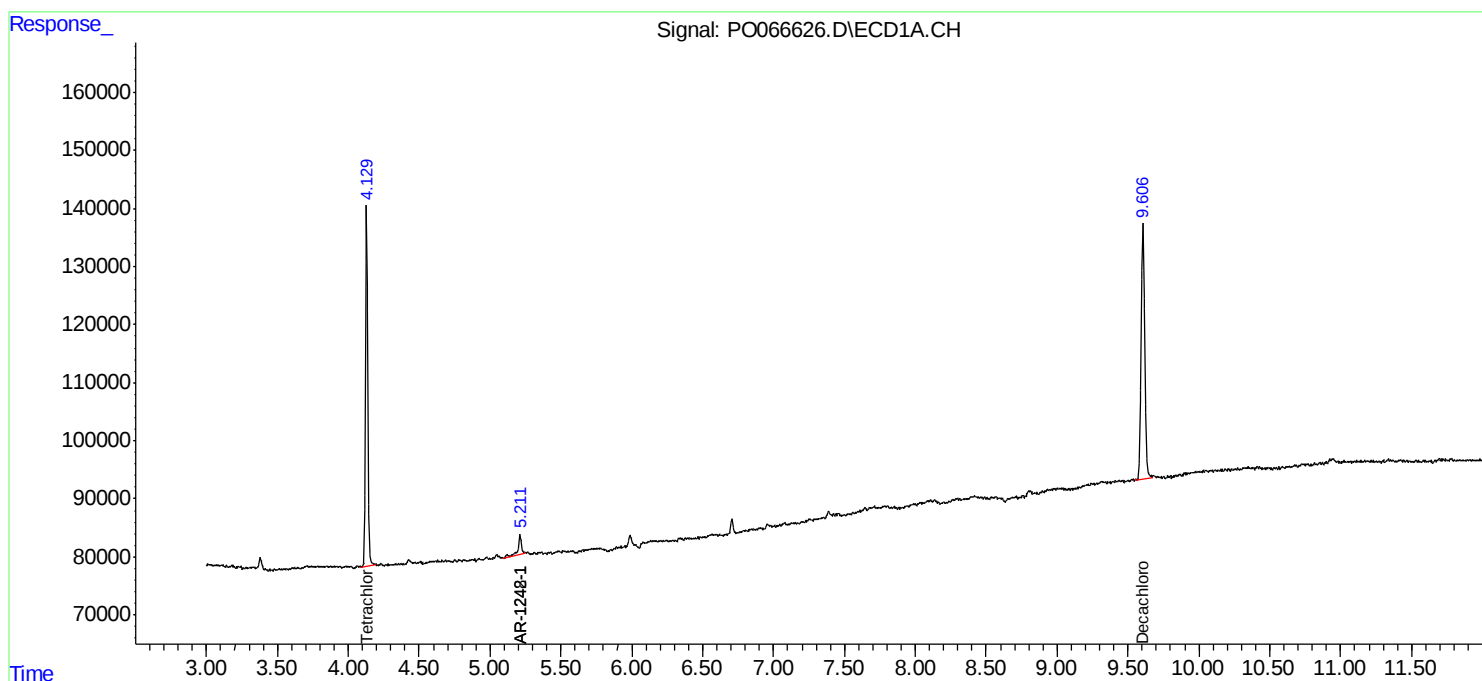


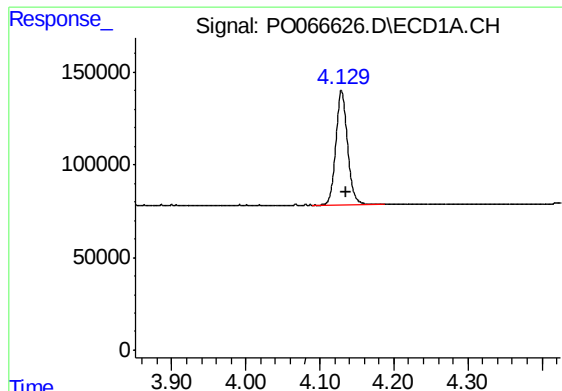

#1 Tetrachloro-m-xylene


R.T.: 4.129 min
Delta R.T.: -0.006 min
Response: 684806
Conc: 20.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
0109-SITE-WATER

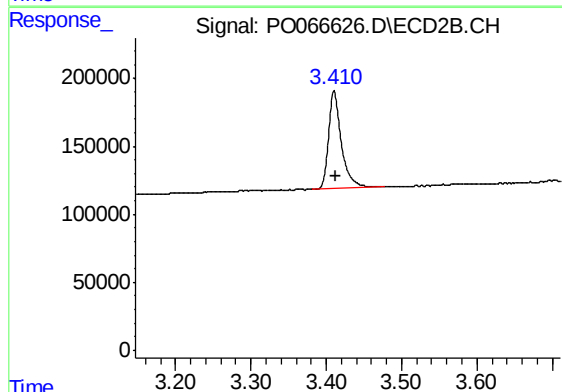


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: -0.002 min
Response: 874273
Conc: 21.70 ng/ml

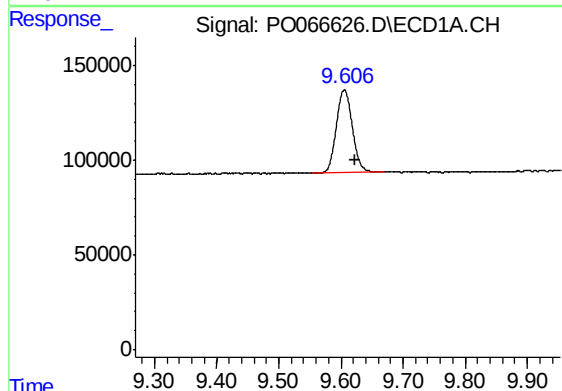


#2 Decachlorobiphenyl

R.T.: 9.606 min
Delta R.T.: -0.017 min
Response: 785786
Conc: 17.14 ng/ml

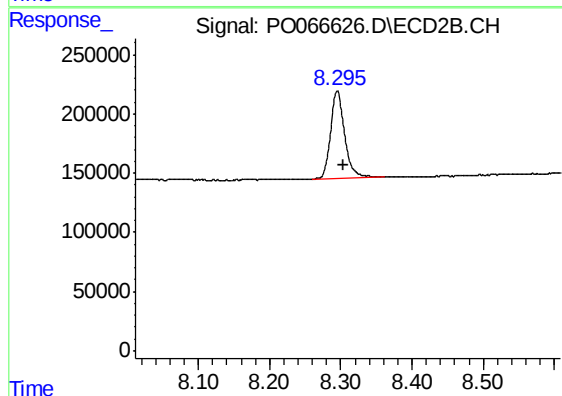

#2 Decachlorobiphenyl


R.T.: 8.295 min
Delta R.T.: -0.009 min
Response: 1010283
Conc: 16.80 ng/ml

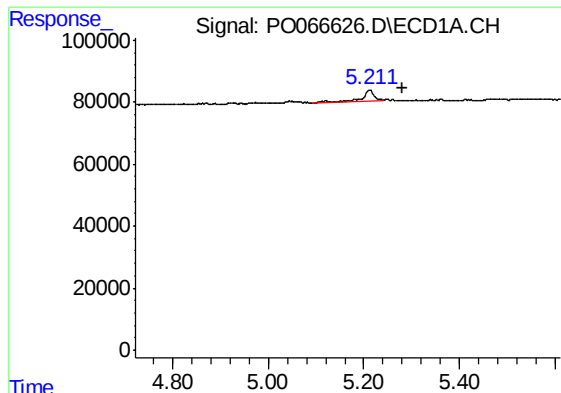

#16 AR-1242-1


R.T.: 5.212 min
Delta R.T.: -0.069 min
Response: 52107
Conc: 50.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
0109-SITE-WATER

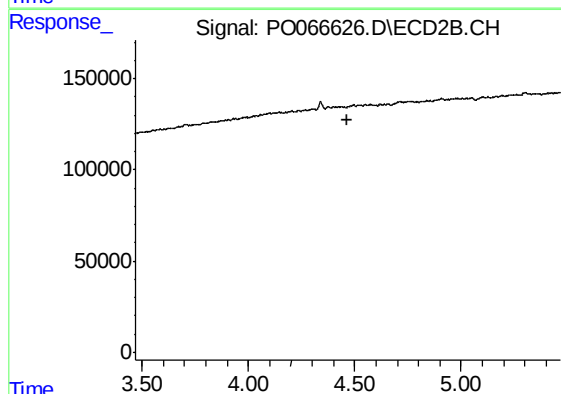


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.468 min
Response: 0
Conc: N.D.

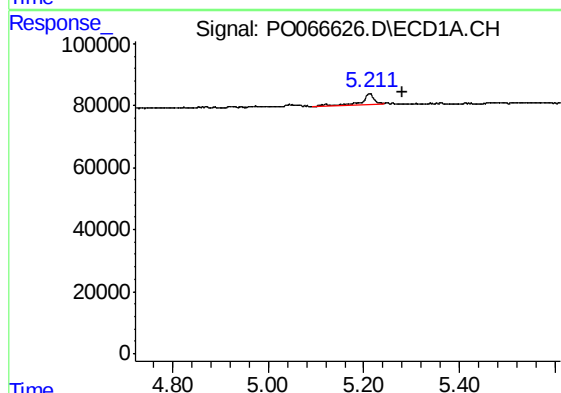

#21 AR-1248-1

R.T.: 5.212 min
Delta R.T.: -0.069 min
Response: 52107
Conc: 64.56 ng/ml

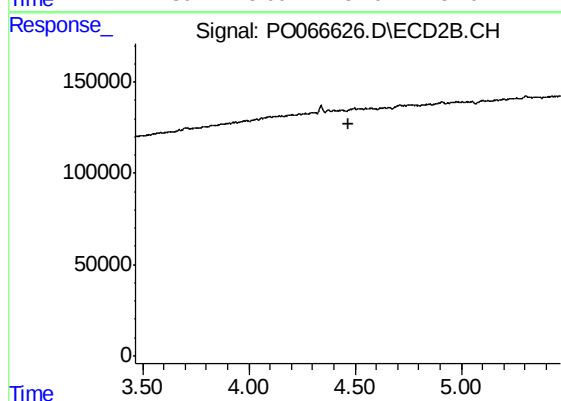

#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.467 min
Response: 0
Conc: N.D.