

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
 Data File : P0066612.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2020 10:15
 Operator : DD\AJ
 Sample : L1560-01RE 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-CRE

Manual Integrations
 APPROVED

Sohil
 2/19/2020 4:07:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 16:53:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.126	3.420	49407	290088	1.444m	7.201m#
2) SA Decachlor...	9.602	8.294	53213	78045	1.160m	1.298m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
Data File : P0066612.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2020 10:15
Operator : DD\AJ
Sample : L1560-01RE 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-CRE


Manual Integrations
APPROVED

Sohil
2/19/2020 4:07:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 16:53:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

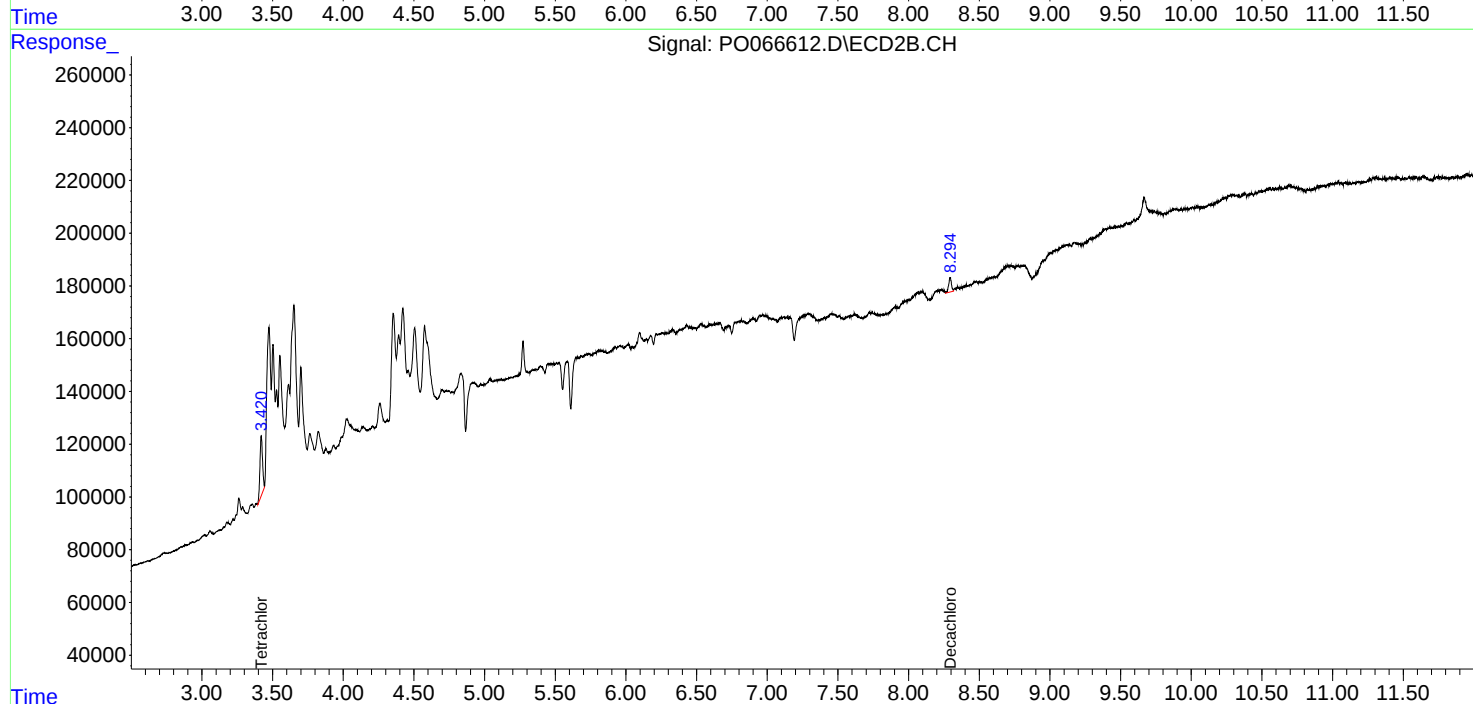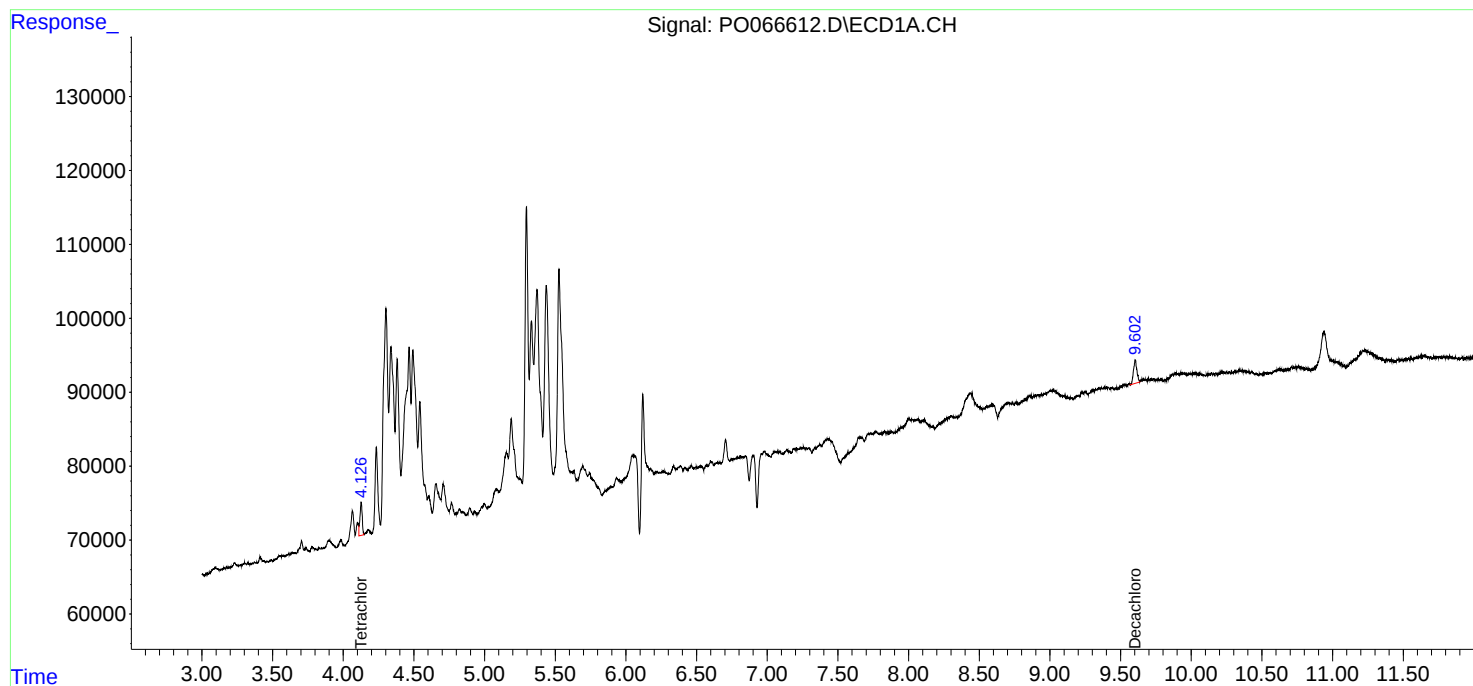

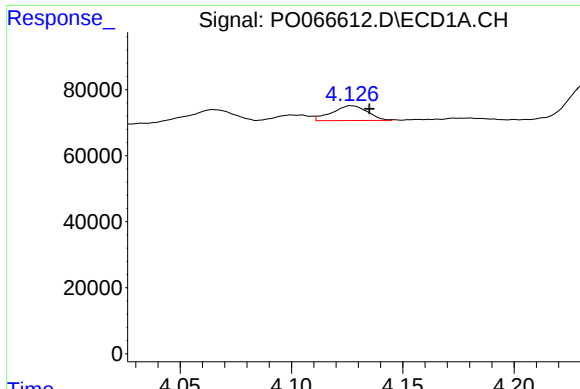


#1 Tetrachloro-m-xylene

R.T.: 4.126 min
Delta R.T.: -0.009 min
Response: 49407
Conc: 1.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-CRE


Manual Integrations
APPROVED

Sohil
2/19/2020 4:07:06 PM

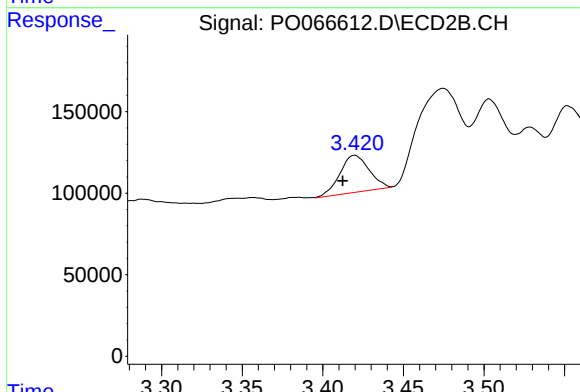


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.007 min
Response: 290088
Conc: 7.20 ng/ml m

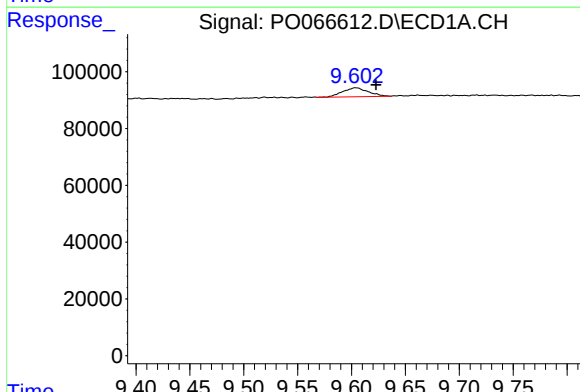

#2 Decachlorobiphenyl

R.T.: 9.602 min
Delta R.T.: -0.020 min
Response: 53213
Conc: 1.16 ng/ml m

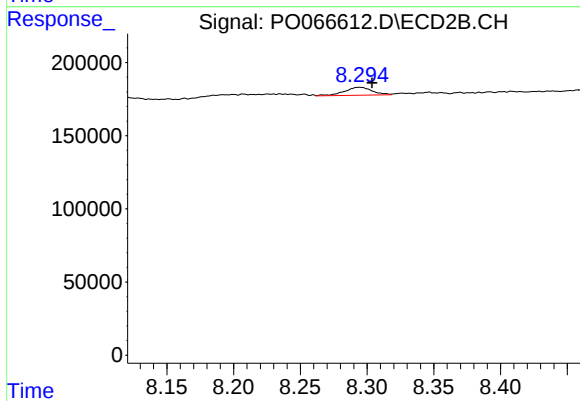

#2 Decachlorobiphenyl

R.T.: 8.294 min
Delta R.T.: -0.010 min
Response: 78045
Conc: 1.30 ng/ml m