

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
 Data File : P0066618.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Feb 2020 13:52
 Operator : DD\AJ
 Sample : L1558-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0166-COMP-BT-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 18 15:58:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.128	3.408	802503	1067398	23.450	26.496
2)	SA Decachlor...	9.603	8.293	830196	1098228	18.104	18.262

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021820\
Data File : P0066618.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Feb 2020 13:52
Operator : DD\AJ
Sample : L1558-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0166-COMP-BT-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 18 15:58:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

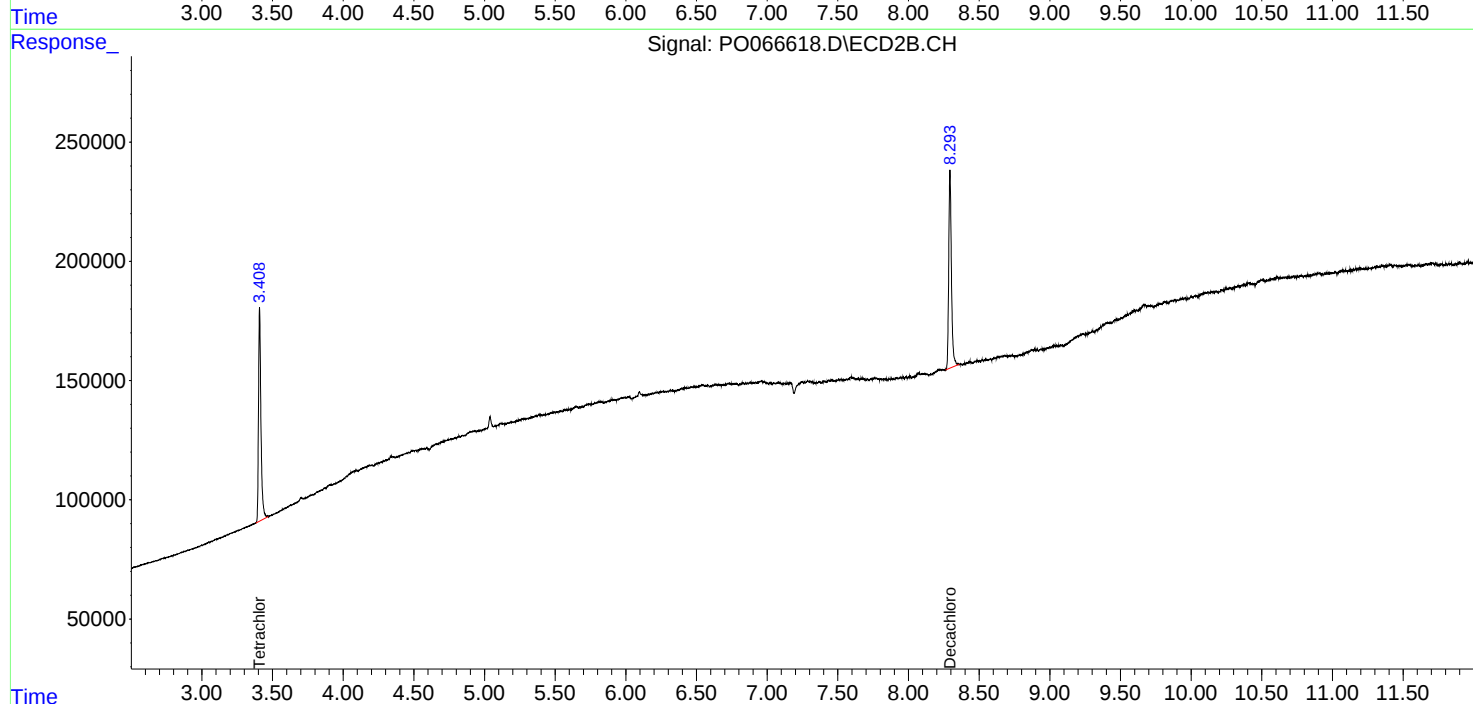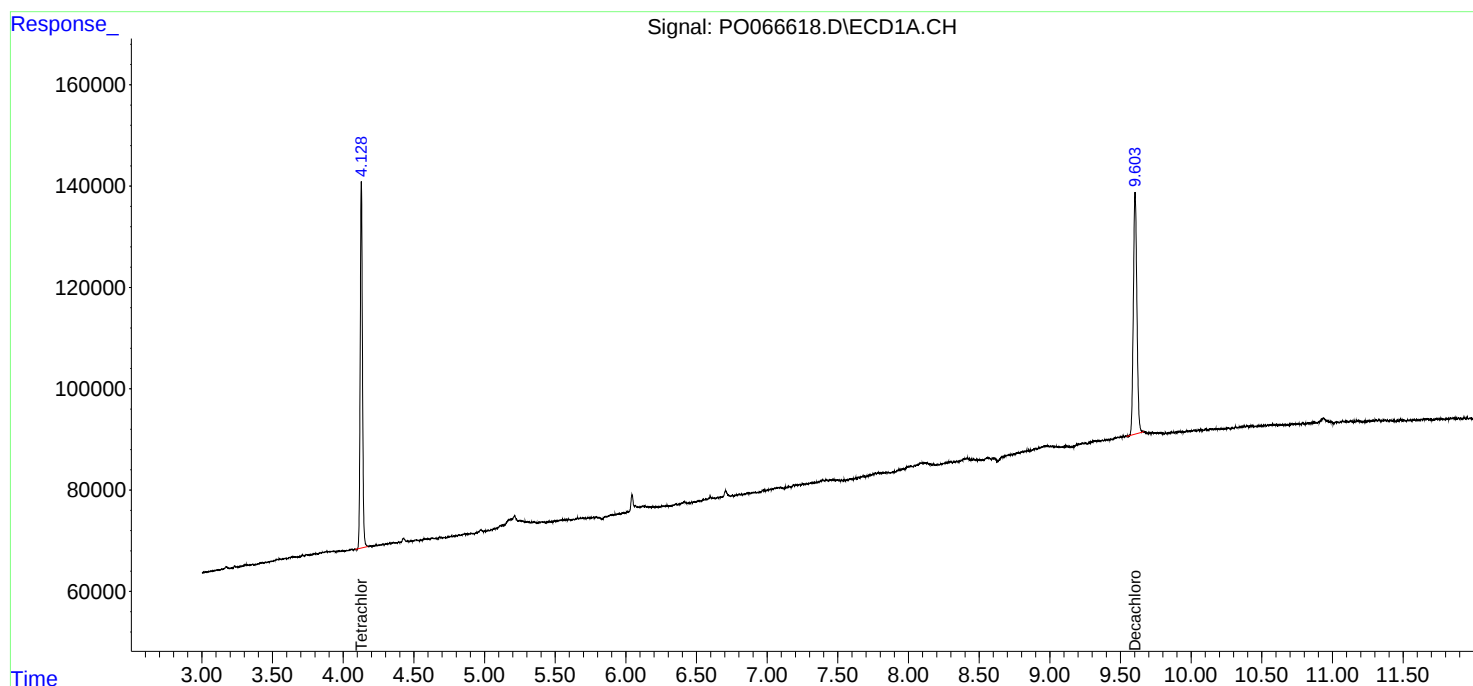


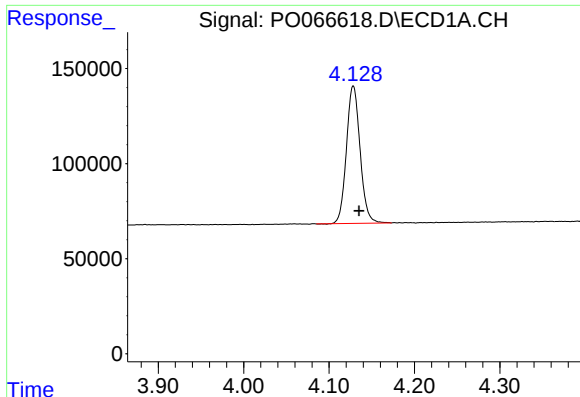

#1 Tetrachloro-m-xylene


R.T.: 4.128 min
Delta R.T.: -0.007 min
Response: 802503
Conc: 23.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
0166-COMP-BT-A

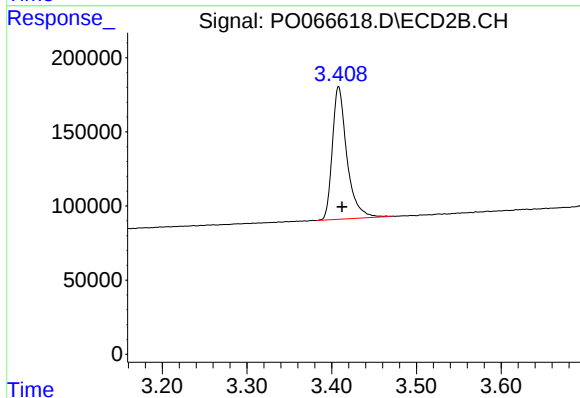


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: -0.004 min
Response: 1067398
Conc: 26.50 ng/ml

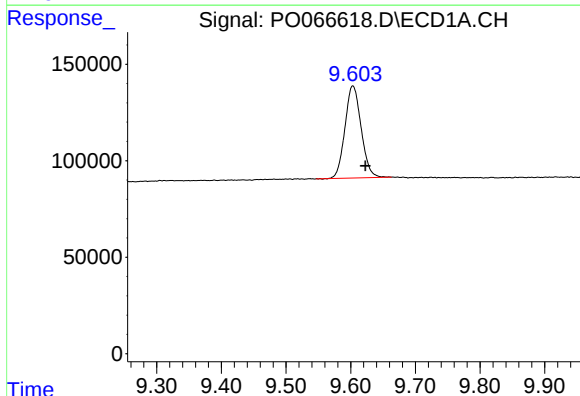

#2 Decachlorobiphenyl

R.T.: 9.603 min
Delta R.T.: -0.020 min
Response: 830196
Conc: 18.10 ng/ml

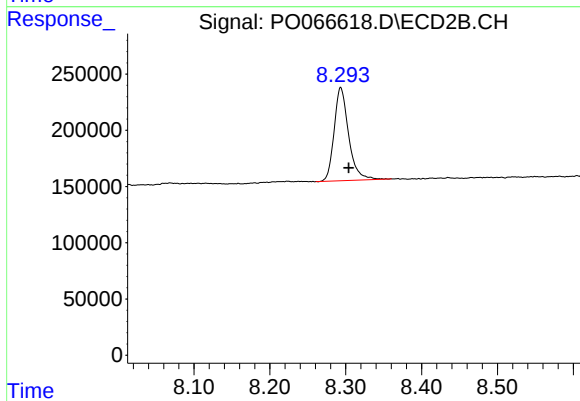

#2 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: -0.010 min
Response: 1098228
Conc: 18.26 ng/ml