

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021919\
 Data File : P0053949.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Feb 2019 17:20
 Operator : SM/SJ
 Sample : PB117215BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB117215BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 23:42:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.062	3.139	59733723	5656842	19.918	21.200
2) SA Decachlor...	9.410	7.722	26630386	6750567	21.207	22.528

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021919\
Data File : P0053949.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Feb 2019 17:20
Operator : SM/SJ
Sample : PB117215BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB117215BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 23:42:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

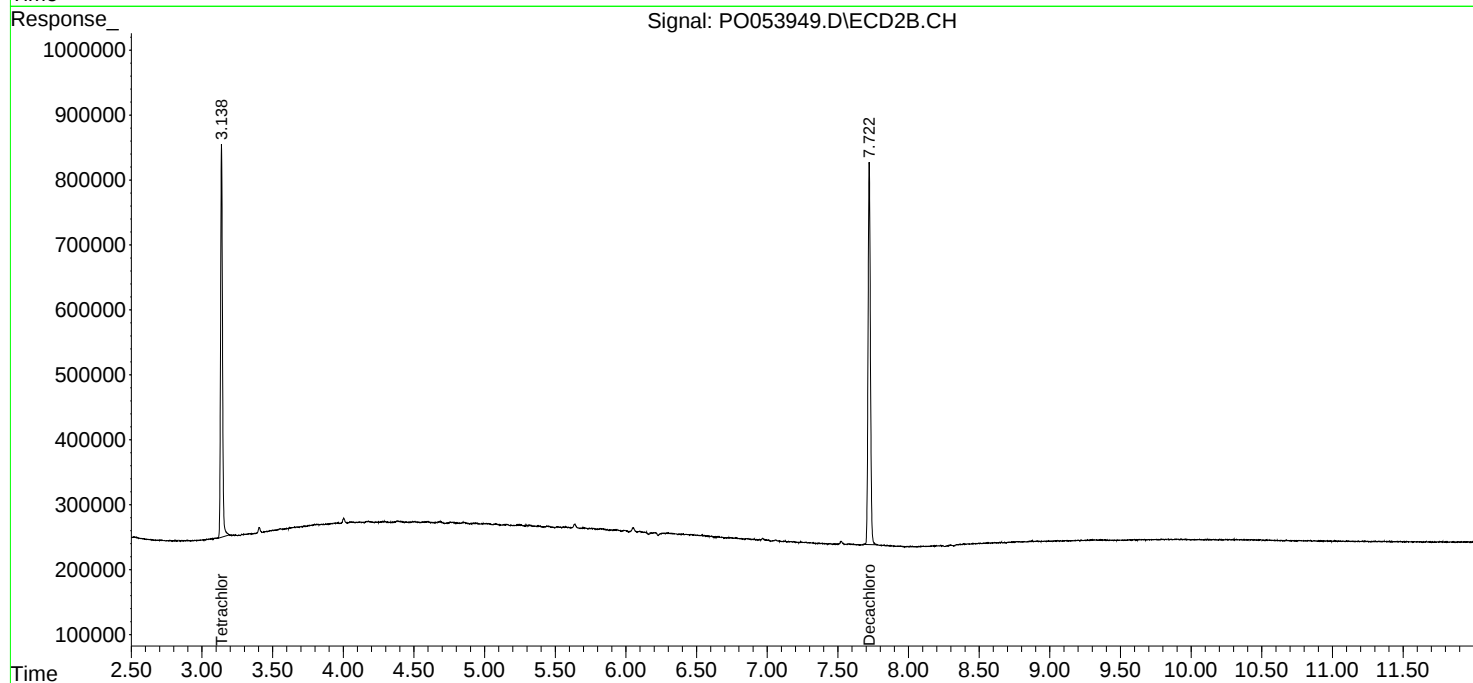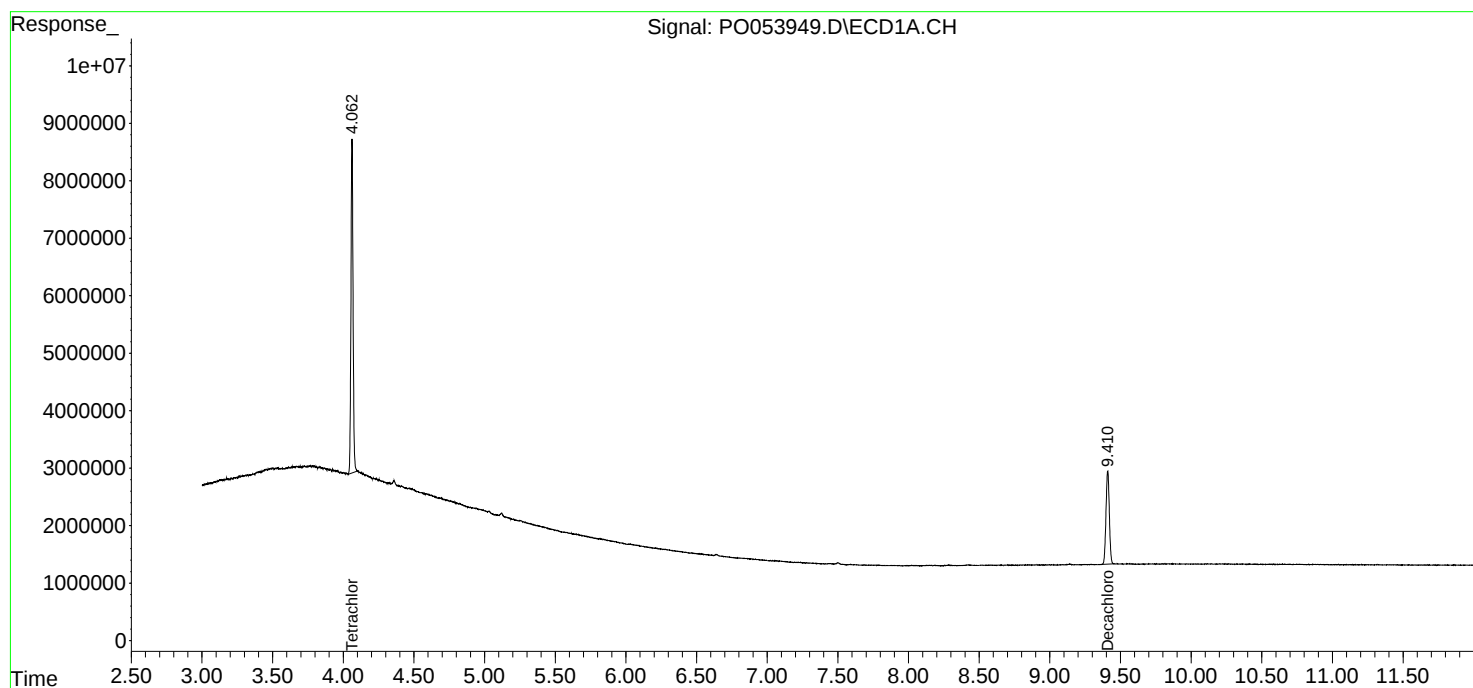


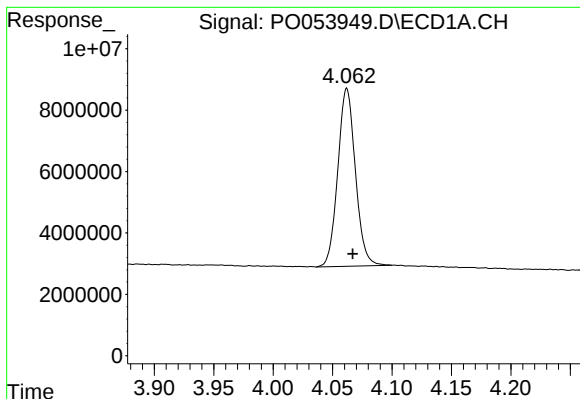

#1 Tetrachloro-m-xylene


R.T.: 4.062 min
Delta R.T.: -0.005 min
Response: 59733723
Conc: 19.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB117215BL

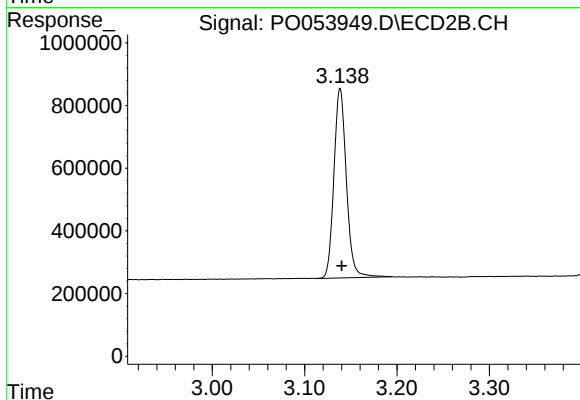


#1 Tetrachloro-m-xylene

R.T.: 3.139 min
Delta R.T.: -0.002 min
Response: 5656842
Conc: 21.20 ng/ml

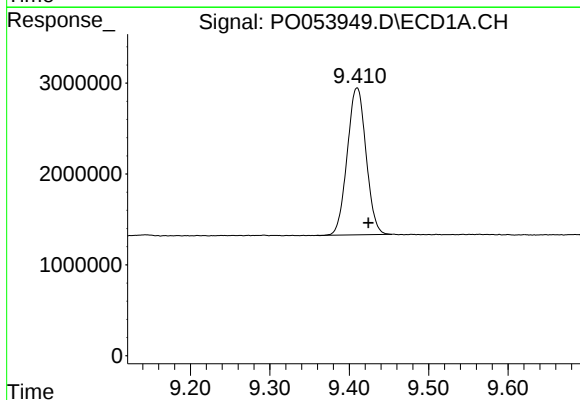

#2 Decachlorobiphenyl

R.T.: 9.410 min
Delta R.T.: -0.014 min
Response: 26630386
Conc: 21.21 ng/ml

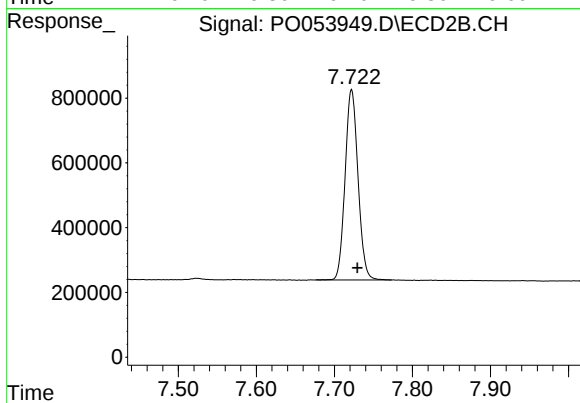

#2 Decachlorobiphenyl

R.T.: 7.722 min
Delta R.T.: -0.007 min
Response: 6750567
Conc: 22.53 ng/ml