

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021920\
 Data File : P0066648.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Feb 2020 9:23
 Operator : DD\AJ
 Sample : L1565-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13-A-13-B-13-C

Manual Integrations
 APPROVED

Sohil
 2/24/2020 10:25:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 16:01:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.127	3.407	818780	920980	23.925	22.862m
2) SA Decachlor...	9.603	8.293	936011	1226900	20.411	20.401

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0021920\
Data File : P0066648.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Feb 2020 9:23
Operator : DD\AJ
Sample : L1565-02
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
13-A-13-B-13-C


Manual Integrations
APPROVED

Sohil
2/24/2020 10:25:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 16:01:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

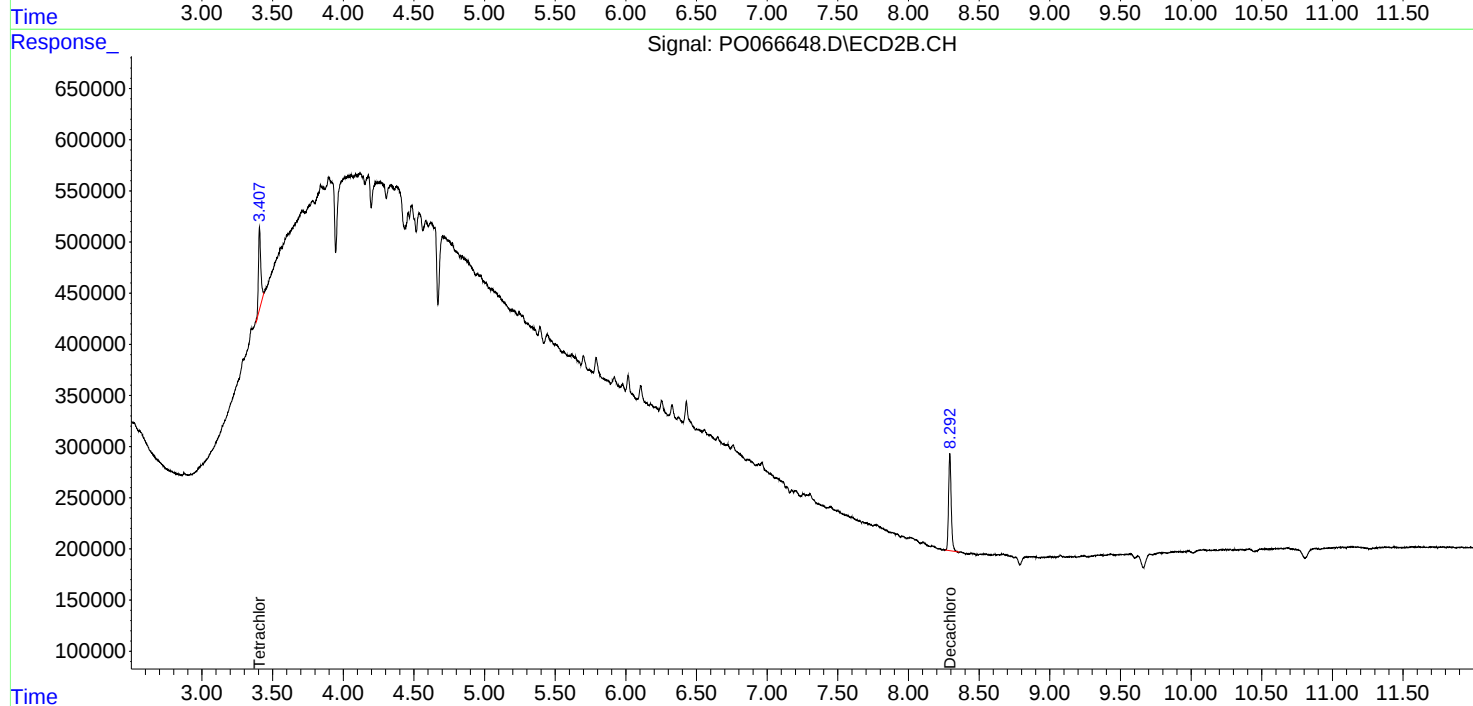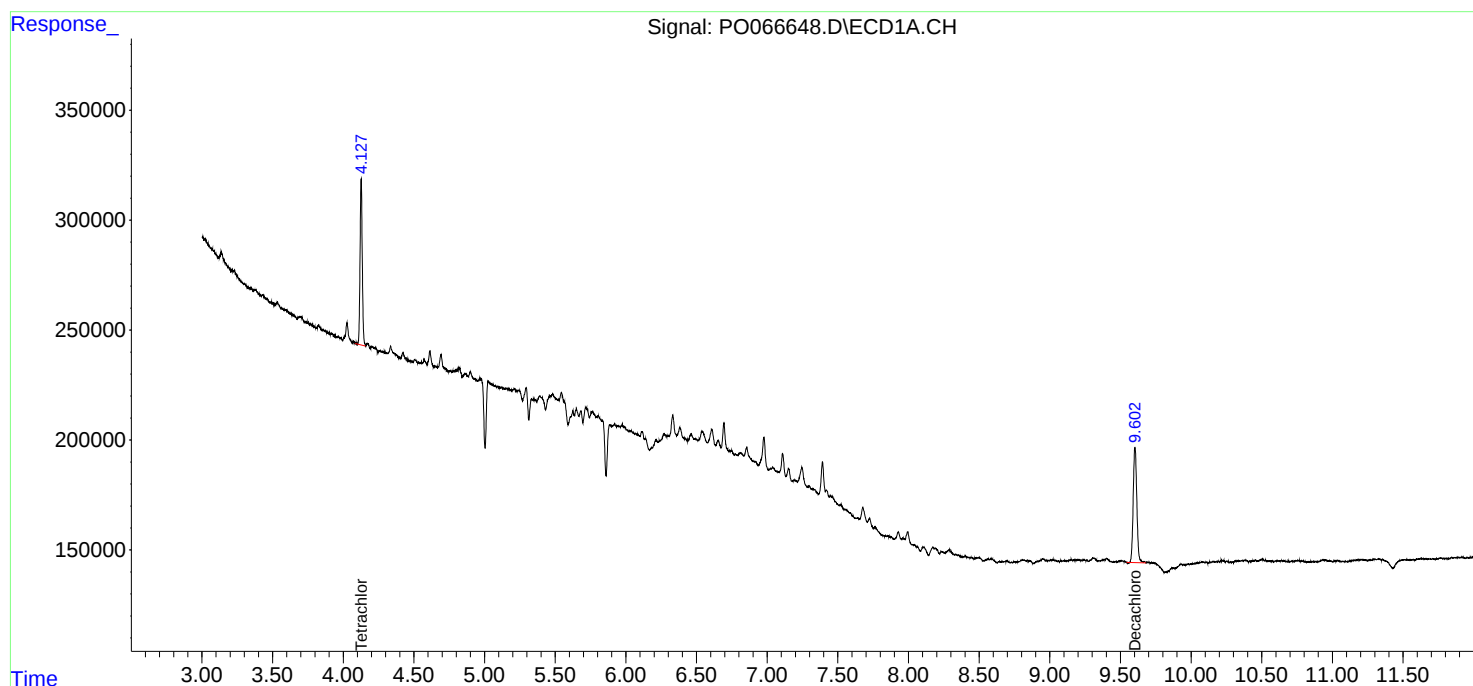

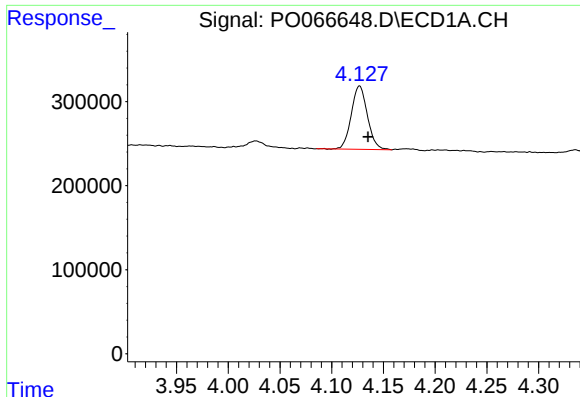


#1 Tetrachloro-m-xylene

R.T.: 4.127 min
Delta R.T.: -0.008 min
Response: 818780
Conc: 23.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
13-A-13-B-13-C


Manual Integrations
APPROVED

Sohil
2/24/2020 10:25:15 AM

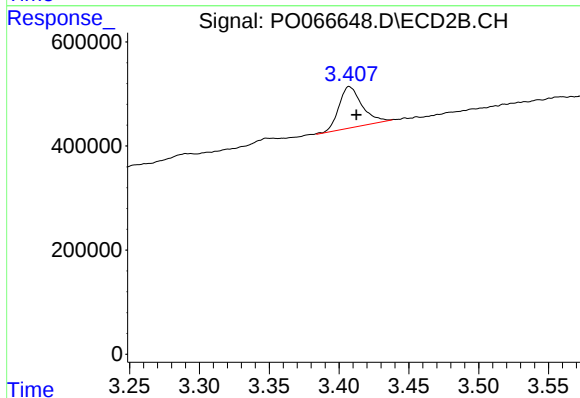


#1 Tetrachloro-m-xylene

R.T.: 3.407 min
Delta R.T.: -0.006 min
Response: 920980
Conc: 22.86 ng/ml m

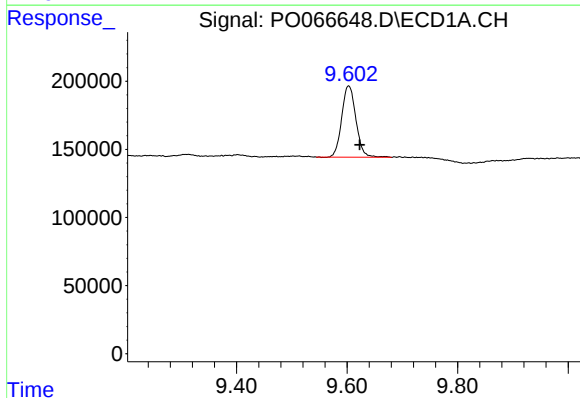

#2 Decachlorobiphenyl

R.T.: 9.603 min
Delta R.T.: -0.020 min
Response: 936011
Conc: 20.41 ng/ml

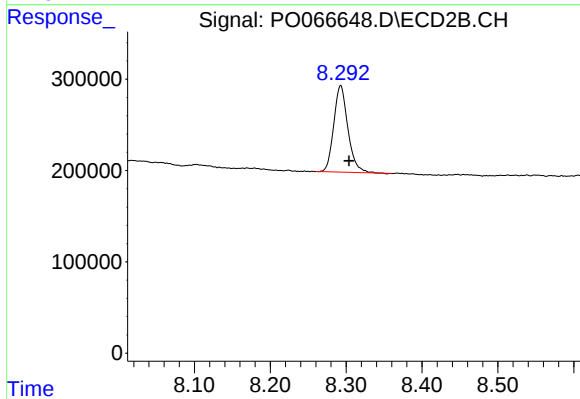

#2 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: -0.011 min
Response: 1226900
Conc: 20.40 ng/ml