

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022020\
 Data File : P0066666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Feb 2020 10:26
 Operator : DD\AJ
 Sample : L1567-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-18-E

Manual Integrations
 APPROVED

Sohil
 2/24/2020 10:27:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 16:10:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.406	841823	998689	24.599m	24.791
2) SA Decachlor...	9.595	8.287	2500564	2852574	54.528m	47.433m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022020\
Data File : P0066666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Feb 2020 10:26
Operator : DD\AJ
Sample : L1567-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
02-18-E


Manual Integrations
APPROVED

Sohil
2/24/2020 10:27:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 16:10:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

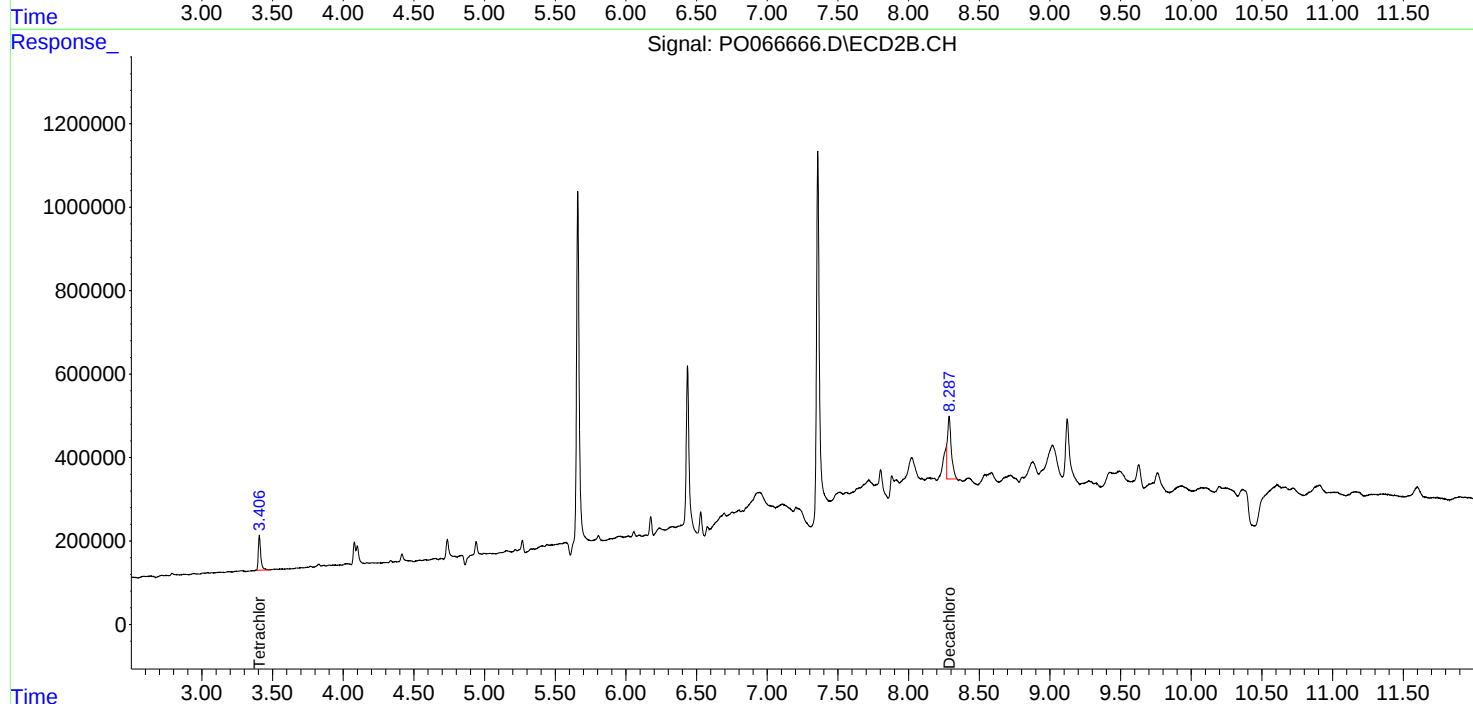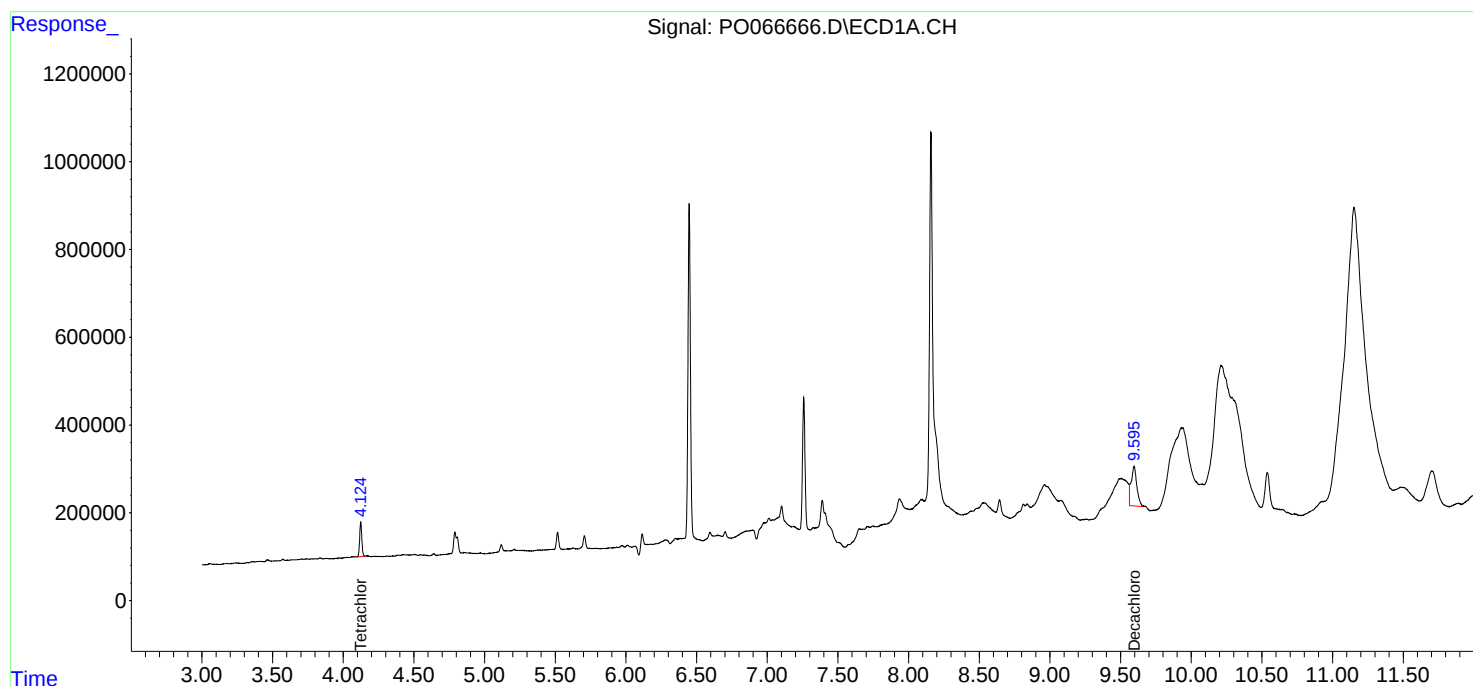

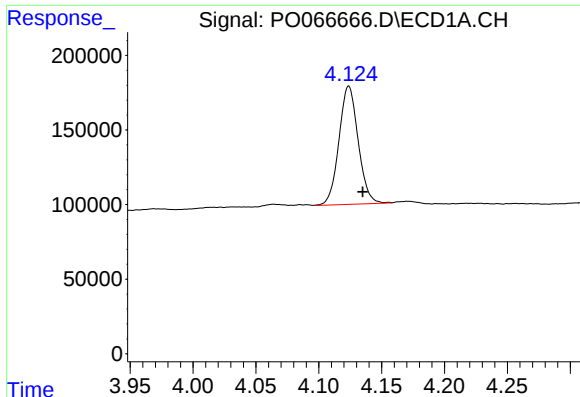


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.011 min
Response: 841823
Conc: 24.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-18-E


Manual Integrations
APPROVED

Sohil
2/24/2020 10:27:50 AM

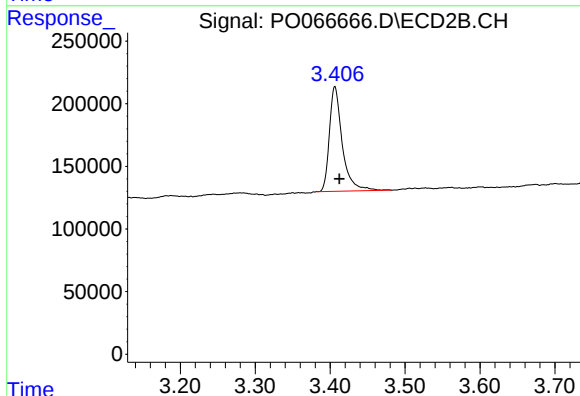


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: -0.006 min
Response: 998689
Conc: 24.79 ng/ml

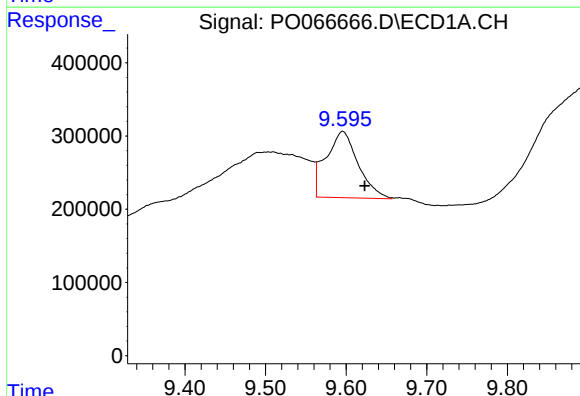

#2 Decachlorobiphenyl

R.T.: 9.595 min
Delta R.T.: -0.028 min
Response: 2500564
Conc: 54.53 ng/ml m

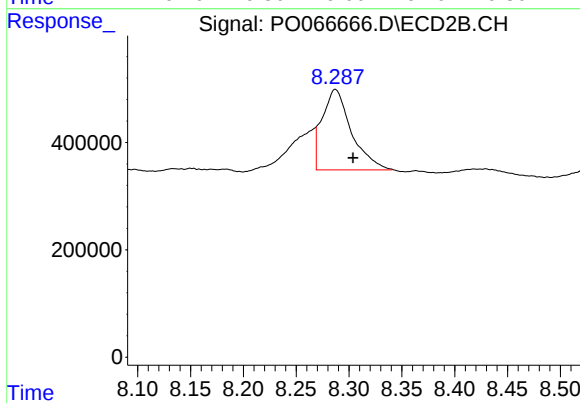

#2 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: -0.017 min
Response: 2852574
Conc: 47.43 ng/ml m