

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022020\
 Data File : P0066700.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Feb 2020 22:50
 Operator : DD\AJ
 Sample : L1583-01 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40708

Manual Integrations
 APPROVED

Sohil
 2/24/2020 10:28:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:52:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Feb 13 16:40:54 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.122	3.405	88706	69450	2.592	1.724m#
2) SA Decachlor...	9.598	8.288	70564	87662	1.539m	1.458

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022020\
Data File : P0066700.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Feb 2020 22:50
Operator : DD\AJ
Sample : L1583-01 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40708


Manual Integrations
APPROVED

Sohil
2/24/2020 10:28:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:52:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Feb 13 16:40:54 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

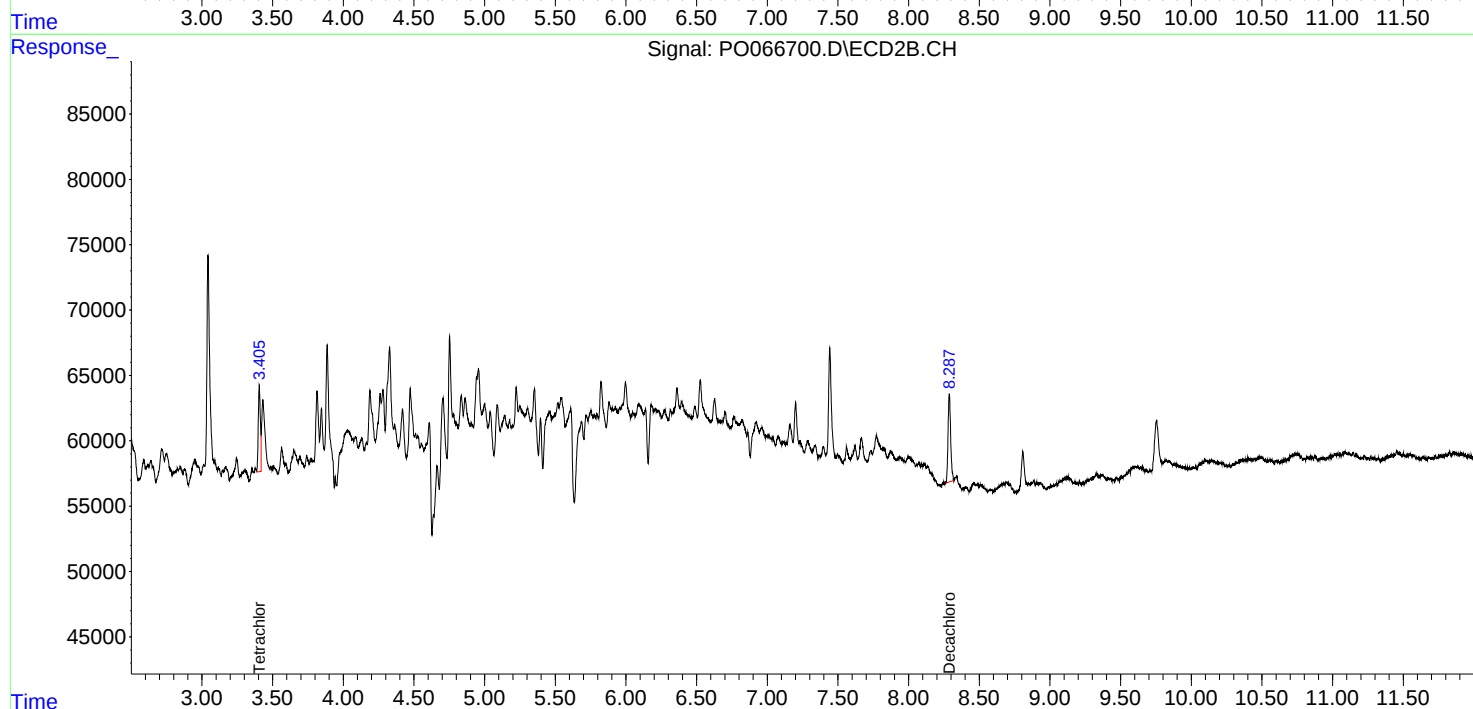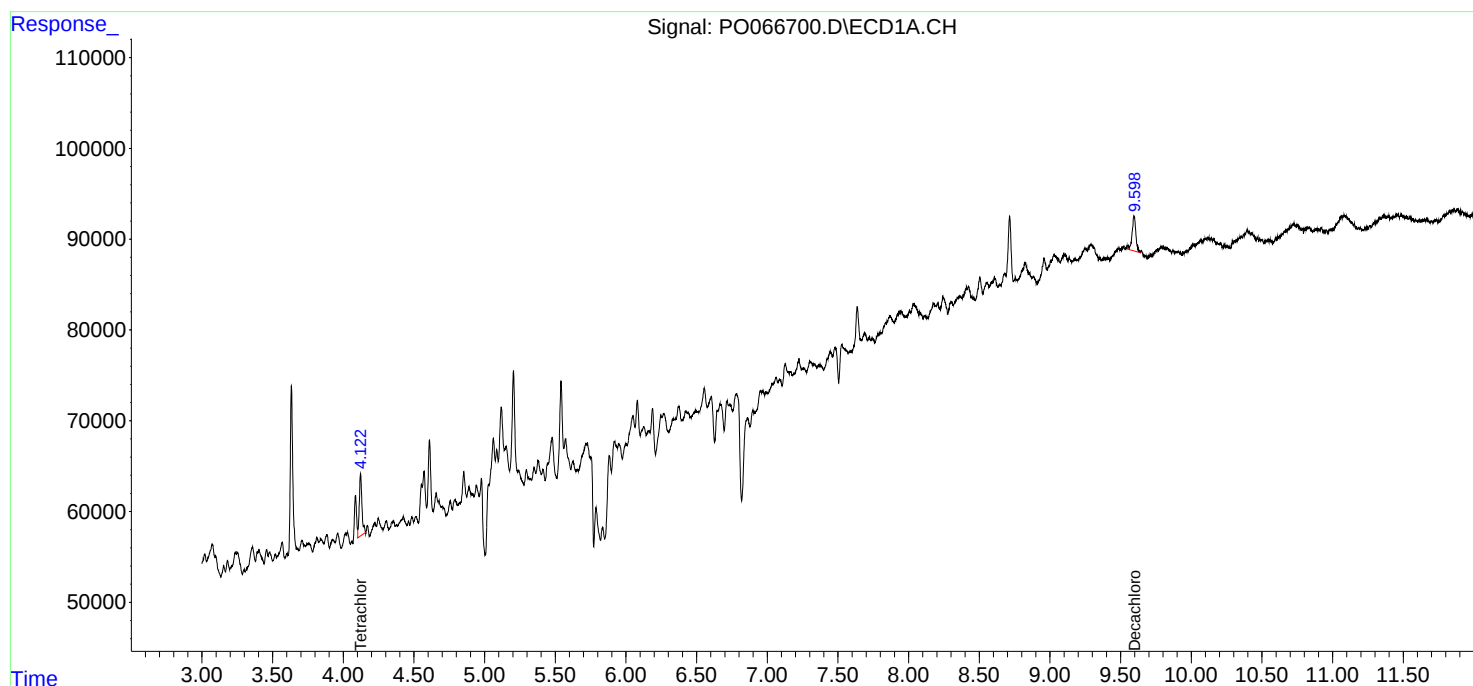

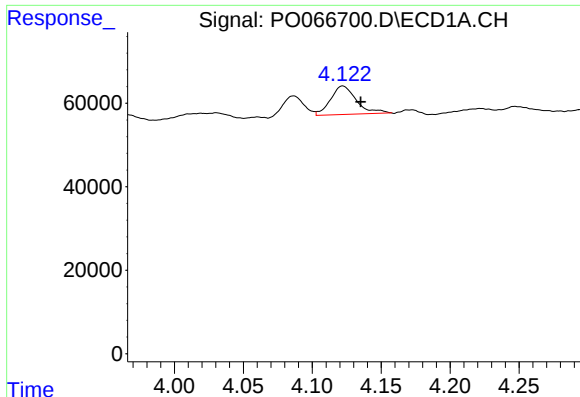


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: -0.013 min
Response: 88706
Conc: 2.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
40708


Manual Integrations
APPROVED

Sohil
2/24/2020 10:28:04 AM

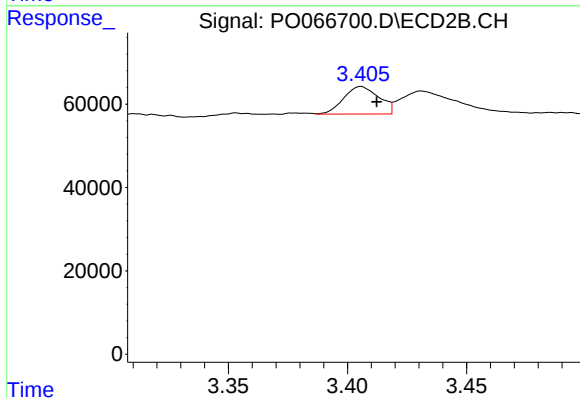


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: -0.007 min
Response: 69450
Conc: 1.72 ng/ml m

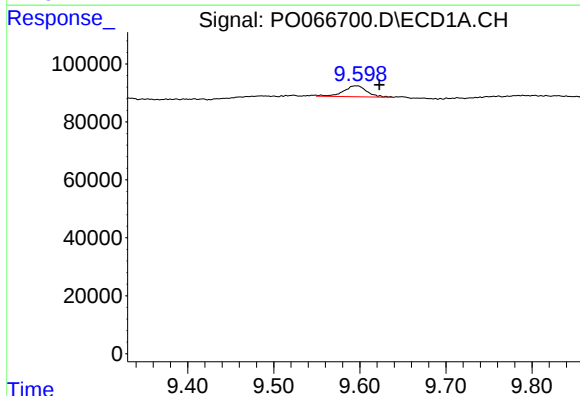

#2 Decachlorobiphenyl

R.T.: 9.598 min
Delta R.T.: -0.025 min
Response: 70564
Conc: 1.54 ng/ml m

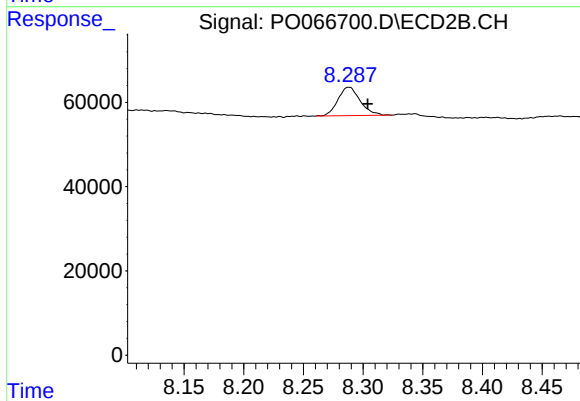

#2 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: -0.016 min
Response: 87662
Conc: 1.46 ng/ml