

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
Data File : P0042530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2018 9:28
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 10:21:35 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 21 09:28:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.102	3.349	5388701	7893418	21.757	21.467
2) SA Decachlor...	9.484	8.136	5654645	8875979	19.235	19.344

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
Data File : P0042530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2018 9:28
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 10:21:35 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 21 09:28:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

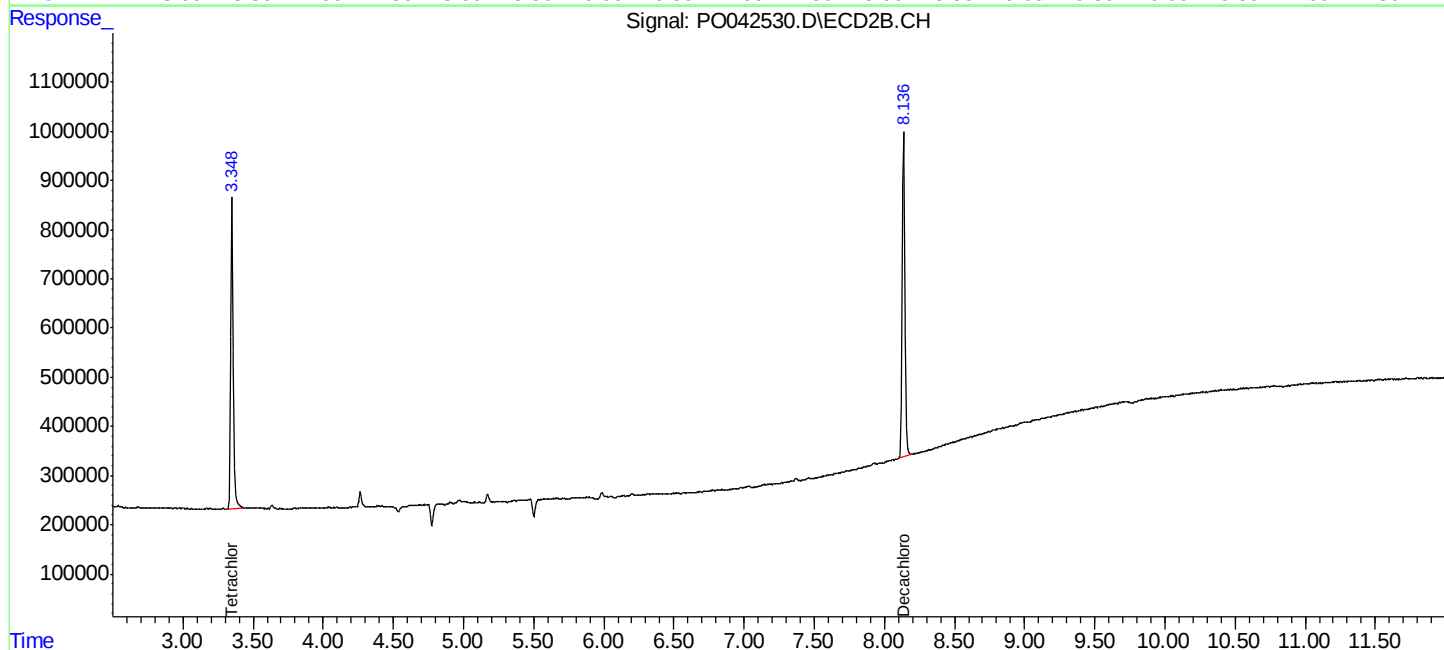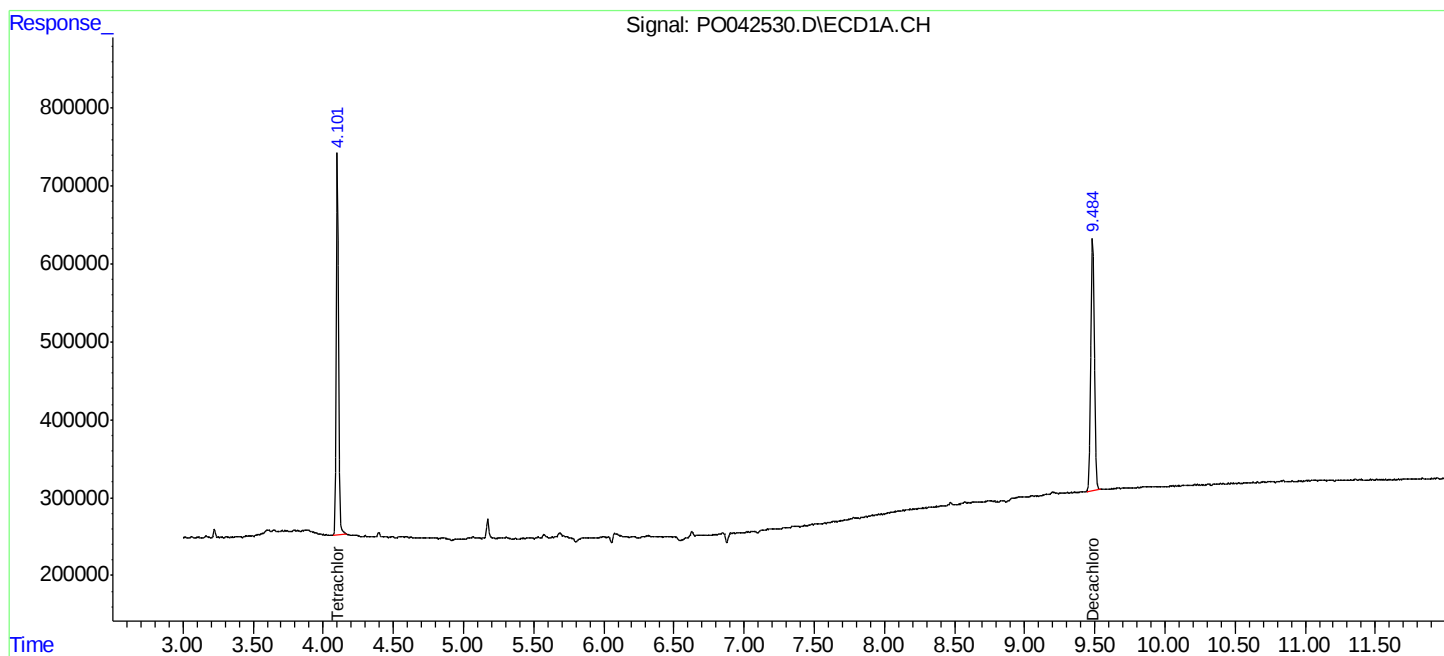


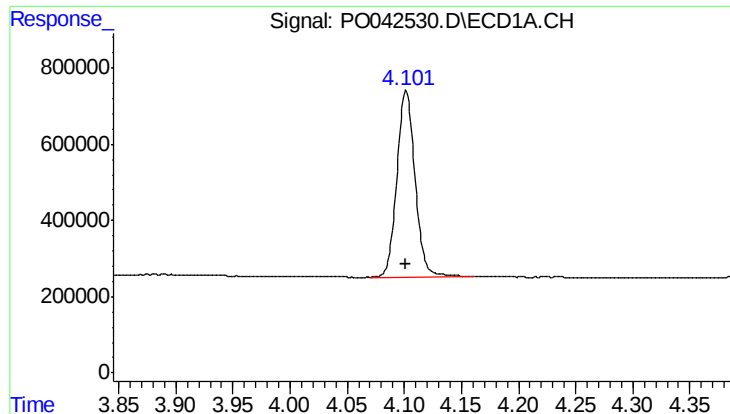

#1 Tetrachloro-m-xylene


R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 5388701
Conc: 21.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

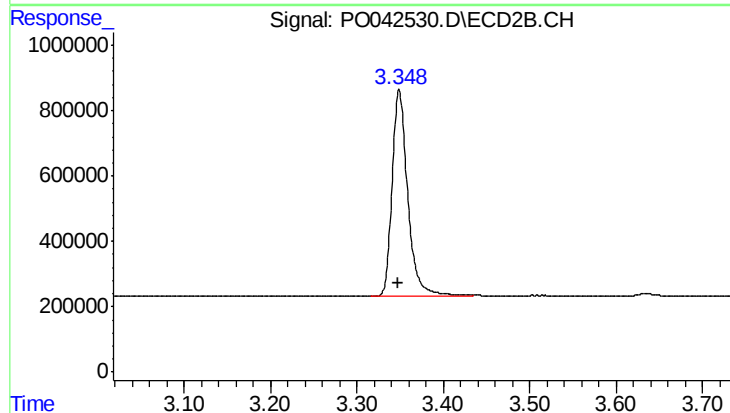


#1 Tetrachloro-m-xylene

R.T.: 3.349 min
Delta R.T.: 0.000 min
Response: 7893418
Conc: 21.47 ng/ml

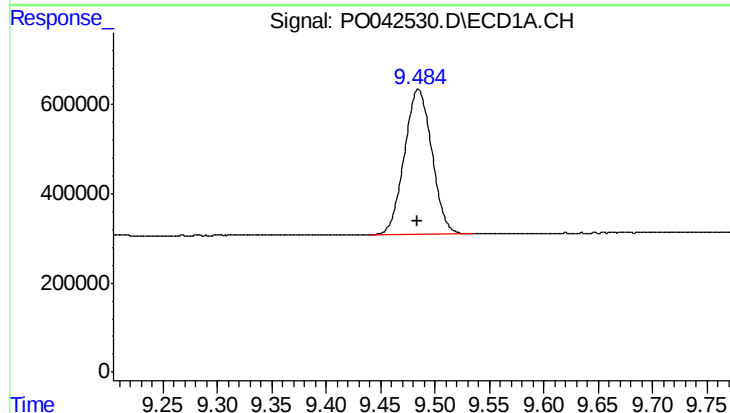

#2 Decachlorobiphenyl

R.T.: 9.484 min
Delta R.T.: 0.000 min
Response: 5654645
Conc: 19.24 ng/ml

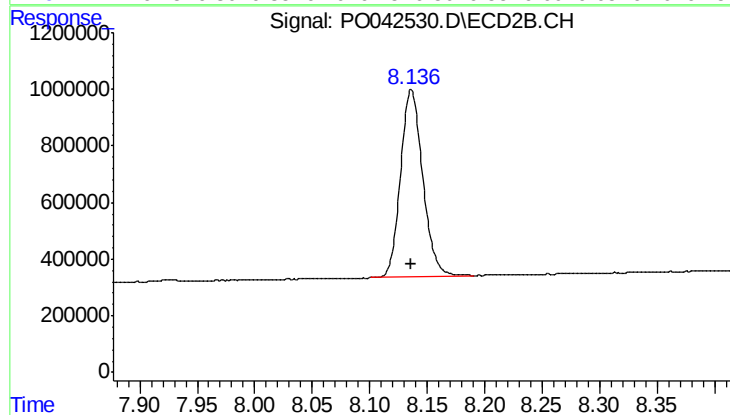

#2 Decachlorobiphenyl

R.T.: 8.136 min
Delta R.T.: 0.000 min
Response: 8875979
Conc: 19.34 ng/ml