

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
 Data File : P0042539.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Feb 2018 12:02
 Operator : SM/UA
 Sample : J1604-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 12:35:38 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 21 09:28:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.107	3.352	2256371	5202116	9.110	14.148 #
2) SA Decachlor...	9.493	8.141	1089836	1249693	3.707	2.724 #
Target Compounds						
7) L1 AR-1016-5	0.000	5.079	0	1393605	N.D.	131.840 #
12) L3 AR-1232-2	5.177	0.000	350664	0	108.869	N.D. #
23) L5 AR-1248-3	0.000	5.079	0	1393605	N.D.	79.839 #
26) L6 AR-1254-1	6.231	5.079	3548294	1393605	234.824	65.249 #
35) L7 AR-1260-5	7.887	0.000	1681149	0	49.566	N.D. #
40) L8 AR-1262-5	7.887	0.000	1681149	0	49.092	N.D. #
44) L9 AR-1268-4	0.000	7.606	0	433560	N.D.	16.132 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
Data File : P0042539.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2018 12:02
Operator : SM/UA
Sample : J1604-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 12:35:38 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 21 09:28:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

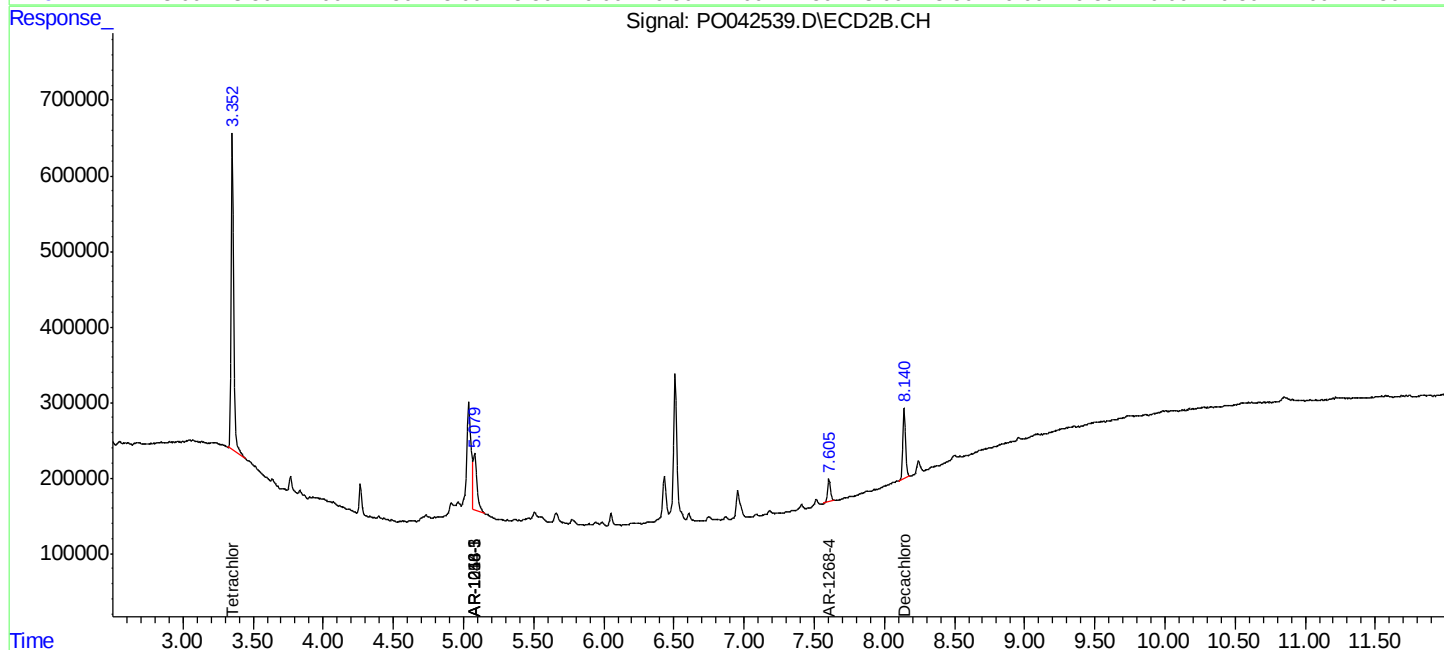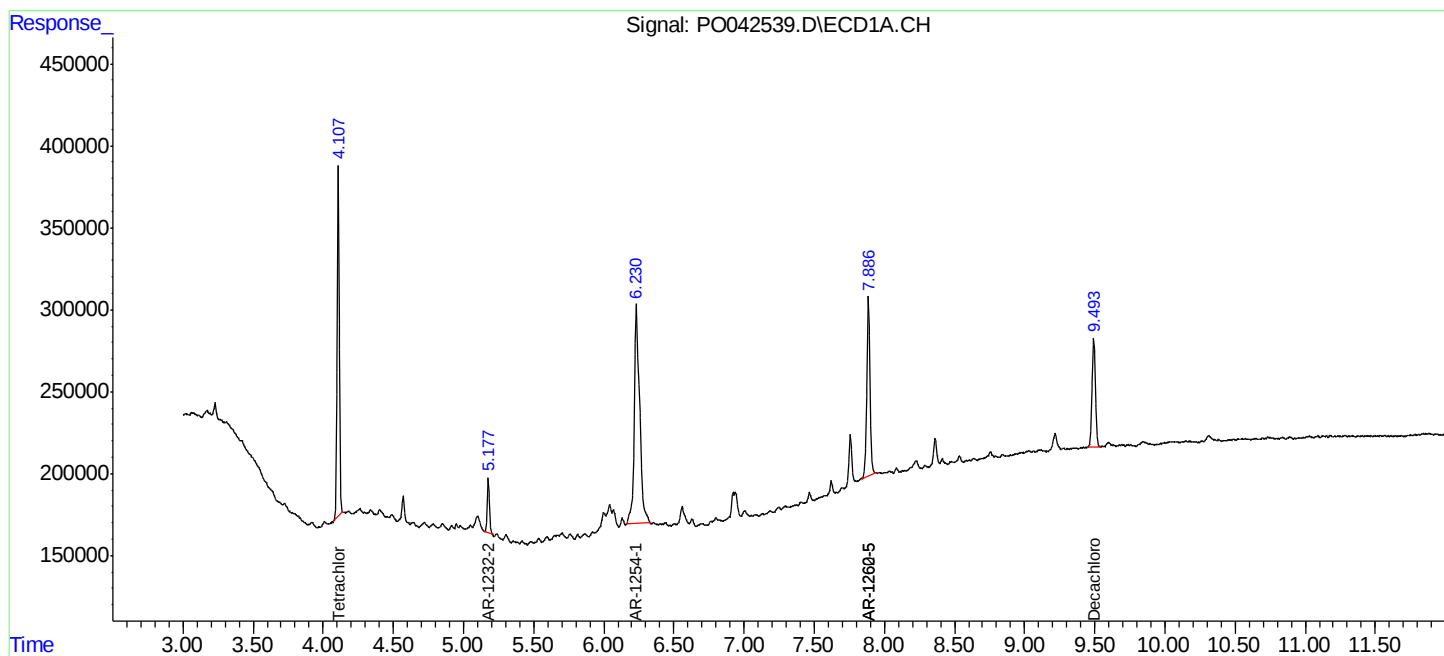


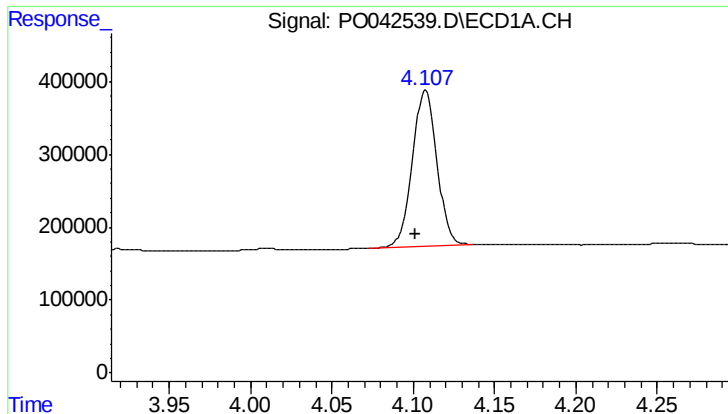

#1 Tetrachloro-m-xylene


R.T.: 4.107 min
Delta R.T.: 0.006 min
Response: 2256371
Conc: 9.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4

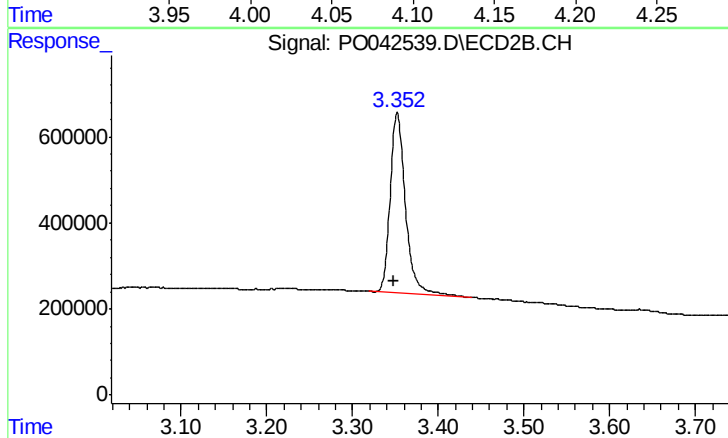


#1 Tetrachloro-m-xylene

R.T.: 3.352 min
Delta R.T.: 0.004 min
Response: 5202116
Conc: 14.15 ng/ml

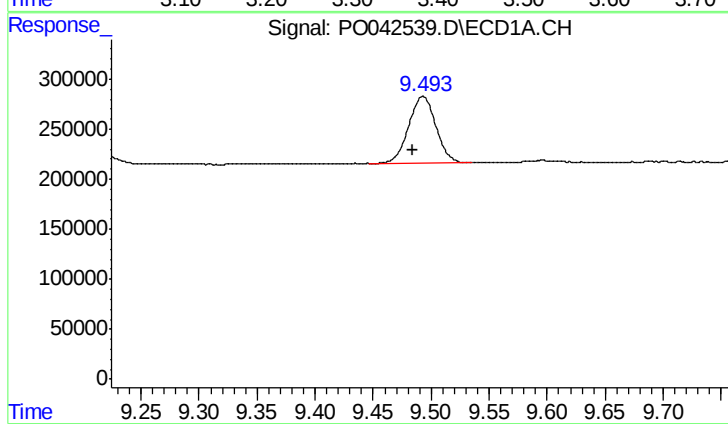


#2 Decachlorobiphenyl

R.T.: 9.493 min
Delta R.T.: 0.009 min
Response: 1089836
Conc: 3.71 ng/ml

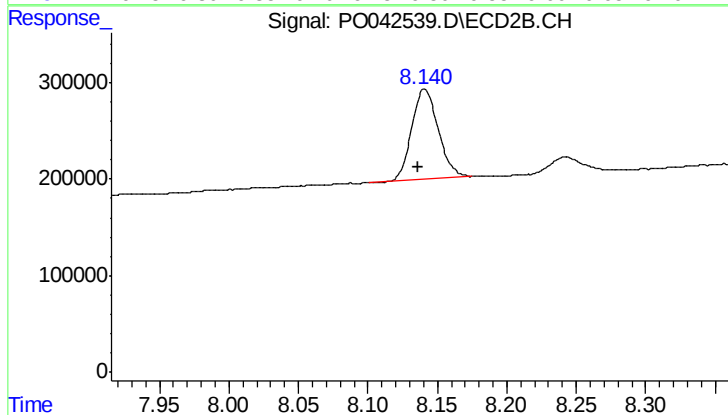

#2 Decachlorobiphenyl


R.T.: 8.141 min
Delta R.T.: 0.004 min
Response: 1249693
Conc: 2.72 ng/ml

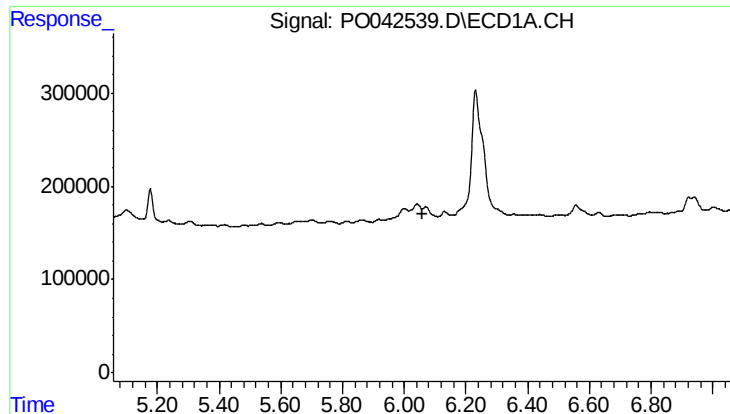

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4

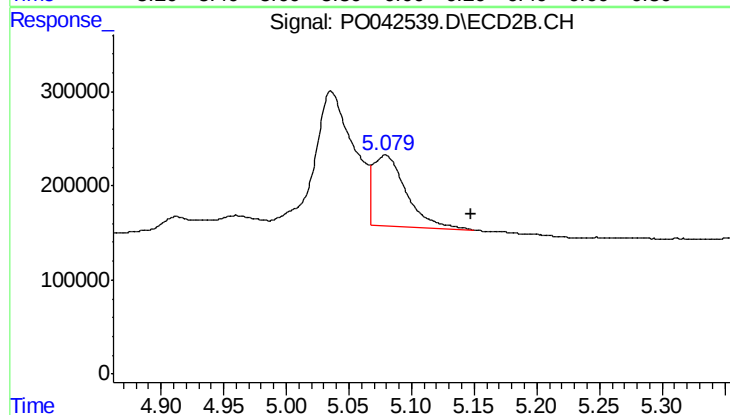


#7 AR-1016-5

R.T.: 5.079 min
Delta R.T.: -0.069 min
Response: 1393605
Conc: 131.84 ng/ml

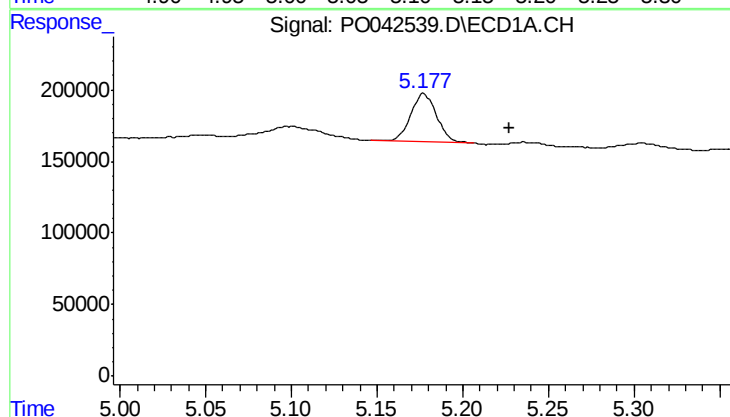


#12 AR-1232-2

R.T.: 5.177 min
Delta R.T.: -0.050 min
Response: 350664
Conc: 108.87 ng/ml

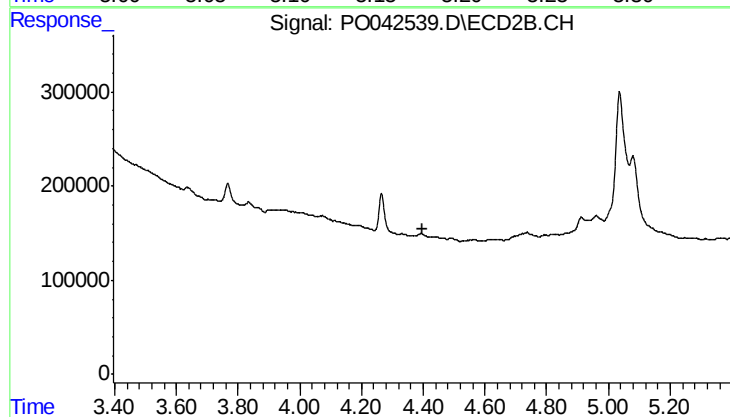

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.396 min
Response: 0
Conc: N.D.

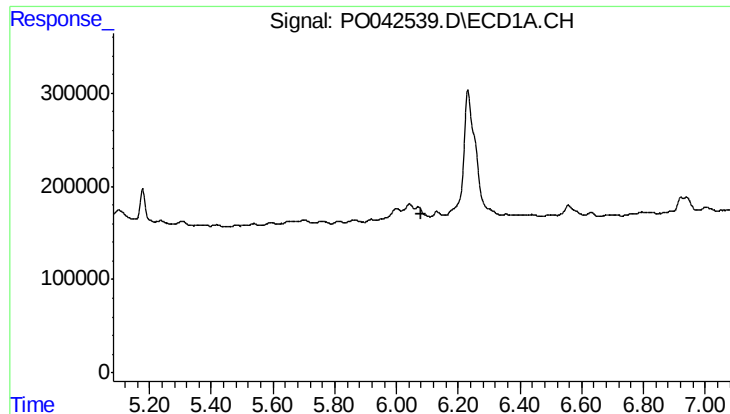

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.082 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4

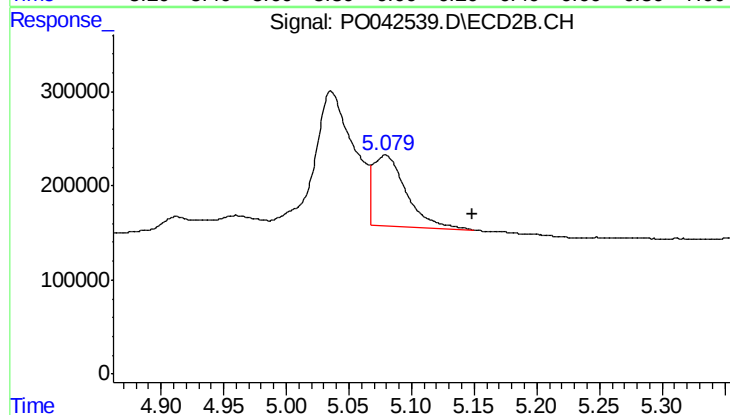


#23 AR-1248-3

R.T.: 5.079 min
Delta R.T.: -0.069 min
Response: 1393605
Conc: 79.84 ng/ml

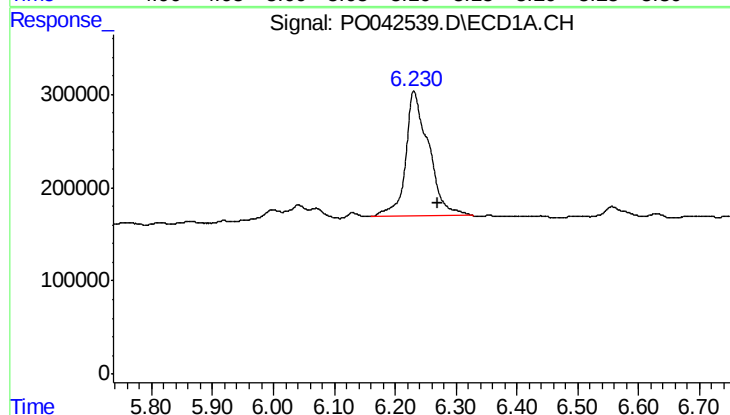


#26 AR-1254-1

R.T.: 6.231 min
Delta R.T.: -0.040 min
Response: 3548294
Conc: 234.82 ng/ml

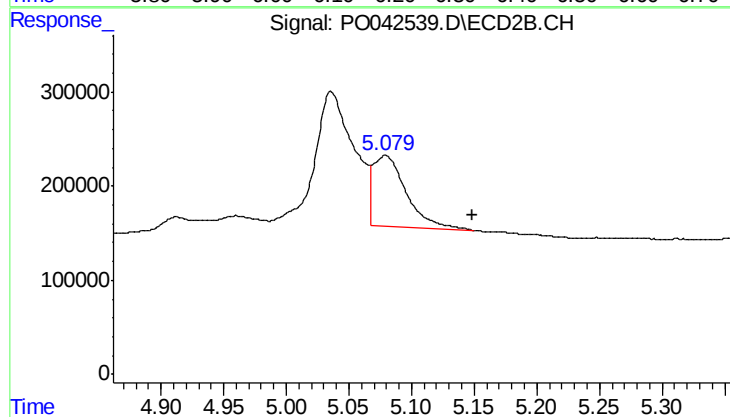

#26 AR-1254-1


R.T.: 5.079 min
Delta R.T.: -0.069 min
Response: 1393605
Conc: 65.25 ng/ml

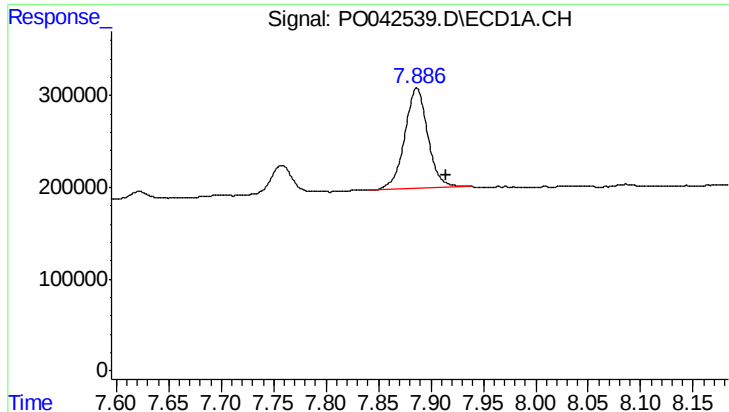

#35 AR-1260-5


R.T.: 7.887 min
Delta R.T.: -0.028 min
Response: 1681149
Conc: 49.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4

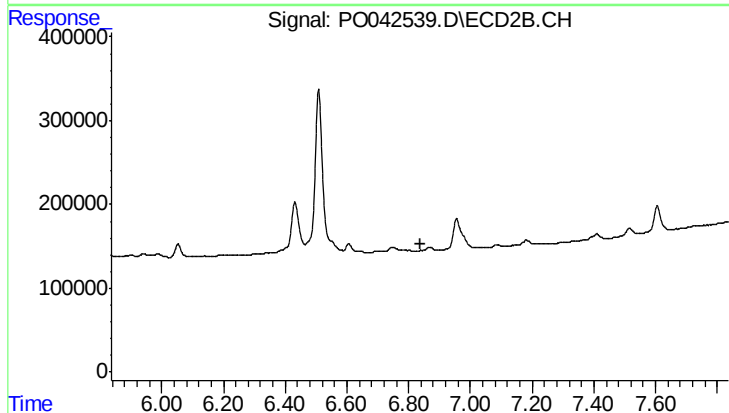


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

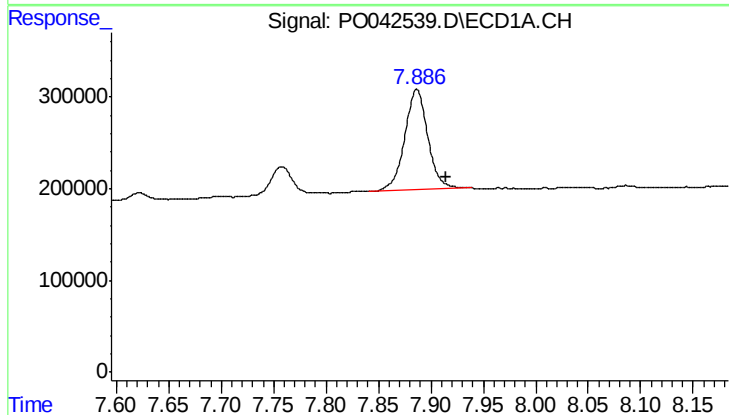


#40 AR-1262-5

R.T.: 7.887 min
Delta R.T.: -0.028 min
Response: 1681149
Conc: 49.09 ng/ml

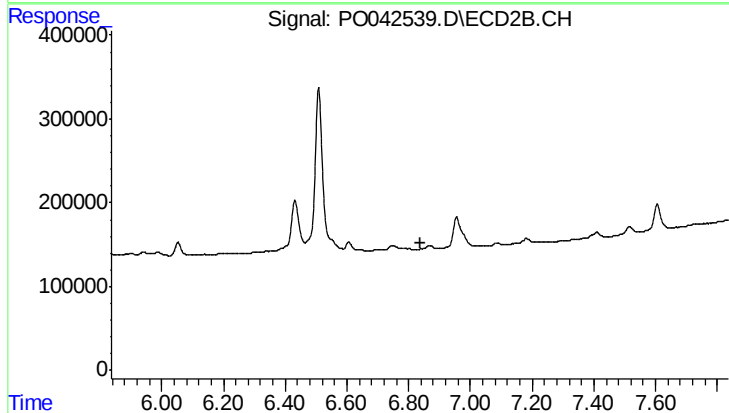

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

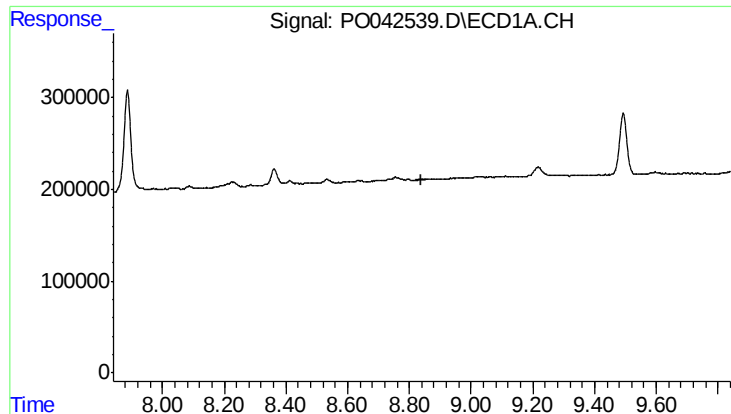

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.841 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-4

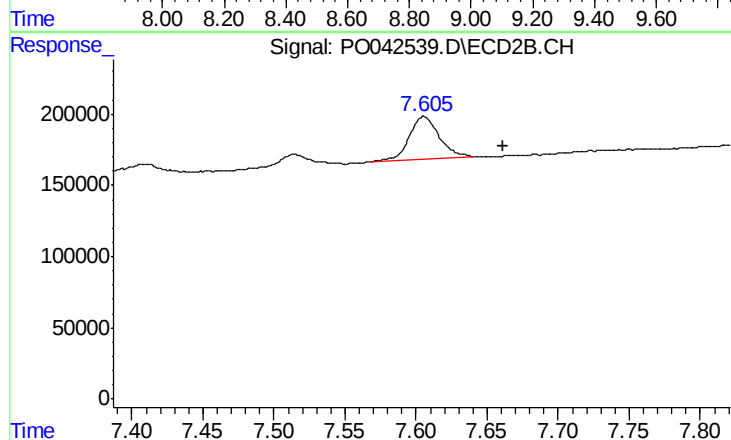

#44 AR-1268-4

R.T.: 7.606 min
Delta R.T.: -0.055 min
Response: 433560
Conc: 16.13 ng/ml