

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
 Data File : P0042541.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Feb 2018 12:32
 Operator : SM/UA
 Sample : J1604-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 13:12:03 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 21 09:28:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.104	3.351	4690176	7156855	18.936	19.464
2) SA Decachlor...	9.489	8.138	1995784	2347075	6.789	5.115
Target Compounds						
7) L1 AR-1016-5	0.000	5.080	0	1274889	N.D.	120.609 #
10) L2 AR-1221-3	0.000	3.765	0	555796	N.D.	65.057 #
11) L3 AR-1232-1	0.000	3.765	0	555796	N.D.	90.879 #
23) L5 AR-1248-3	0.000	5.080	0	1274889	N.D.	73.038 #
26) L6 AR-1254-1	6.237	5.080	1668514	1274889	110.421	59.691 #
35) L7 AR-1260-5	7.884	0.000	741362	0	21.858	N.D. #
40) L8 AR-1262-5	7.884	0.000	741362	0	21.649	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0022218\
Data File : P0042541.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Feb 2018 12:32
Operator : SM/UA
Sample : J1604-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 13:12:03 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 21 09:28:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

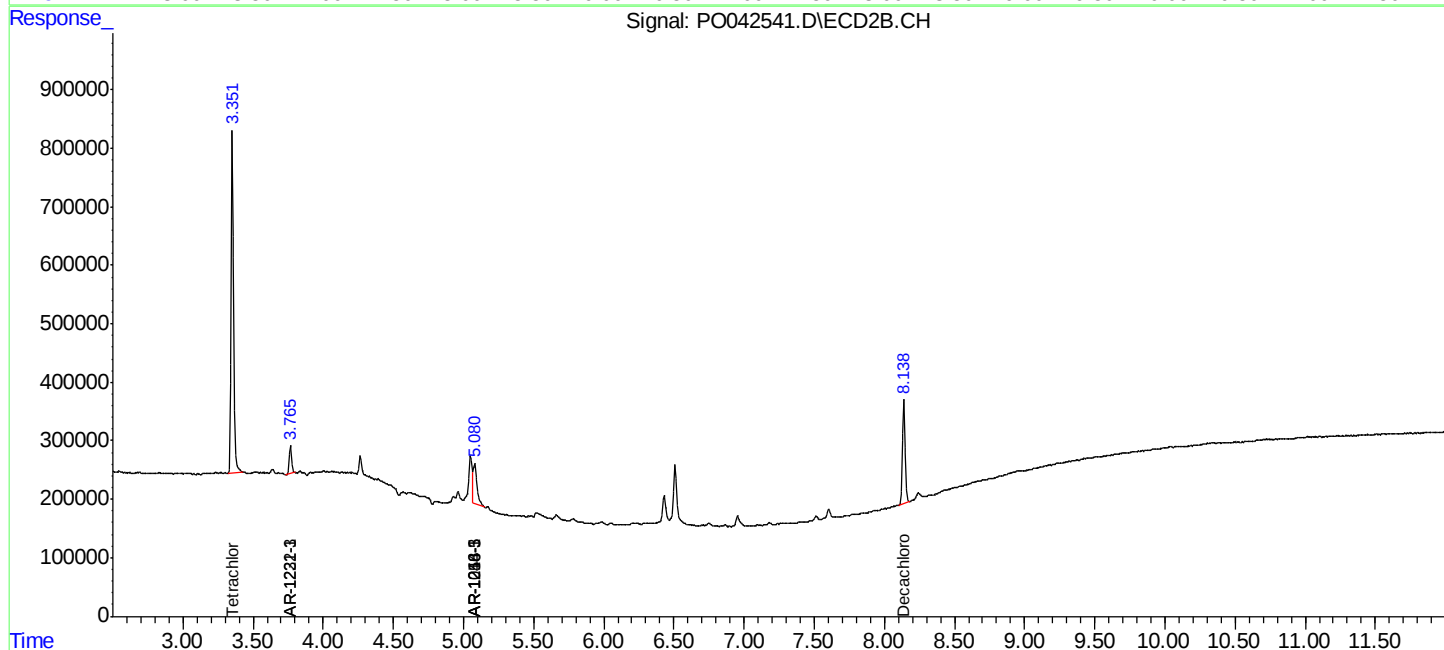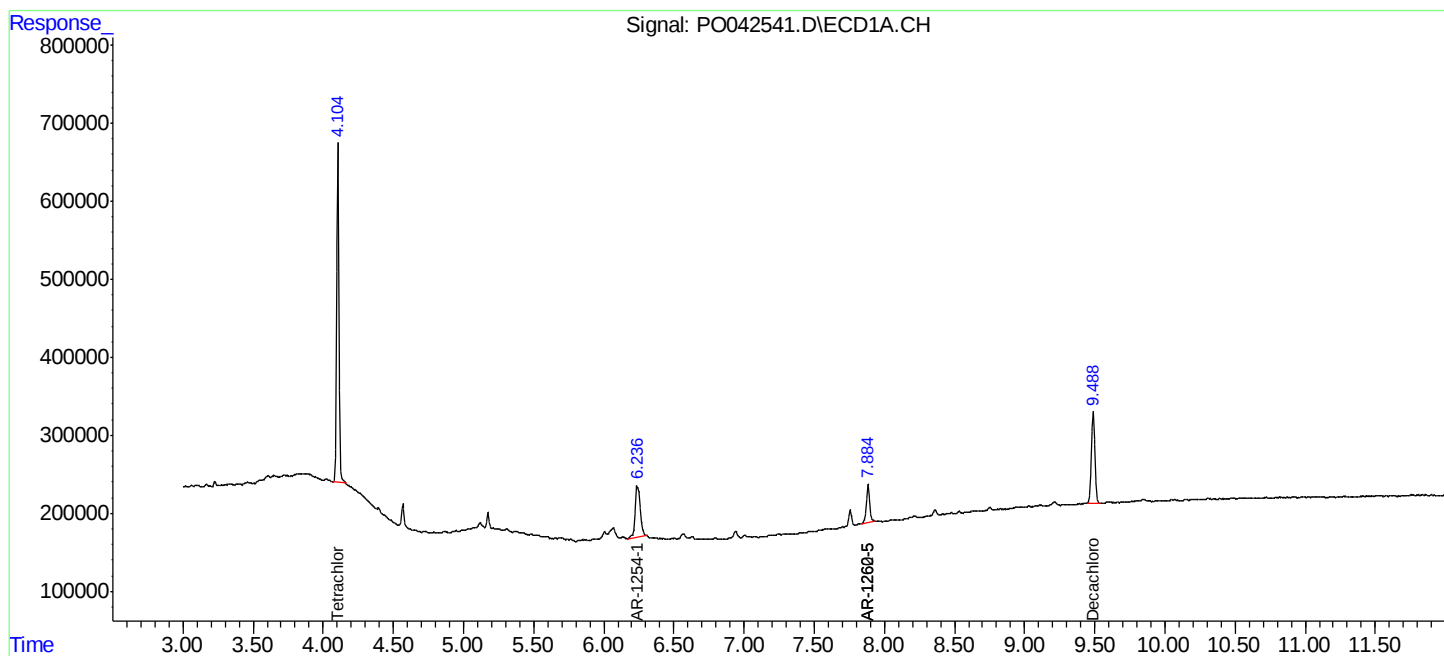


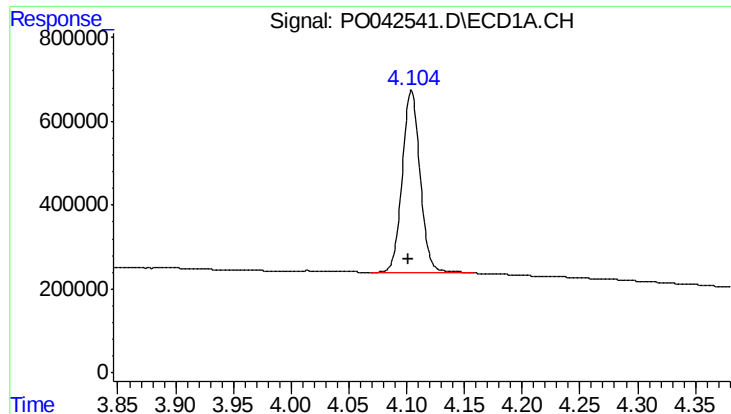

#1 Tetrachloro-m-xylene


R.T.: 4.104 min
Delta R.T.: 0.003 min
Response: 4690176
Conc: 18.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1RE

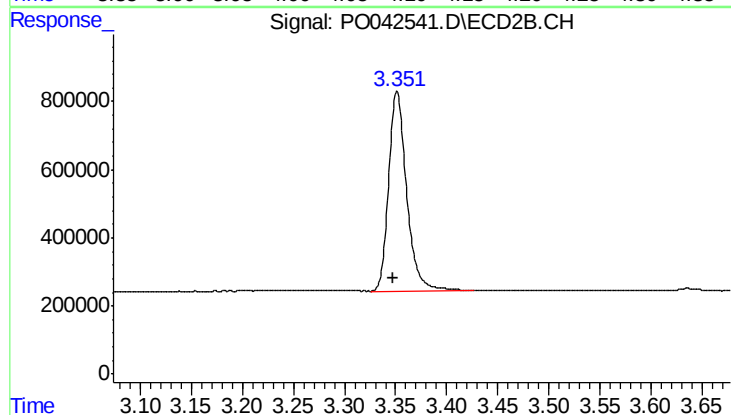


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: 0.003 min
Response: 7156855
Conc: 19.46 ng/ml

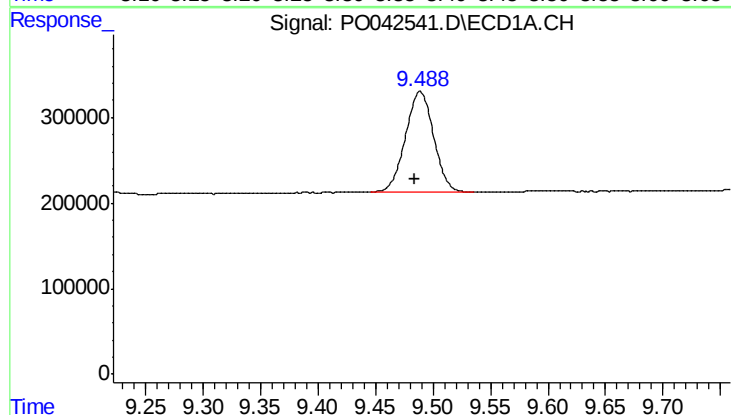


#2 Decachlorobiphenyl

R.T.: 9.489 min
Delta R.T.: 0.005 min
Response: 1995784
Conc: 6.79 ng/ml

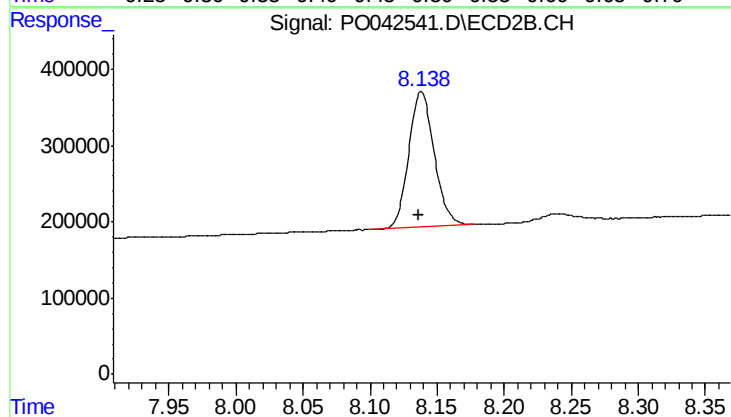

#2 Decachlorobiphenyl


R.T.: 8.138 min
Delta R.T.: 0.002 min
Response: 2347075
Conc: 5.12 ng/ml

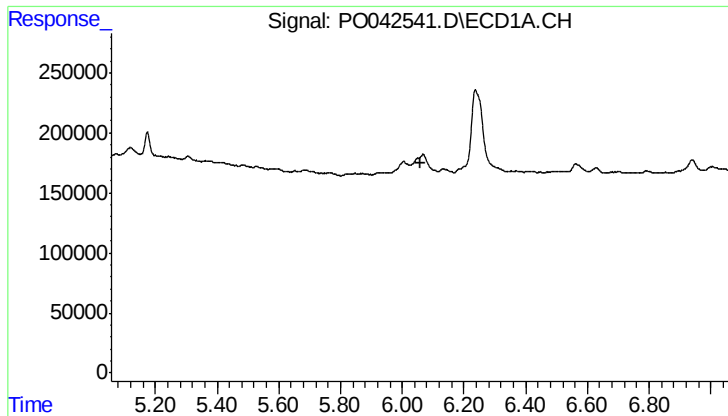

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1RE

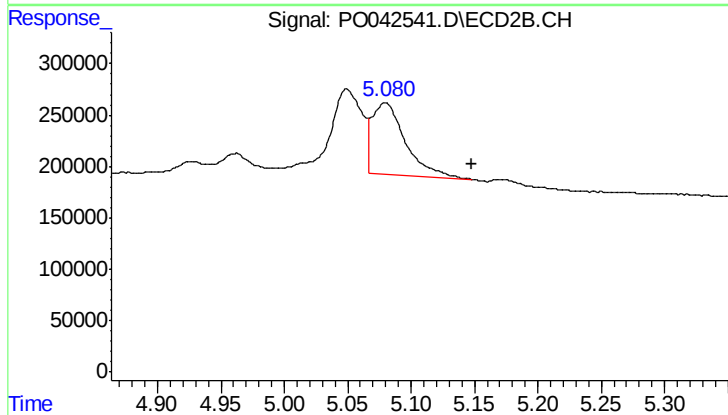


#7 AR-1016-5

R.T.: 5.080 min
Delta R.T.: -0.068 min
Response: 1274889
Conc: 120.61 ng/ml

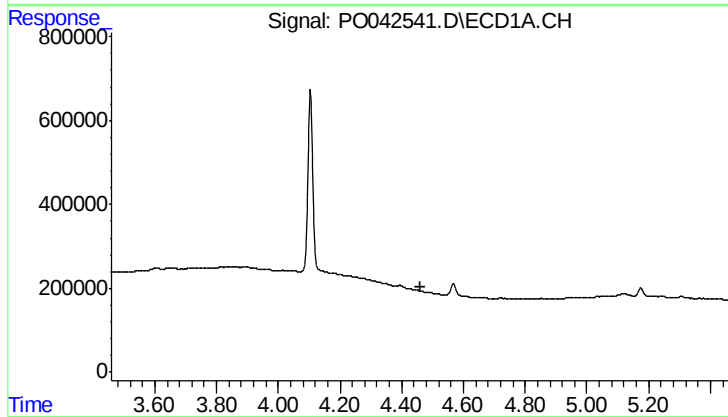


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

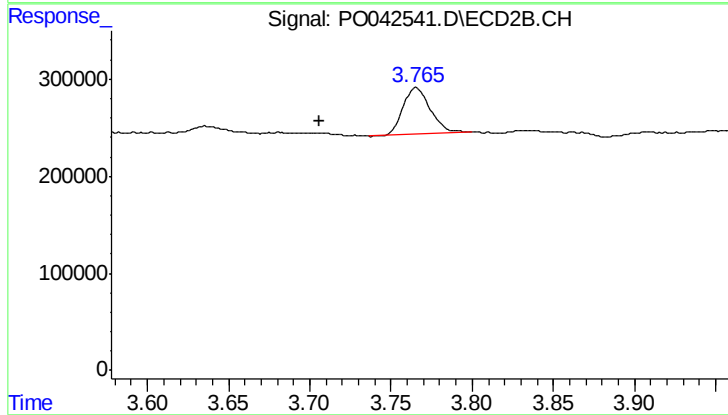

#10 AR-1221-3


R.T.: 3.765 min
Delta R.T.: 0.059 min
Response: 555796
Conc: 65.06 ng/ml

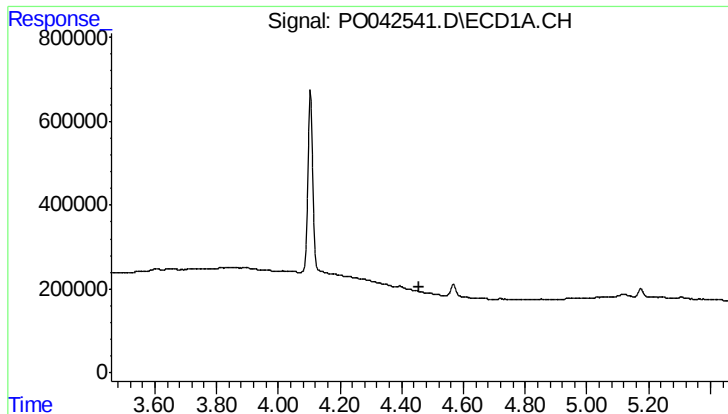

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-1RE

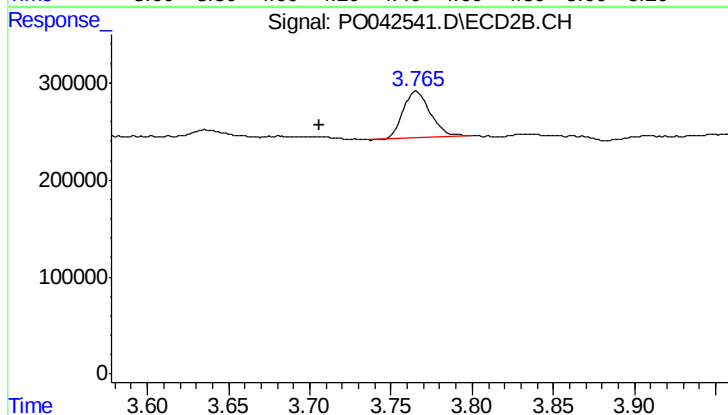


#11 AR-1232-1

R.T.: 3.765 min
Delta R.T.: 0.060 min
Response: 555796
Conc: 90.88 ng/ml

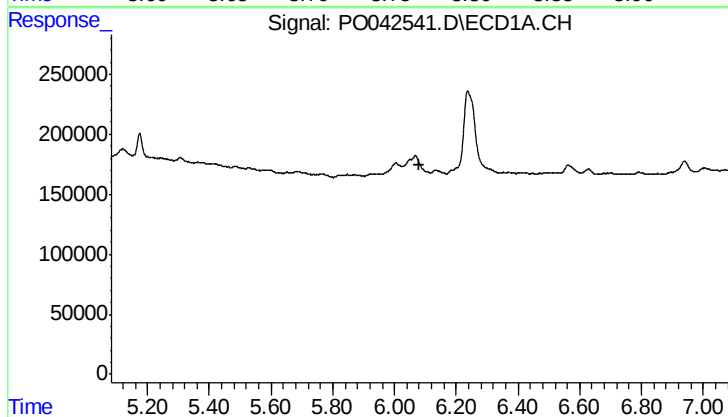


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 6.082 min
Response: 0
Conc: N.D.

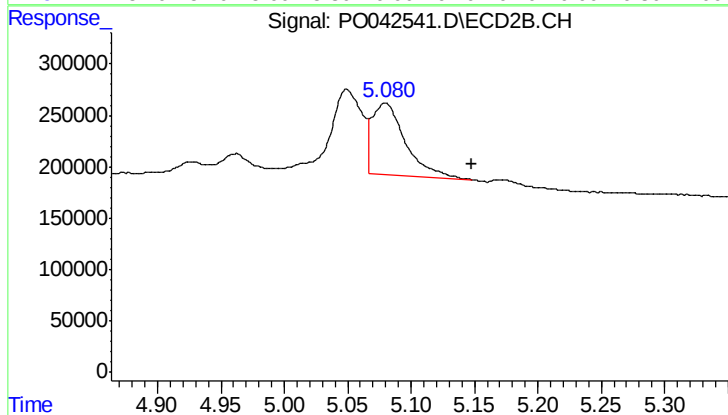

#23 AR-1248-3


R.T.: 5.080 min
Delta R.T.: -0.068 min
Response: 1274889
Conc: 73.04 ng/ml

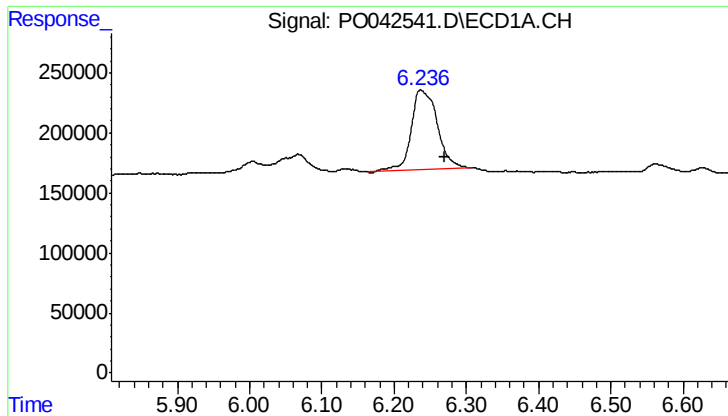

#26 AR-1254-1


R.T.: 6.237 min
Delta R.T.: -0.034 min
Response: 1668514
Conc: 110.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1RE

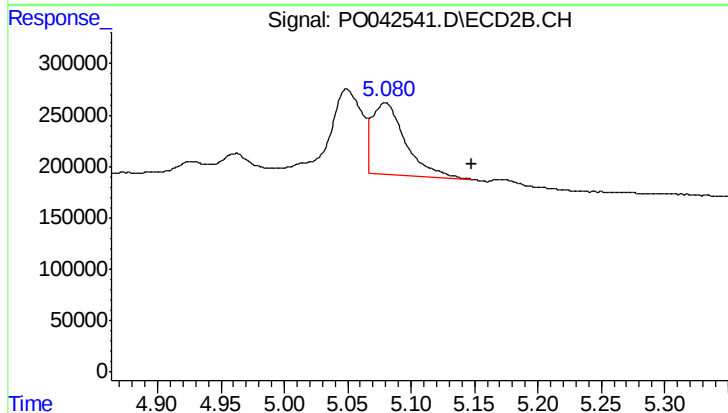


#26 AR-1254-1

R.T.: 5.080 min
Delta R.T.: -0.068 min
Response: 1274889
Conc: 59.69 ng/ml

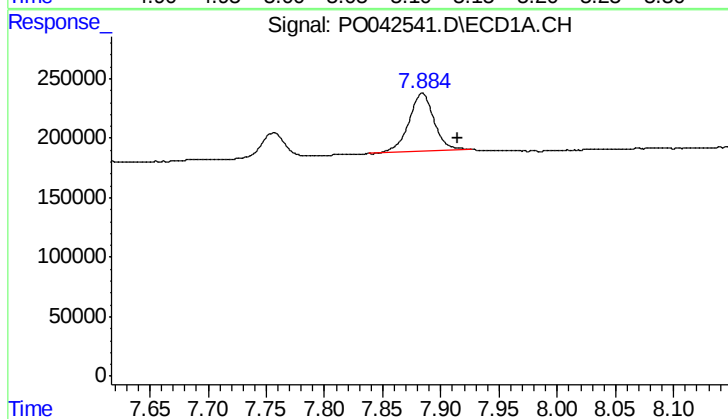


#35 AR-1260-5

R.T.: 7.884 min
Delta R.T.: -0.030 min
Response: 741362
Conc: 21.86 ng/ml

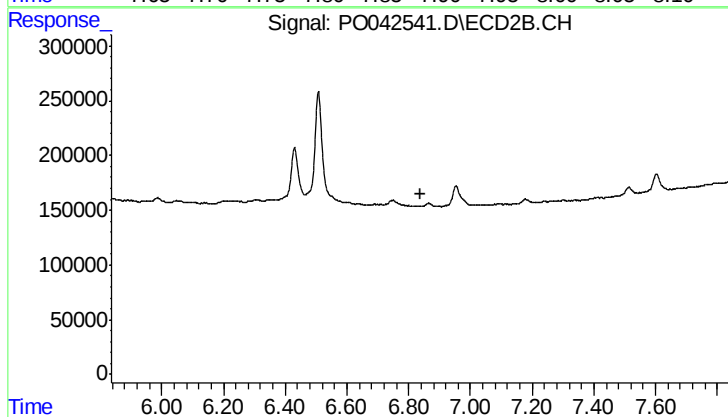

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

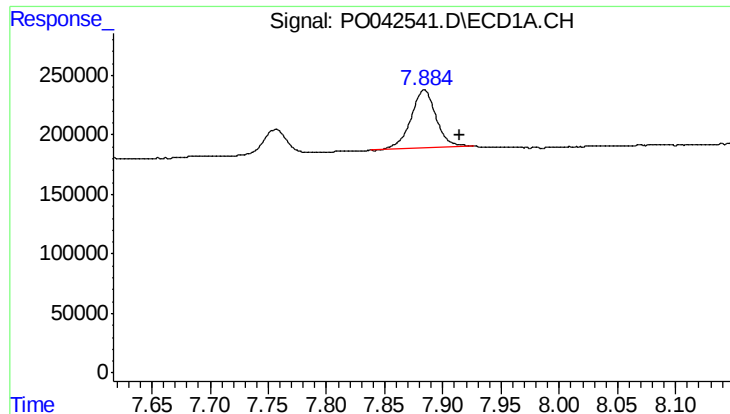

#40 AR-1262-5

R.T.: 7.884 min
Delta R.T.: -0.031 min
Response: 741362
Conc: 21.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1RE

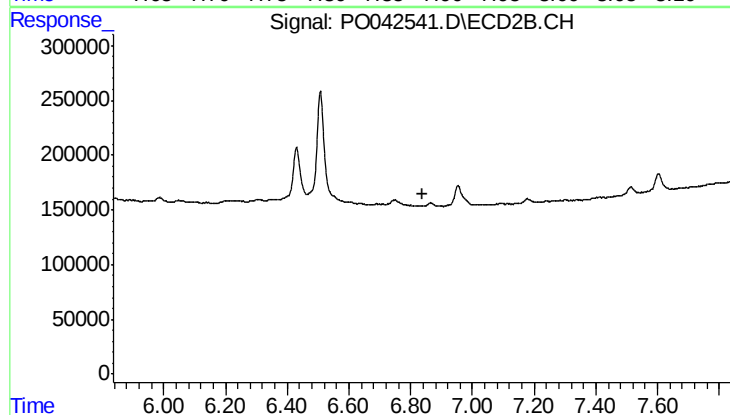

#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.