

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022420\
 Data File : P0066783.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Feb 2020 19:25
 Operator : DD\AJ
 Sample : L1655-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 01:06:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 14:58:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.406	1061865	1232193	25.270	22.813
2) SA Decachlor...	9.597	8.289	970229	1150557	23.642	20.704

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022420\
Data File : P0066783.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Feb 2020 19:25
Operator : DD\AJ
Sample : L1655-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 01:06:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 14:58:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

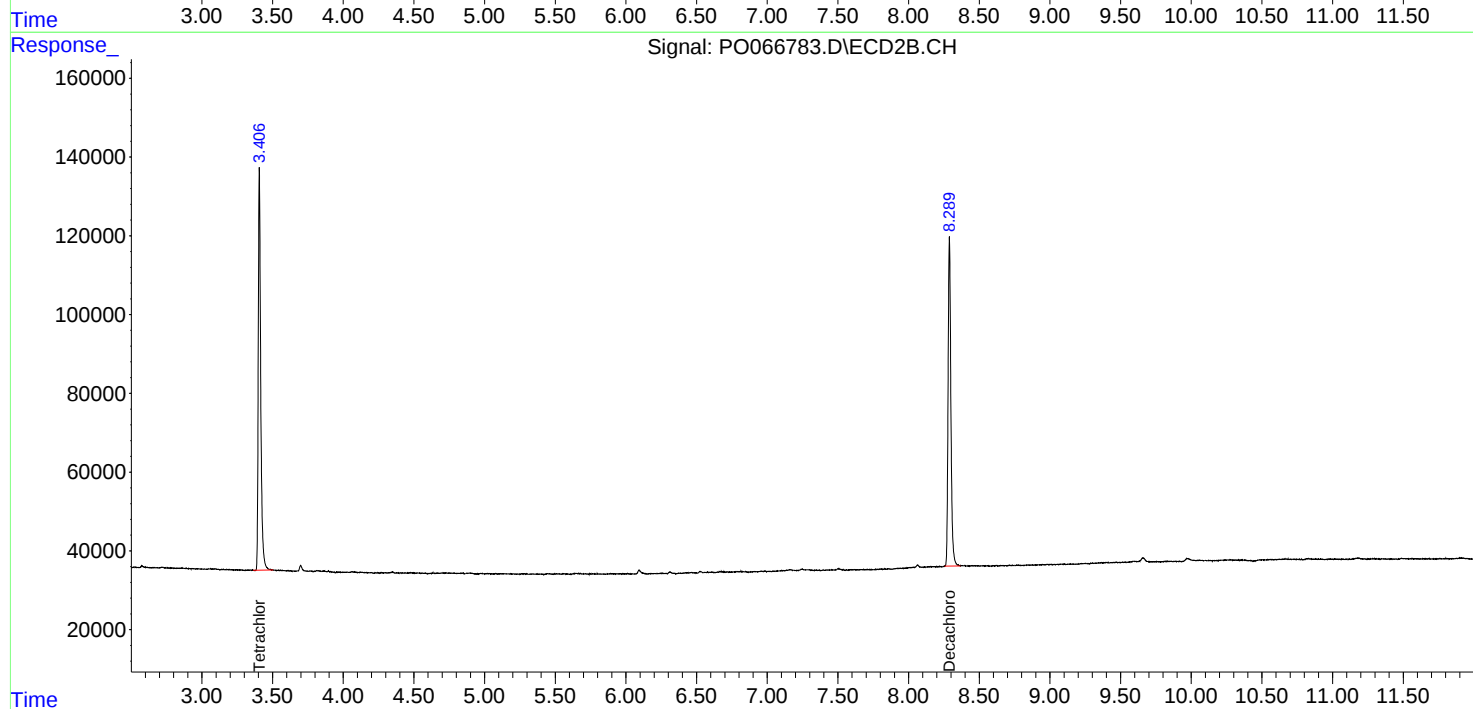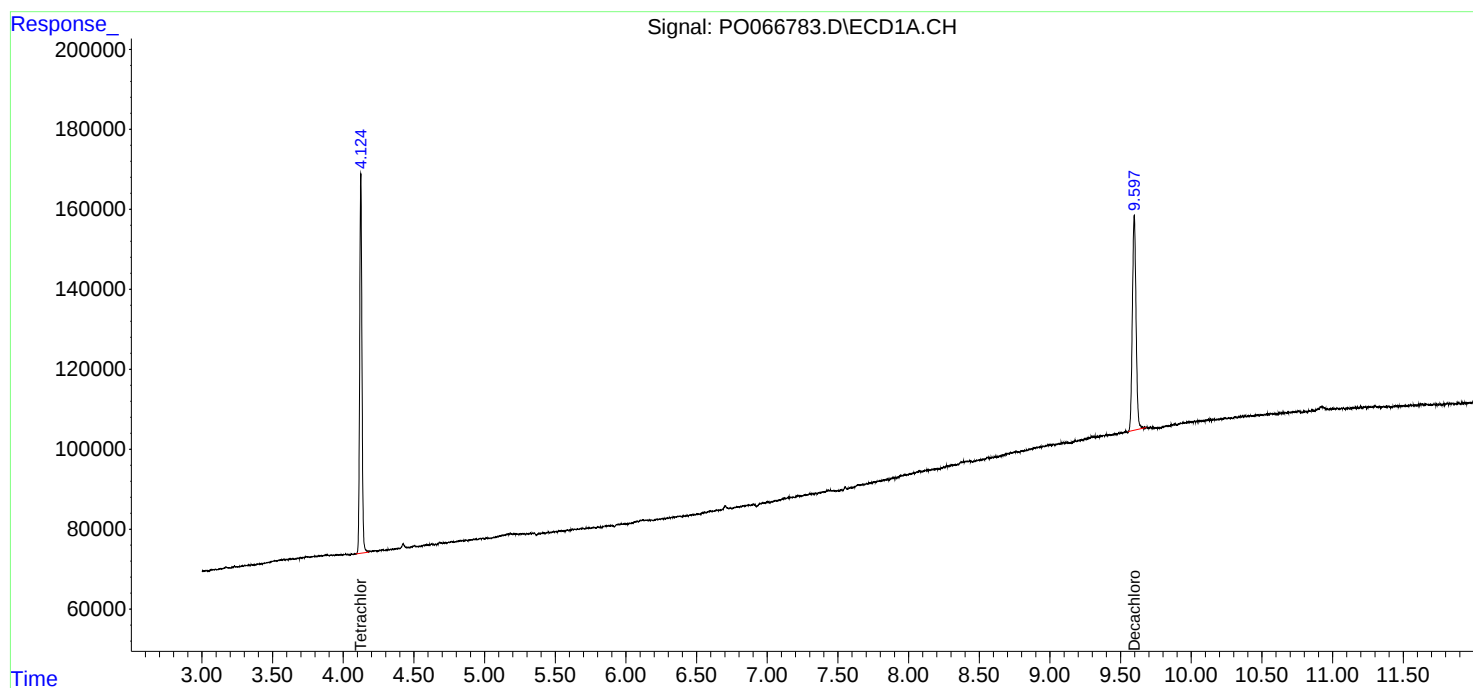


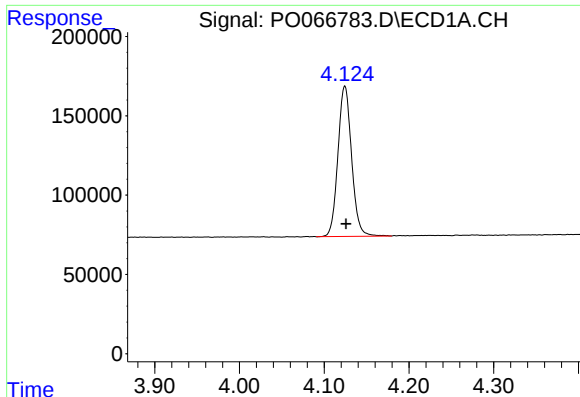

#1 Tetrachloro-m-xylene


R.T.: 4.124 min
Delta R.T.: -0.002 min
Response: 1061865
Conc: 25.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

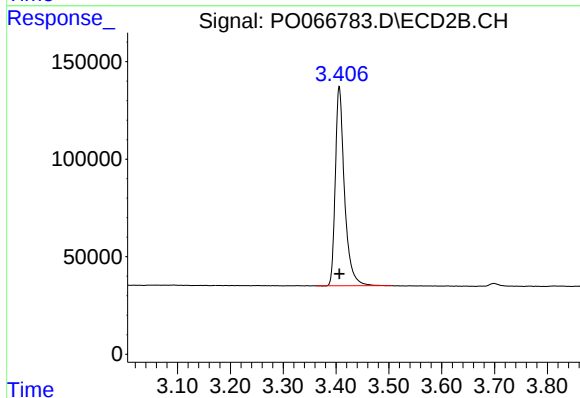


#1 Tetrachloro-m-xylene

R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 1232193
Conc: 22.81 ng/ml

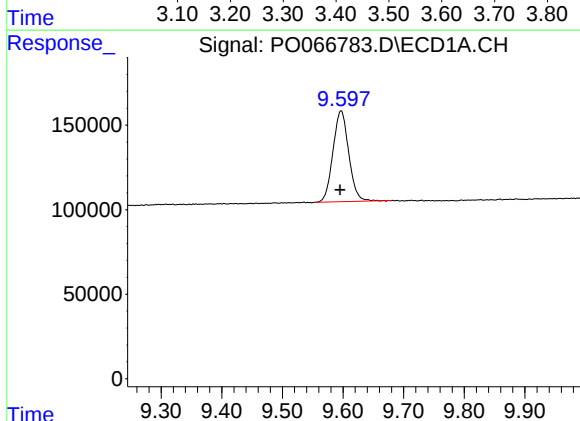

#2 Decachlorobiphenyl

R.T.: 9.597 min
Delta R.T.: 0.002 min
Response: 970229
Conc: 23.64 ng/ml

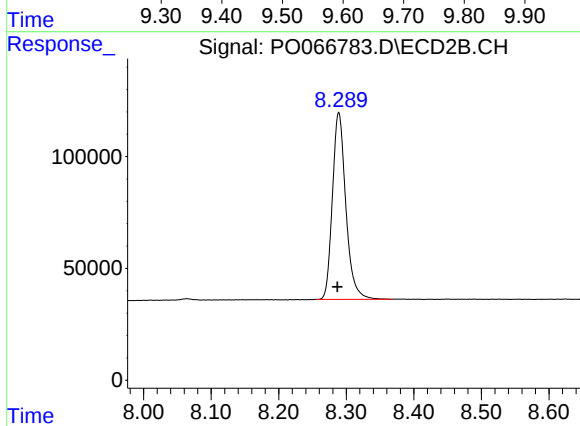

#2 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.002 min
Response: 1150557
Conc: 20.70 ng/ml