

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
 Data File : P0054047.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2019 20:30
 Operator : SM/SJ
 Sample : K1597-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 02:24:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.053	3.132	48483315	4709816	16.167	17.650
2)	SA Decachlor...	9.396	7.714	12876781	3013427	10.255	10.056
Target Compounds							
6)	L1 AR-1016-4	0.000	4.357	0	489822	N.D.	69.822 #
7)	L1 AR-1016-5	0.000	4.559	0	561495	N.D.	59.271 #
12)	L3 AR-1232-2	5.004	0.000	4130760	0	205.923	N.D. #
14)	L3 AR-1232-4	0.000	4.357	0	489822	N.D.	159.759 #
15)	L3 AR-1232-5	5.508	4.559	393230	561495	30.631	159.417 #
19)	L4 AR-1242-4	0.000	4.357	0	489822	N.D.	73.462 #
22)	L5 AR-1248-2	5.508	4.357	393230	489822	7.703	51.906 #
23)	L5 AR-1248-3	0.000	4.357	0	489822	N.D.	50.873 #
24)	L5 AR-1248-4	0.000	4.559	0	561495	N.D.	46.688 #
29)	L6 AR-1254-4	0.000	5.518	0	1956381	N.D.	45.089 #
31)	L7 AR-1260-1	0.000	5.460	0	1685754	N.D.	88.326 #
32)	L7 AR-1260-2	0.000	5.630	0	719447	N.D.	30.792 #
38)	L8 AR-1262-3	0.000	6.789	0	380226	N.D.	24.042 #
39)	L8 AR-1262-4	0.000	6.789	0	380226	N.D.	12.979 #
41)	L9 AR-1268-1	0.000	6.789	0	380226	N.D.	8.337 #
42)	L9 AR-1268-2	0.000	6.789	0	380226	N.D.	8.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022519\
Data File : PO054047.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 20:30
Operator : SM/SJ
Sample : K1597-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:24:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

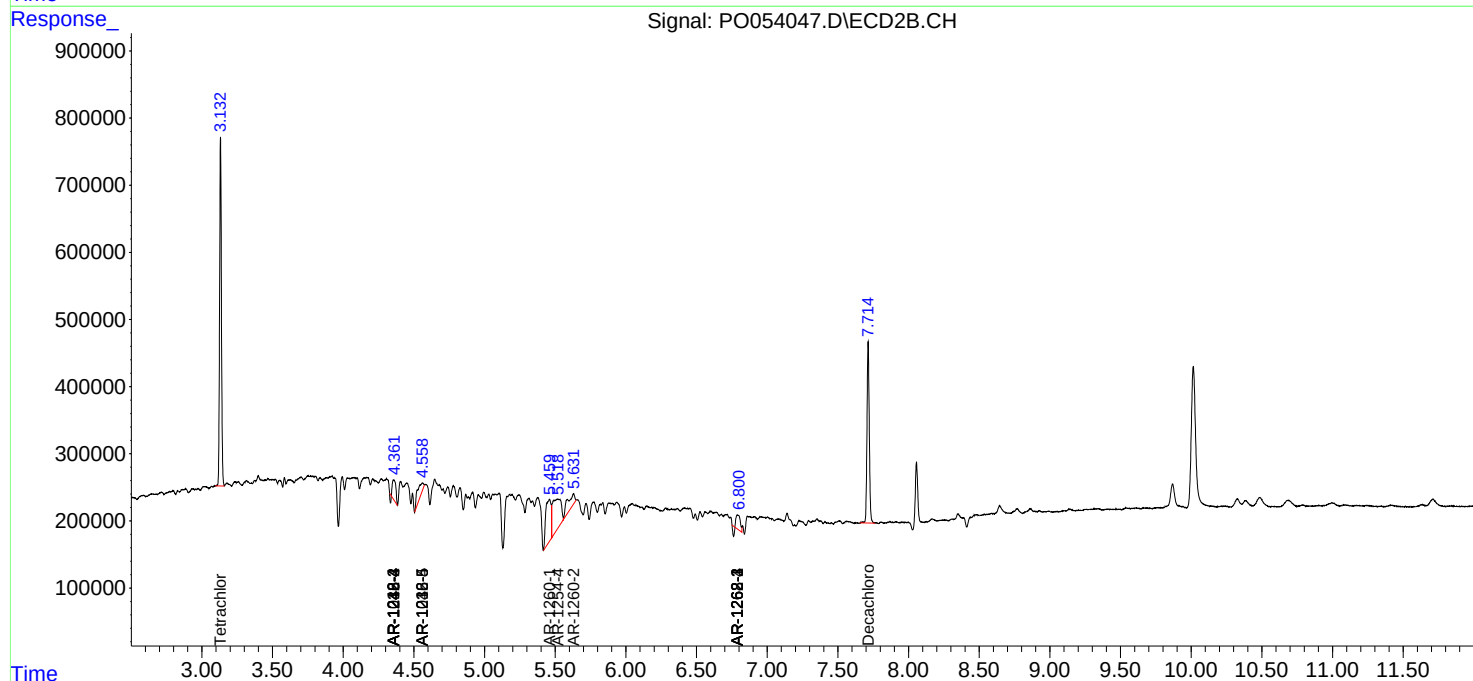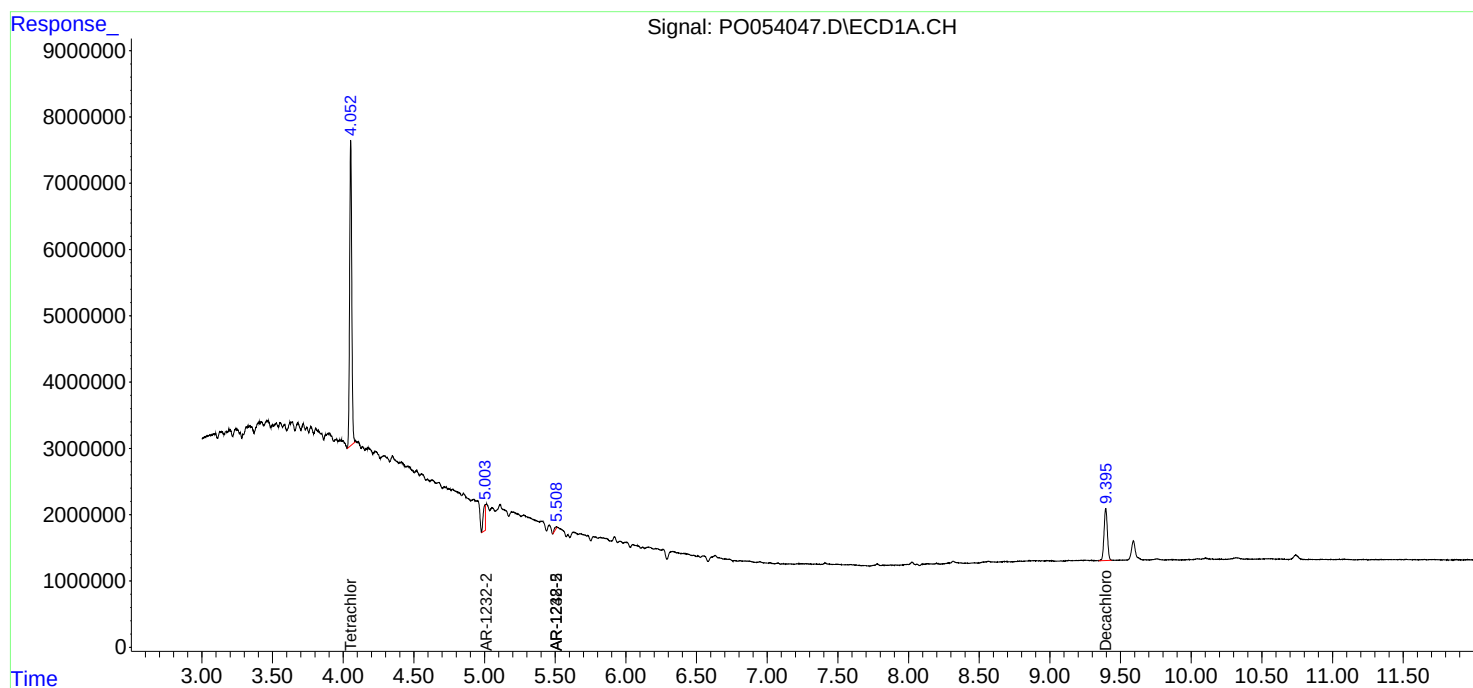


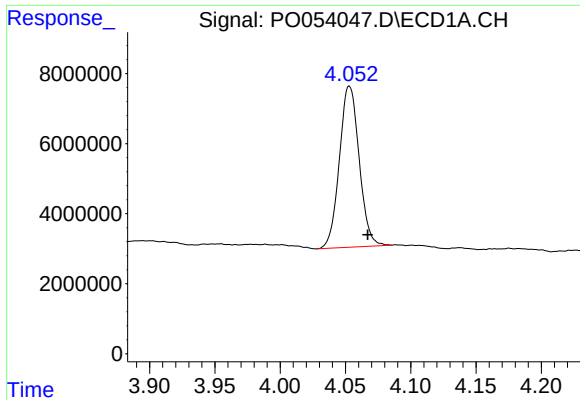

#1 Tetrachloro-m-xylene


R.T.: 4.053 min
Delta R.T.: -0.014 min
Response: 48483315
Conc: 16.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-26

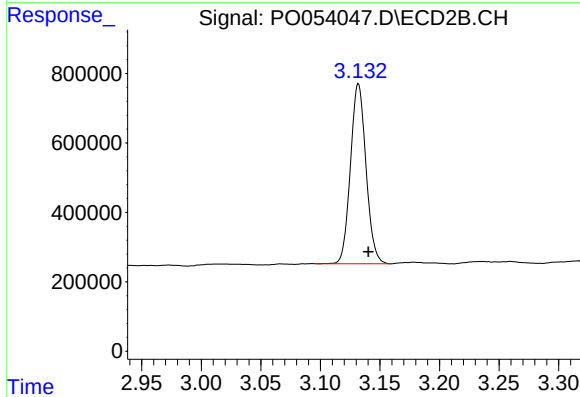


#1 Tetrachloro-m-xylene

R.T.: 3.132 min
Delta R.T.: -0.008 min
Response: 4709816
Conc: 17.65 ng/ml

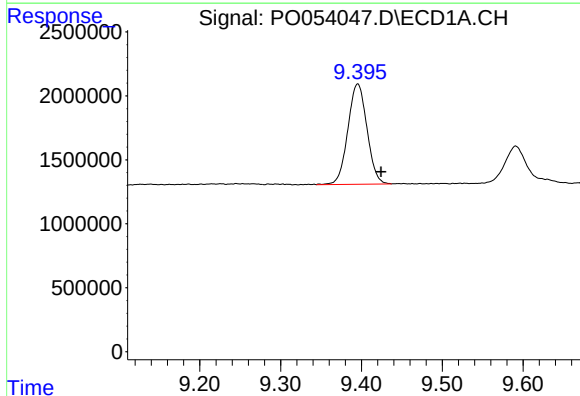


#2 Decachlorobiphenyl

R.T.: 9.396 min
Delta R.T.: -0.028 min
Response: 12876781
Conc: 10.25 ng/ml

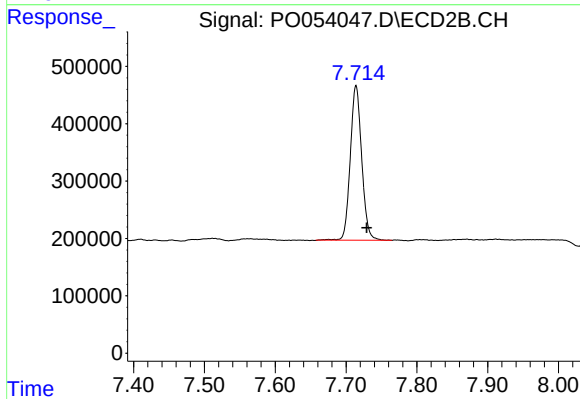

#2 Decachlorobiphenyl


R.T.: 7.714 min
Delta R.T.: -0.015 min
Response: 3013427
Conc: 10.06 ng/ml

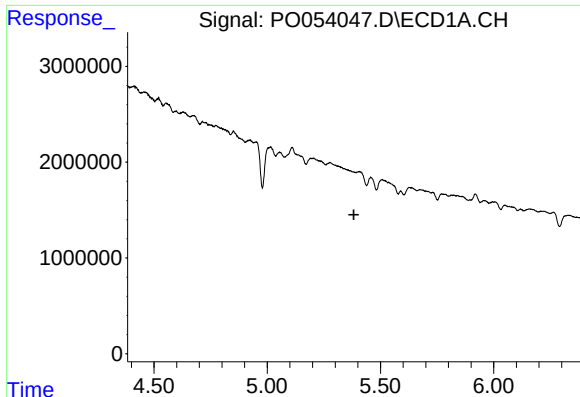

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26

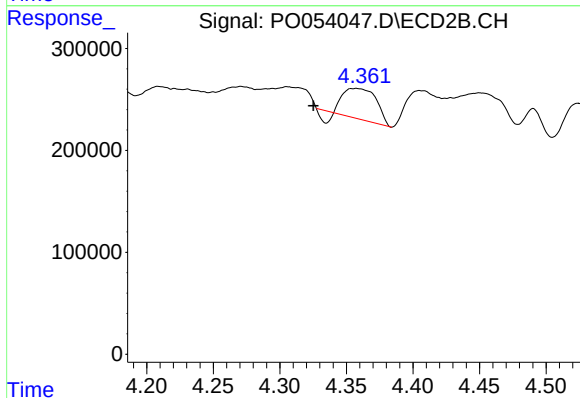


#6 AR-1016-4

R.T.: 4.357 min
Delta R.T.: 0.032 min
Response: 489822
Conc: 69.82 ng/ml

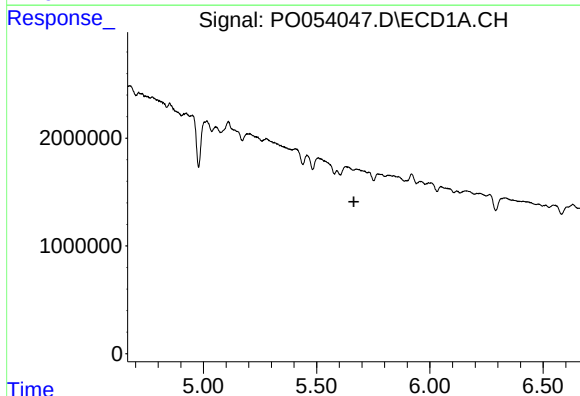


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 5.664 min
Response: 0
Conc: N.D.

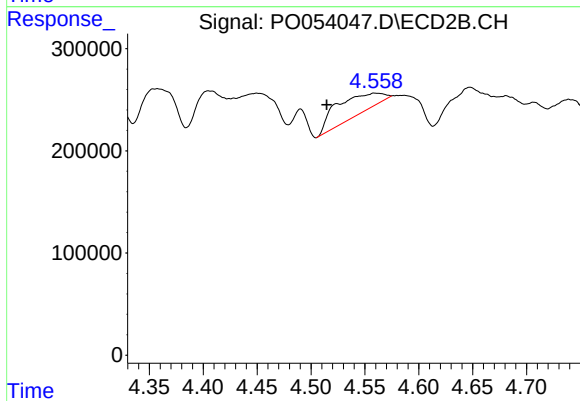

#7 AR-1016-5


R.T.: 4.559 min
Delta R.T.: 0.044 min
Response: 561495
Conc: 59.27 ng/ml

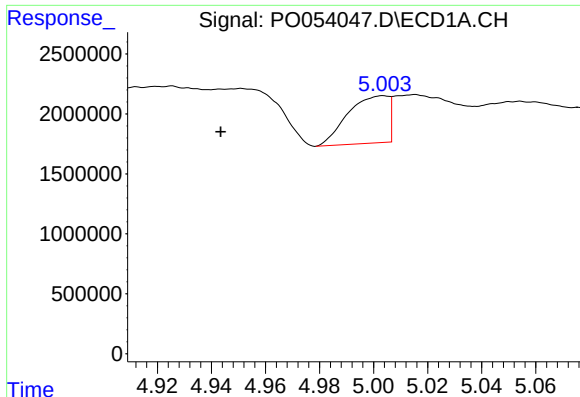

#12 AR-1232-2


R.T.: 5.004 min
Delta R.T.: 0.060 min
Response: 4130760
Conc: 205.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-26

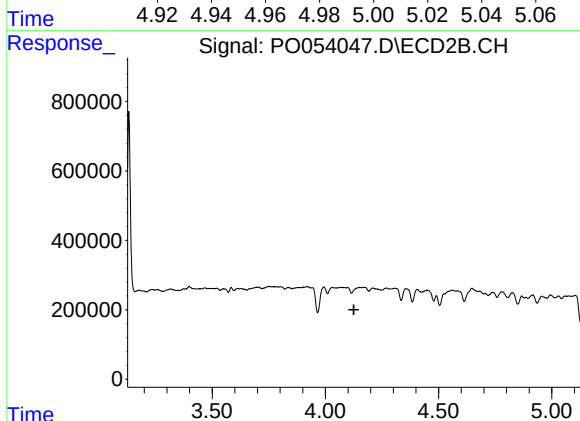


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.126 min
Response: 0
Conc: N.D.

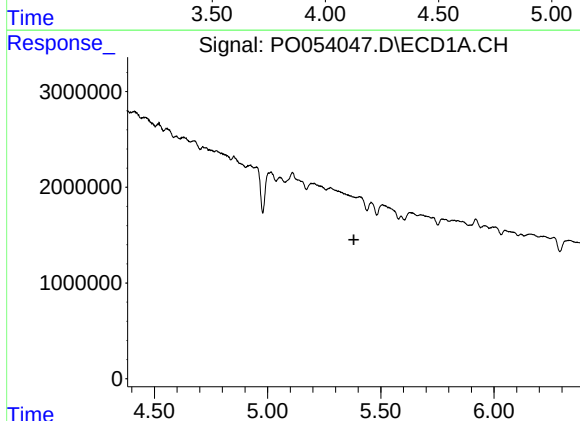


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.381 min
Response: 0
Conc: N.D.

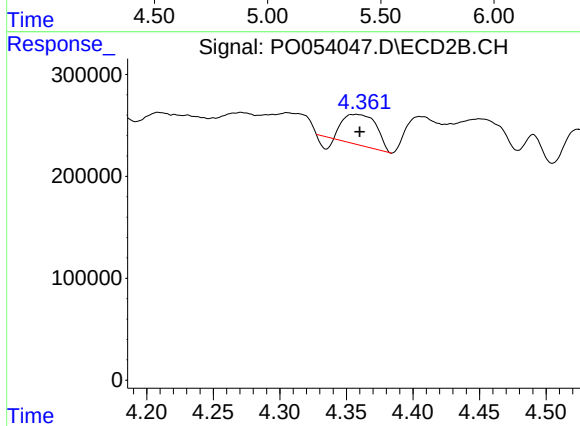

#14 AR-1232-4


R.T.: 4.357 min
Delta R.T.: -0.002 min
Response: 489822
Conc: 159.76 ng/ml

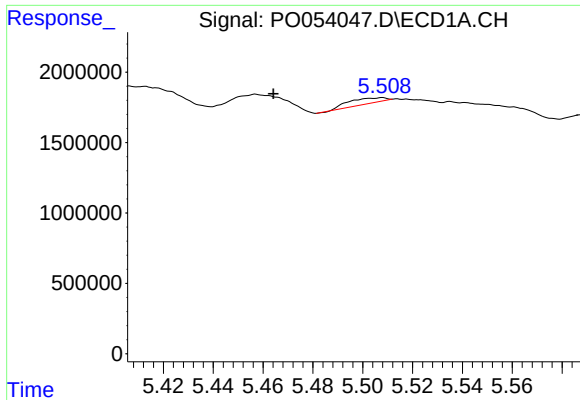

#15 AR-1232-5


R.T.: 5.508 min
Delta R.T.: 0.044 min
Response: 393230
Conc: 30.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-26

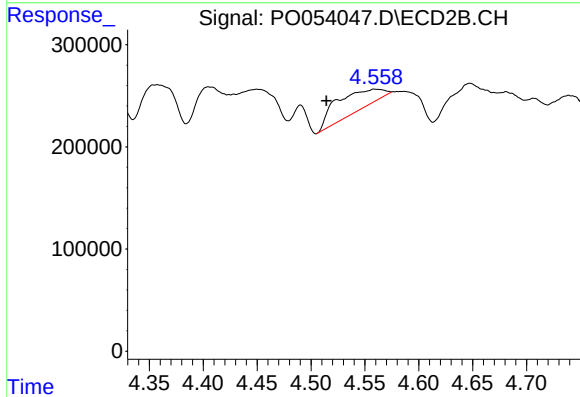


#15 AR-1232-5

R.T.: 4.559 min
Delta R.T.: 0.045 min
Response: 561495
Conc: 159.42 ng/ml

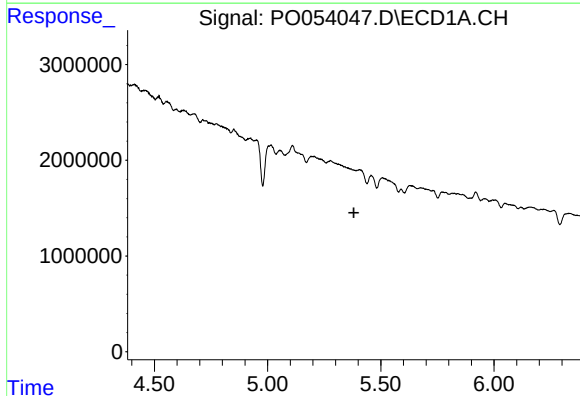


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.381 min
Response: 0
Conc: N.D.

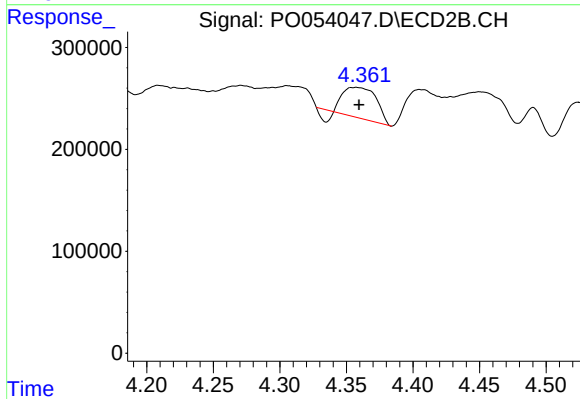

#19 AR-1242-4


R.T.: 4.357 min
Delta R.T.: -0.002 min
Response: 489822
Conc: 73.46 ng/ml

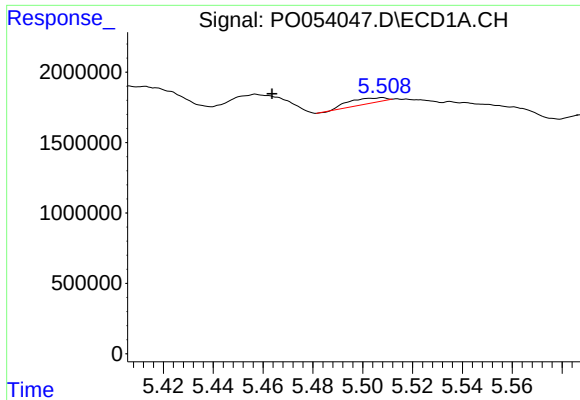

#22 AR-1248-2


R.T.: 5.508 min
Delta R.T.: 0.044 min
Response: 393230
Conc: 7.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-26

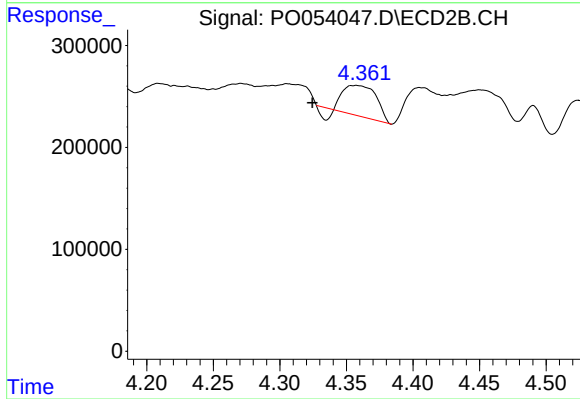


#22 AR-1248-2

R.T.: 4.357 min
Delta R.T.: 0.033 min
Response: 489822
Conc: 51.91 ng/ml

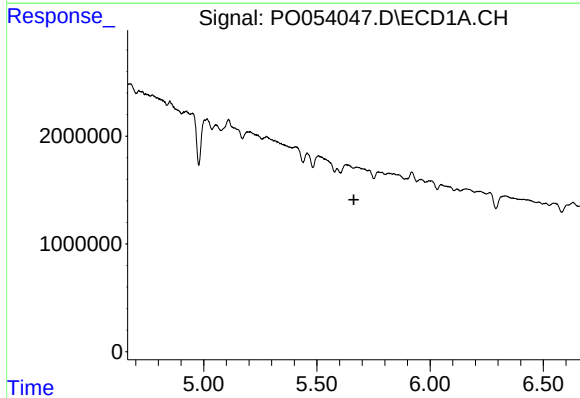


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.663 min
Response: 0
Conc: N.D.

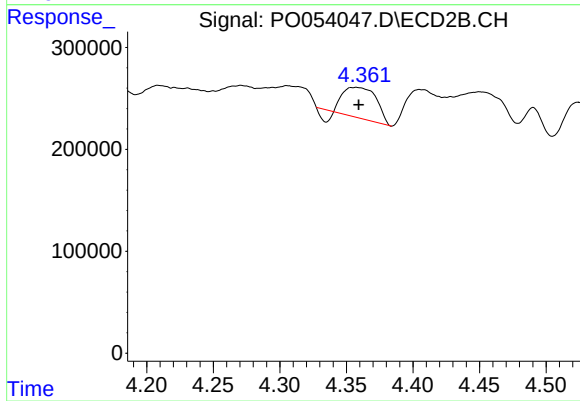

#23 AR-1248-3


R.T.: 4.357 min
Delta R.T.: -0.002 min
Response: 489822
Conc: 50.87 ng/ml

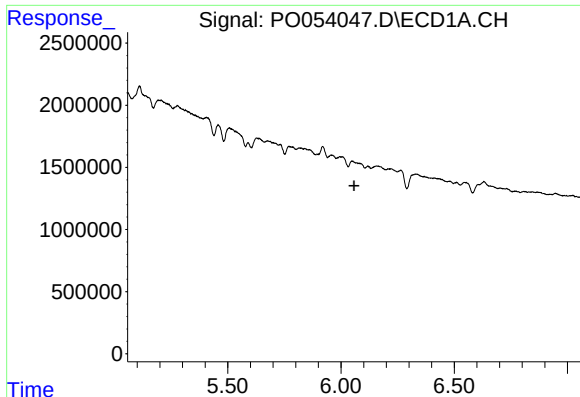

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 6.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26

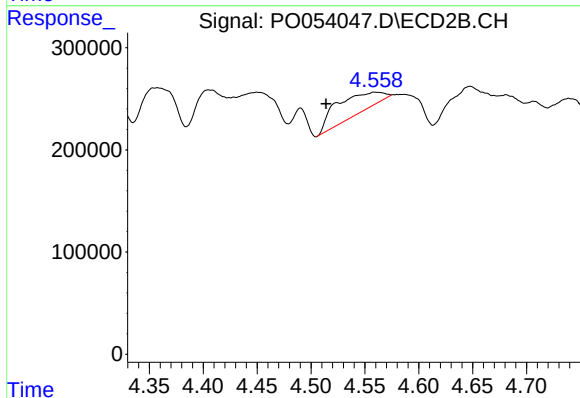


#24 AR-1248-4

R.T.: 4.559 min
Delta R.T.: 0.045 min
Response: 561495
Conc: 46.69 ng/ml

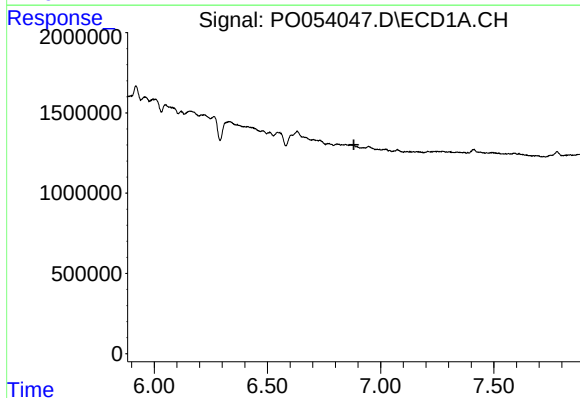


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

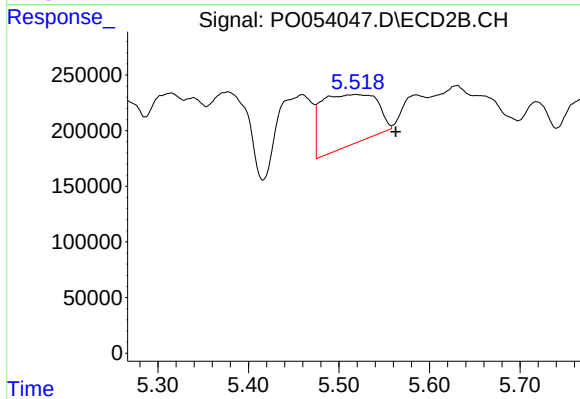

#29 AR-1254-4


R.T.: 5.518 min
Delta R.T.: -0.045 min
Response: 1956381
Conc: 45.09 ng/ml

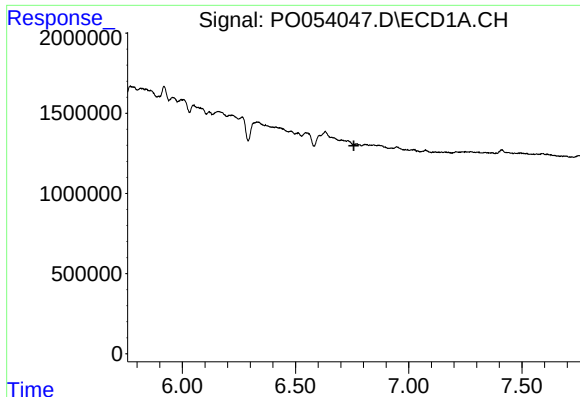

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26

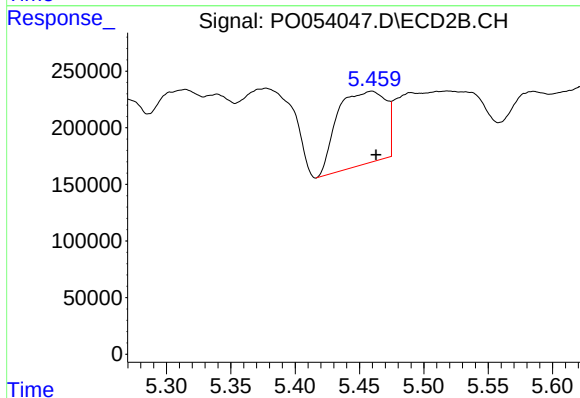


#31 AR-1260-1

R.T.: 5.460 min
Delta R.T.: -0.003 min
Response: 1685754
Conc: 88.33 ng/ml

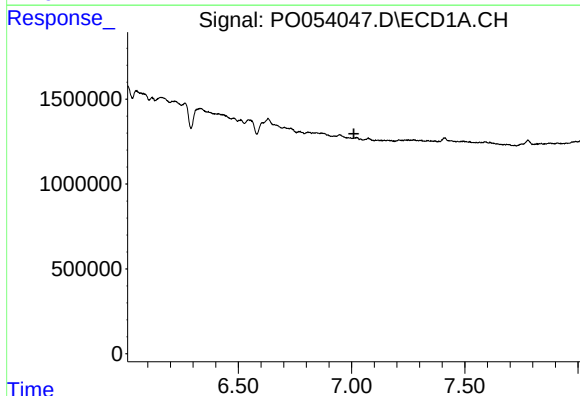


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.010 min
Response: 0
Conc: N.D.

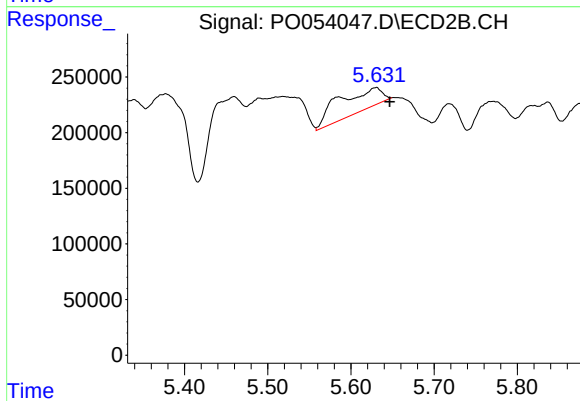

#32 AR-1260-2


R.T.: 5.630 min
Delta R.T.: -0.016 min
Response: 719447
Conc: 30.79 ng/ml

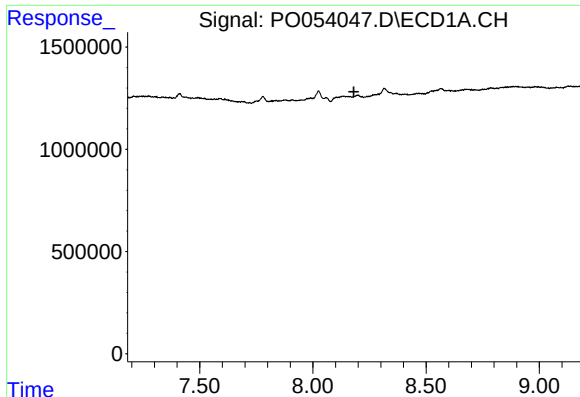

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26

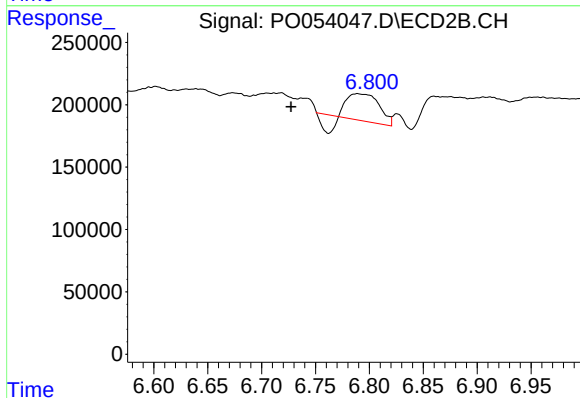


#38 AR-1262-3

R.T.: 6.789 min
Delta R.T.: 0.062 min
Response: 380226
Conc: 24.04 ng/ml

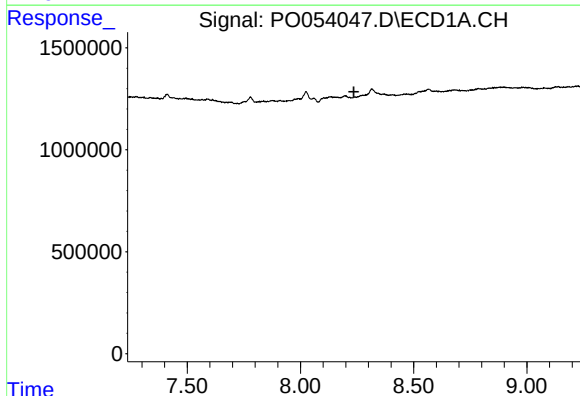


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.236 min
Response: 0
Conc: N.D.

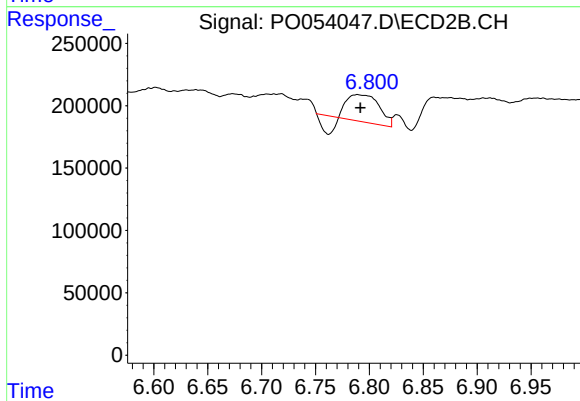

#39 AR-1262-4


R.T.: 6.789 min
Delta R.T.: -0.003 min
Response: 380226
Conc: 12.98 ng/ml

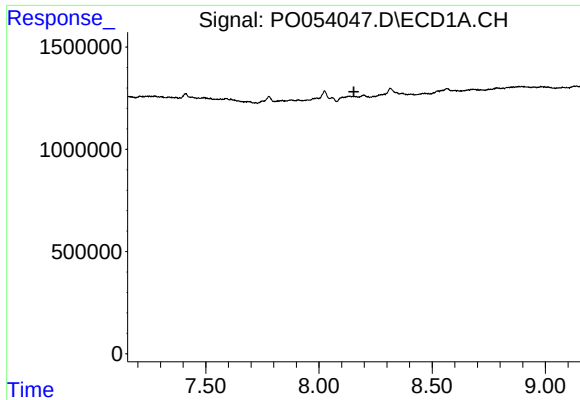

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26

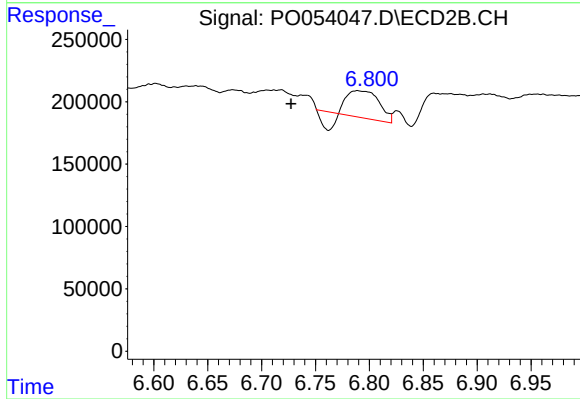


#41 AR-1268-1

R.T.: 6.789 min
Delta R.T.: 0.062 min
Response: 380226
Conc: 8.34 ng/ml

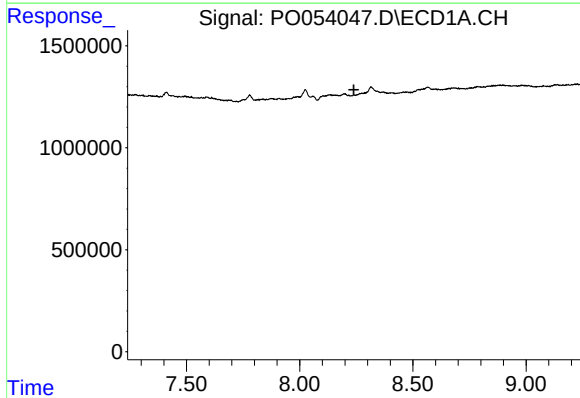

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.239 min
Response: 0
Conc: N.D.

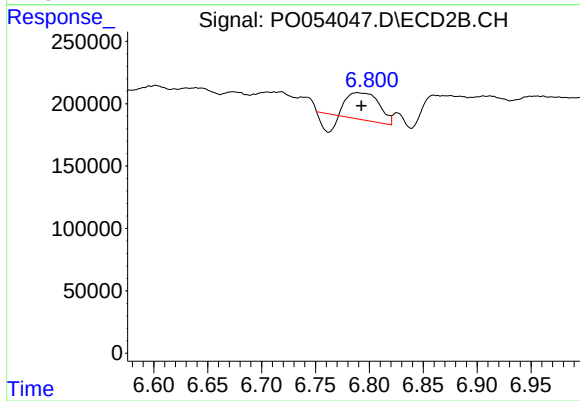

#42 AR-1268-2

R.T.: 6.789 min
Delta R.T.: -0.004 min
Response: 380226
Conc: 8.87 ng/ml