

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
 Data File : P0054026.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2019 12:42
 Operator : SM/SJ
 Sample : K1572-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Sohil
 2/26/2019 10:08:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 02:13:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.054	3.132	6276930	743421	2.093m	2.786 #
2) SA Decachlor...	9.401	7.716	3041824	821582	2.422	2.742m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
Data File : P0054026.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 12:42
Operator : SM/SJ
Sample : K1572-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Sohil
2/26/2019 10:08:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:13:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

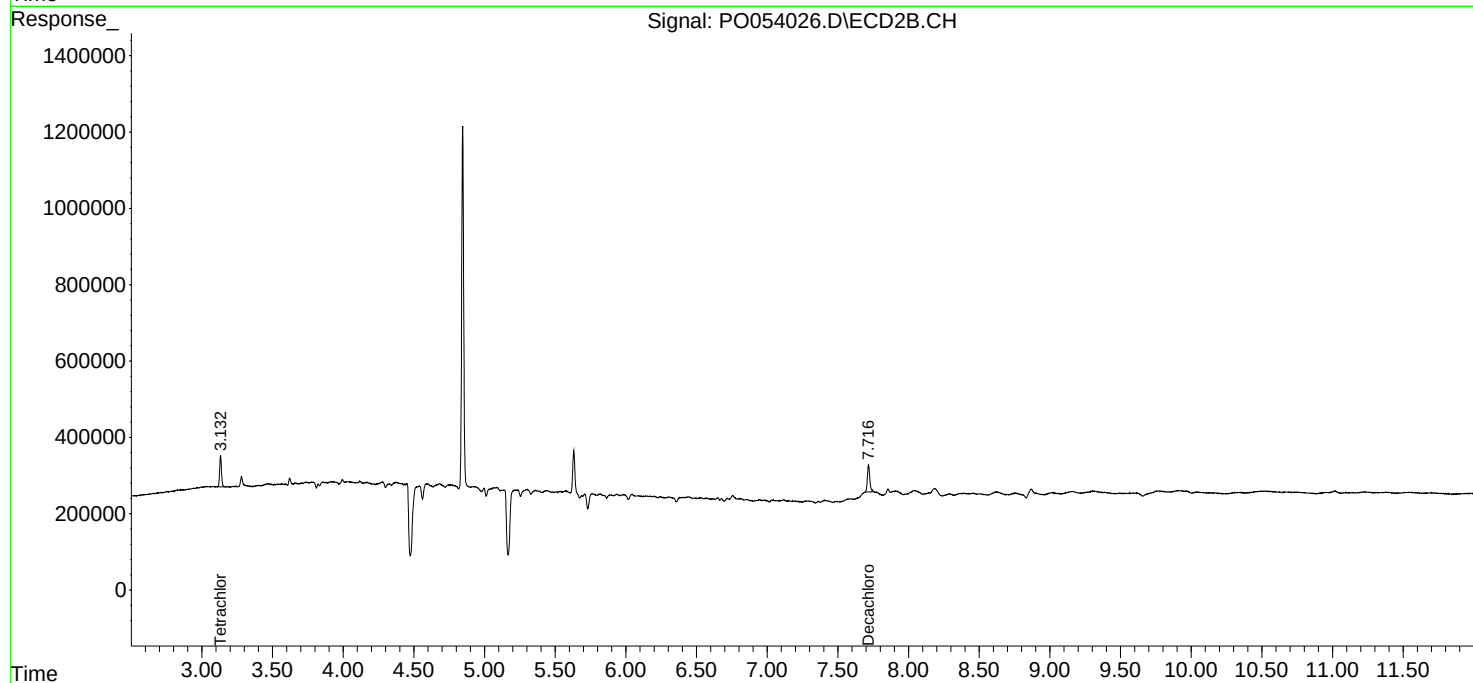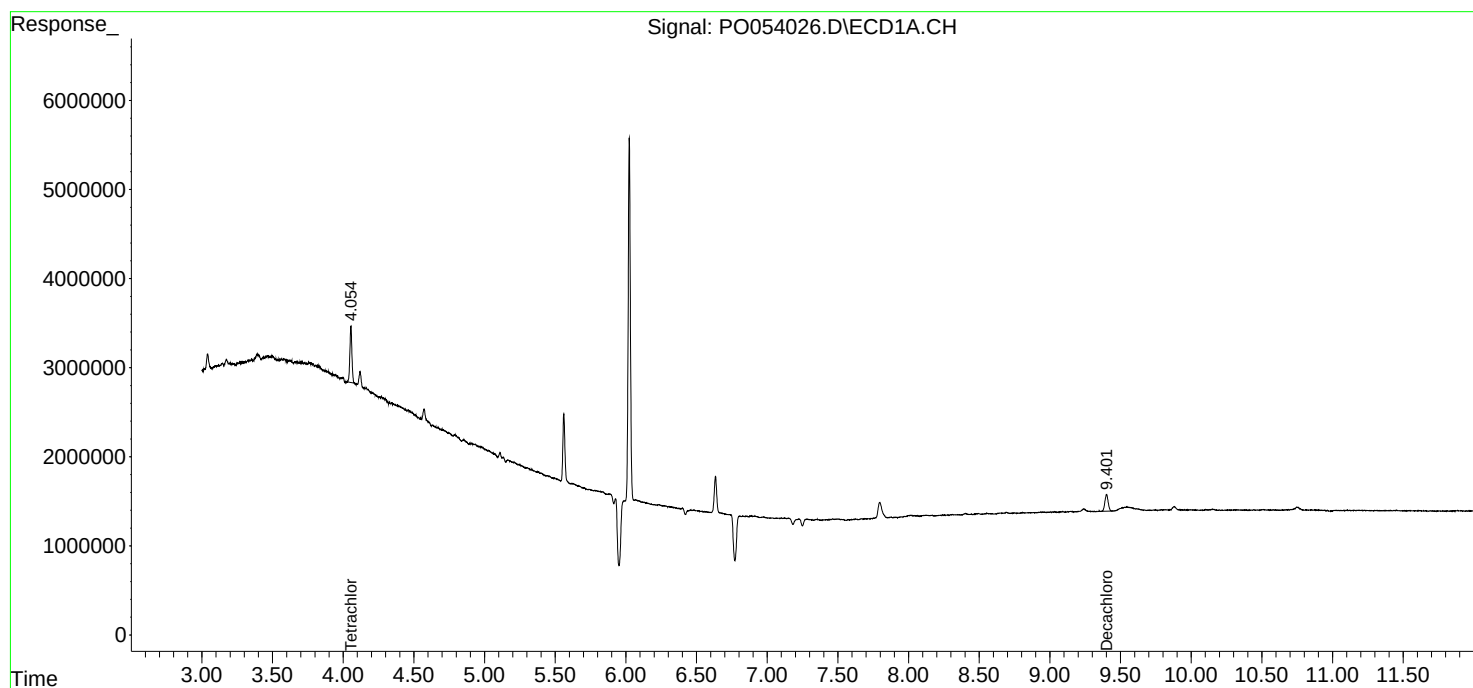

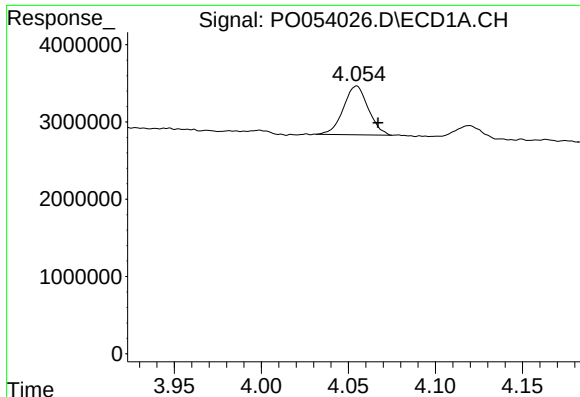


#1 Tetrachloro-m-xylene

R.T.: 4.054 min
Delta R.T.: -0.013 min
Response: 6276930
Conc: 2.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Sohil
2/26/2019 10:08:01 AM

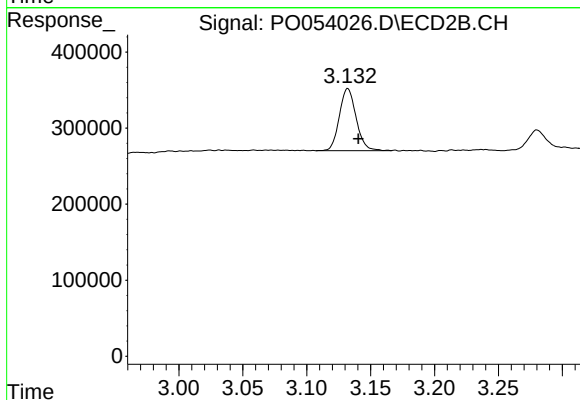


#1 Tetrachloro-m-xylene

R.T.: 3.132 min
Delta R.T.: -0.008 min
Response: 743421
Conc: 2.79 ng/ml

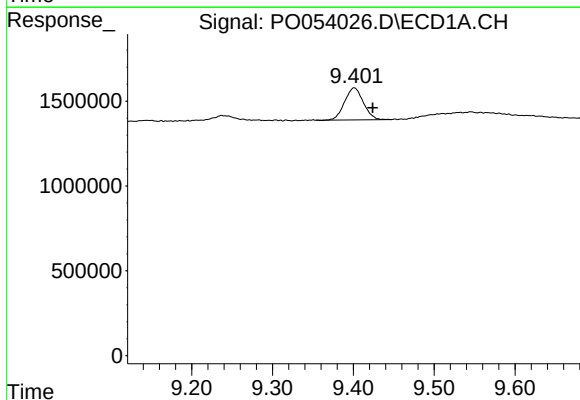

#2 Decachlorobiphenyl

R.T.: 9.401 min
Delta R.T.: -0.023 min
Response: 3041824
Conc: 2.42 ng/ml

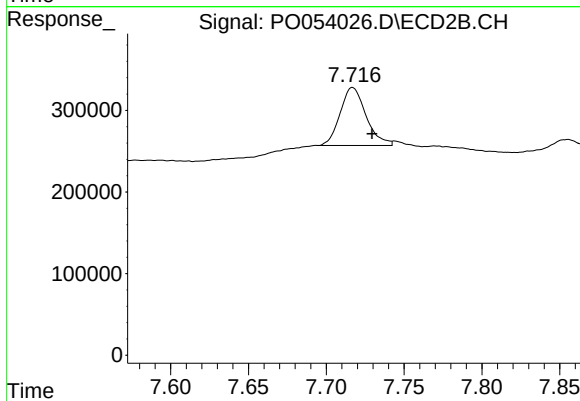

#2 Decachlorobiphenyl

R.T.: 7.716 min
Delta R.T.: -0.013 min
Response: 821582
Conc: 2.74 ng/ml m