

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
 Data File : P0054031.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2019 16:00
 Operator : SM/SJ
 Sample : K1348-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-022219-A

Manual Integrations
 APPROVED

Sohil
 2/26/2019 10:07:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 02:15:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.055	3.132	55680982	5769041	18.567m	21.620
2) SA Decachlor...	9.400	7.715	17400311	3895824	13.857	13.001

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022519\
Data File : PO054031.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 16:00
Operator : SM/SJ
Sample : K1348-03
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-03-022219-A


Manual Integrations
APPROVED

Sohil
2/26/2019 10:07:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:15:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

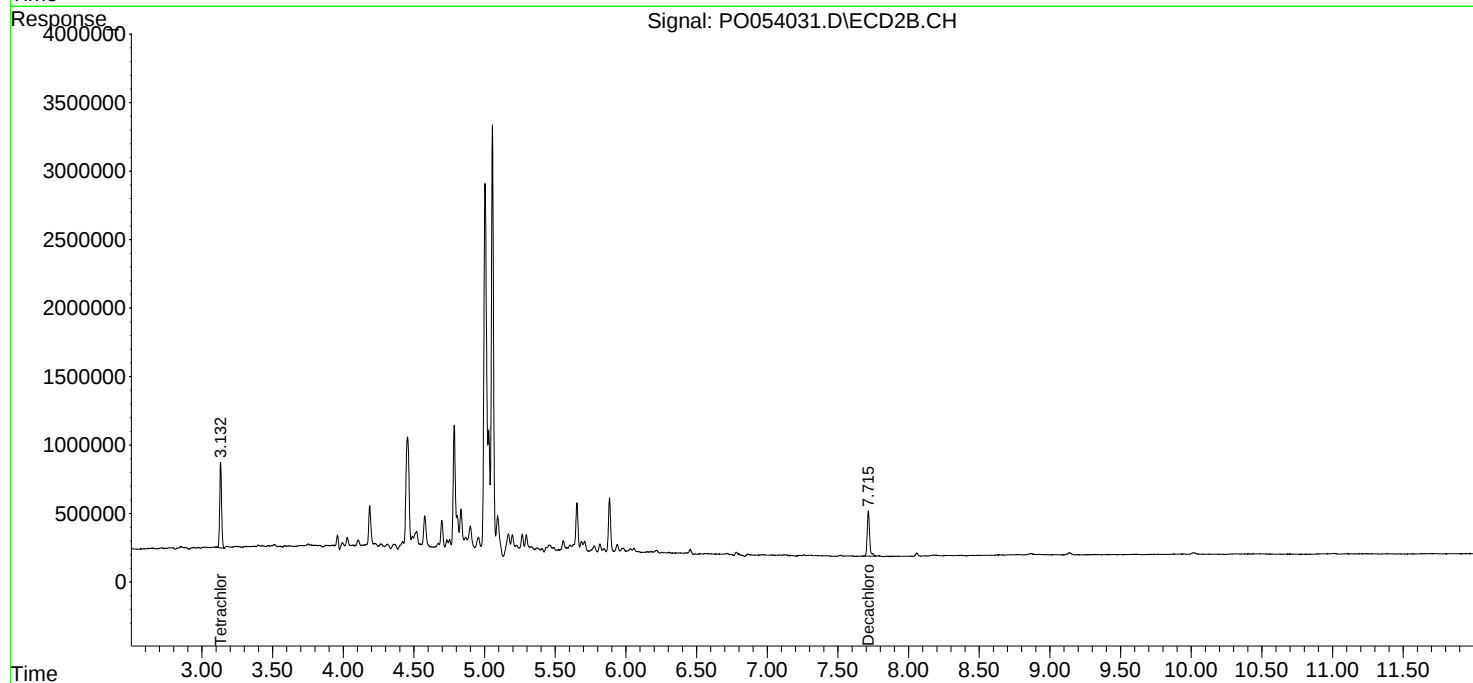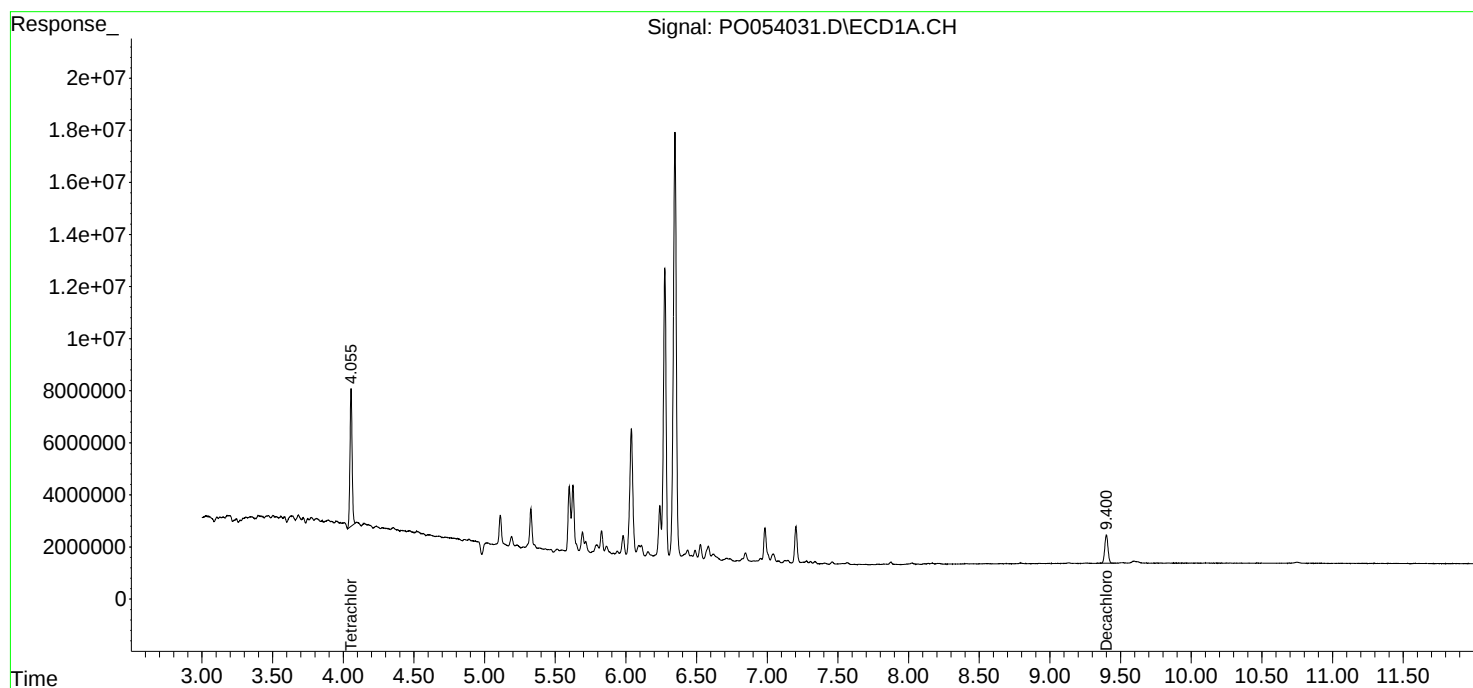

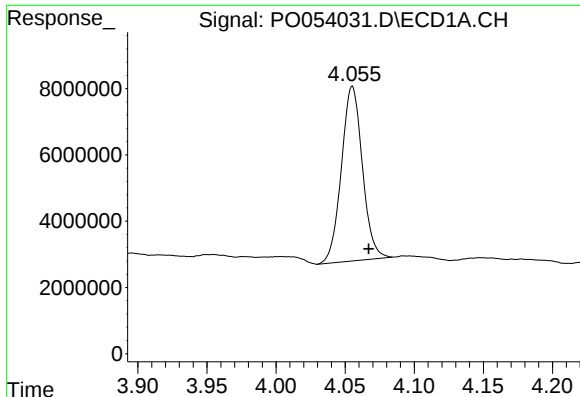


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: -0.012 min
Response: 55680982
Conc: 18.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-03-022219-A


Manual Integrations
APPROVED

Sohil
2/26/2019 10:07:33 AM

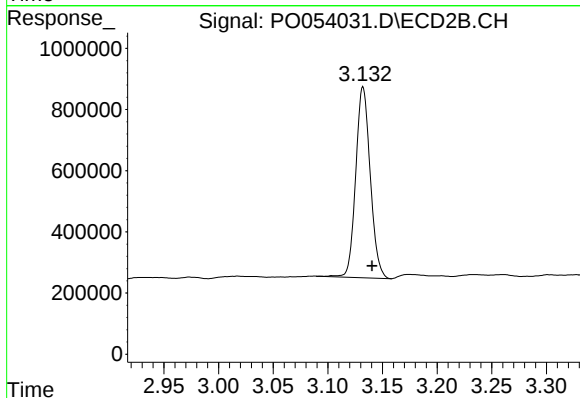


#1 Tetrachloro-m-xylene

R.T.: 3.132 min
Delta R.T.: -0.008 min
Response: 5769041
Conc: 21.62 ng/ml

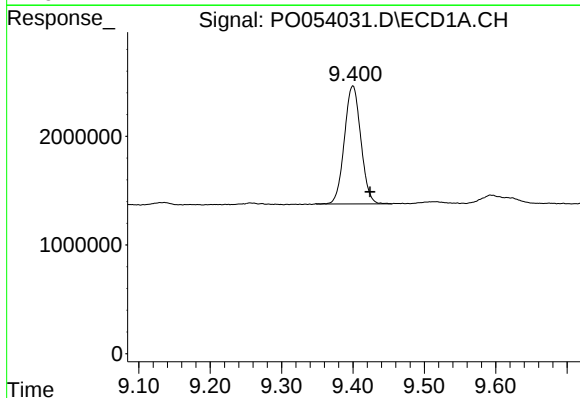

#2 Decachlorobiphenyl

R.T.: 9.400 min
Delta R.T.: -0.024 min
Response: 17400311
Conc: 13.86 ng/ml

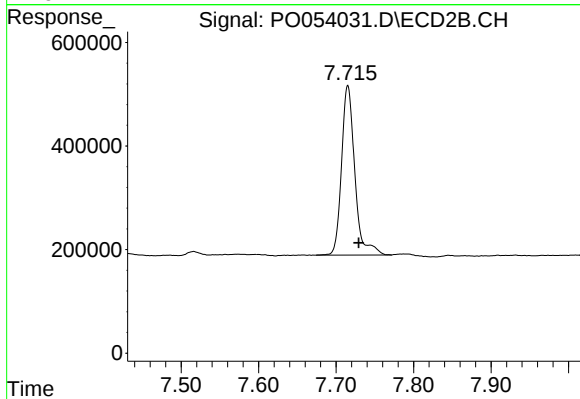

#2 Decachlorobiphenyl

R.T.: 7.715 min
Delta R.T.: -0.014 min
Response: 3895824
Conc: 13.00 ng/ml