

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
Data File : P0054032.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 16:17
Operator : SM/SJ
Sample : K1348-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-022219-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:16:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.054	3.133	50171075	5472803	16.729	20.510
2) SA Decachlor...	9.399	7.716	13913255	2891191	11.080	9.648

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
Data File : P0054032.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 16:17
Operator : SM/SJ
Sample : K1348-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-03-022219-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:16:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

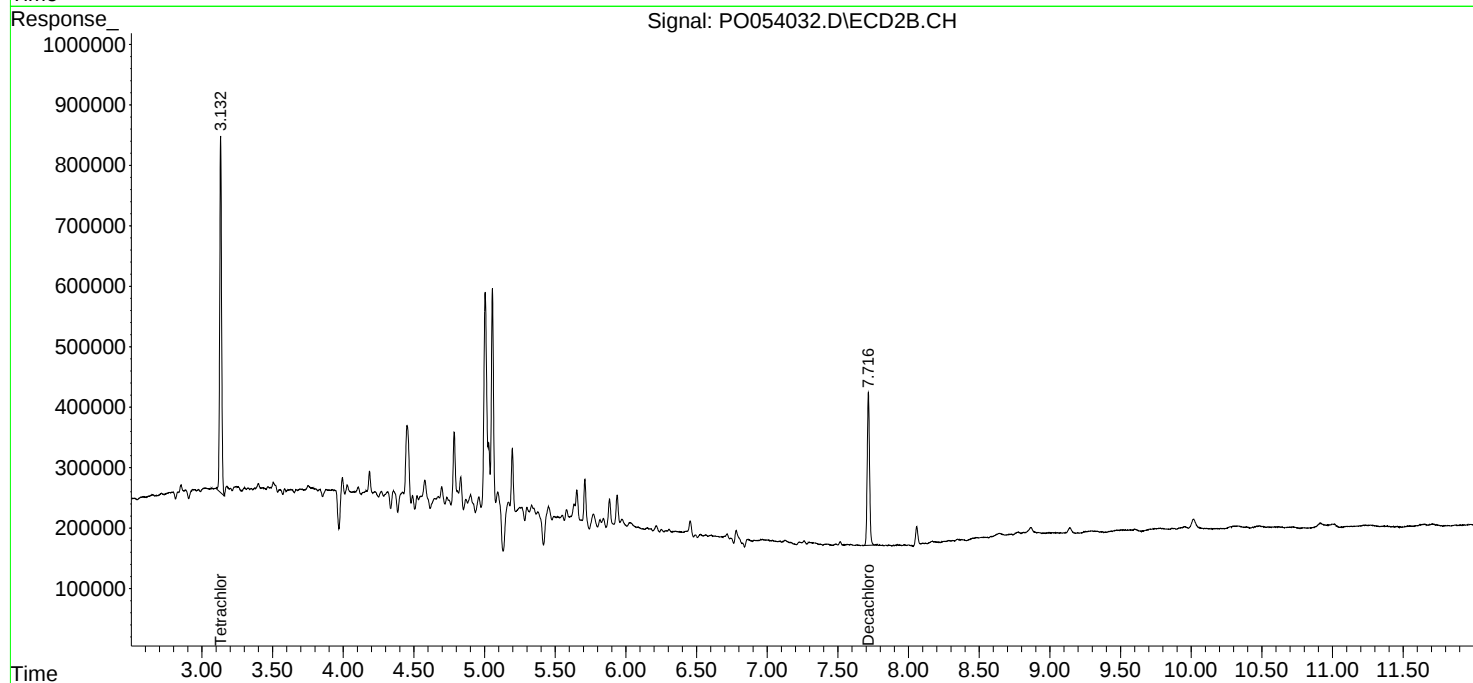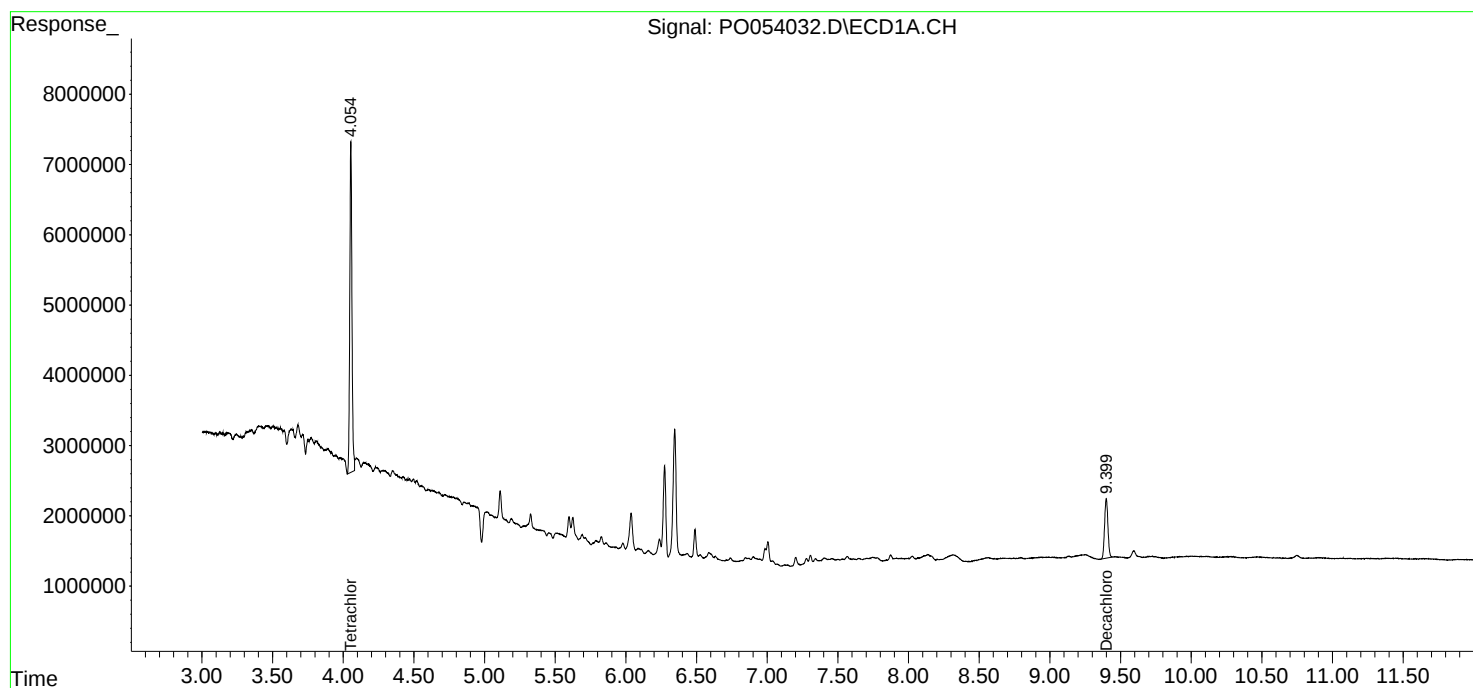


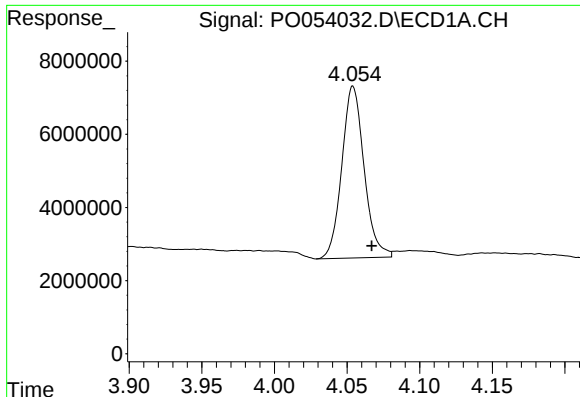

#1 Tetrachloro-m-xylene


R.T.: 4.054 min
Delta R.T.: -0.013 min
Response: 50171075
Conc: 16.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-03-022219-B

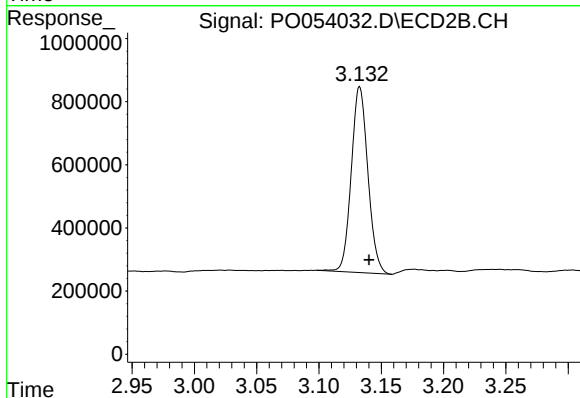


#1 Tetrachloro-m-xylene

R.T.: 3.133 min
Delta R.T.: -0.008 min
Response: 5472803
Conc: 20.51 ng/ml

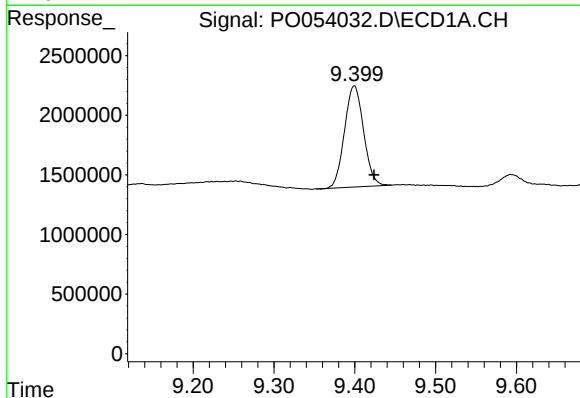

#2 Decachlorobiphenyl

R.T.: 9.399 min
Delta R.T.: -0.025 min
Response: 13913255
Conc: 11.08 ng/ml

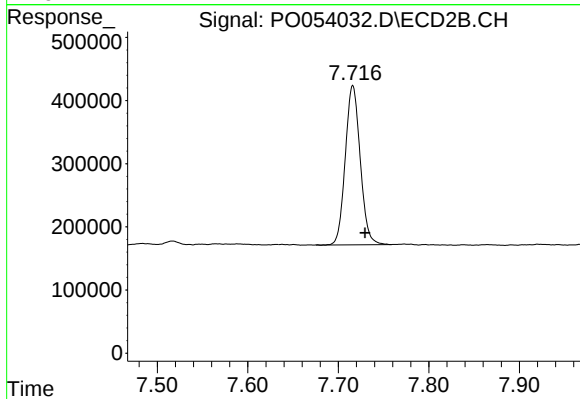

#2 Decachlorobiphenyl

R.T.: 7.716 min
Delta R.T.: -0.013 min
Response: 2891191
Conc: 9.65 ng/ml