

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
 Data File : P0054045.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2019 19:56
 Operator : SM/SJ
 Sample : K1596-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-15

Manual Integrations
 APPROVED

Sohil
 2/28/2019 1:57:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 02:23:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.053	3.132	48837018	5398689	16.285	20.232
2) SA Decachlor...	9.396	7.714	15151726	3227260	12.066m	10.770

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
Data File : P0054045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 19:56
Operator : SM/SJ
Sample : K1596-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-15


Manual Integrations
APPROVED

Sohil
2/28/2019 1:57:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:23:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

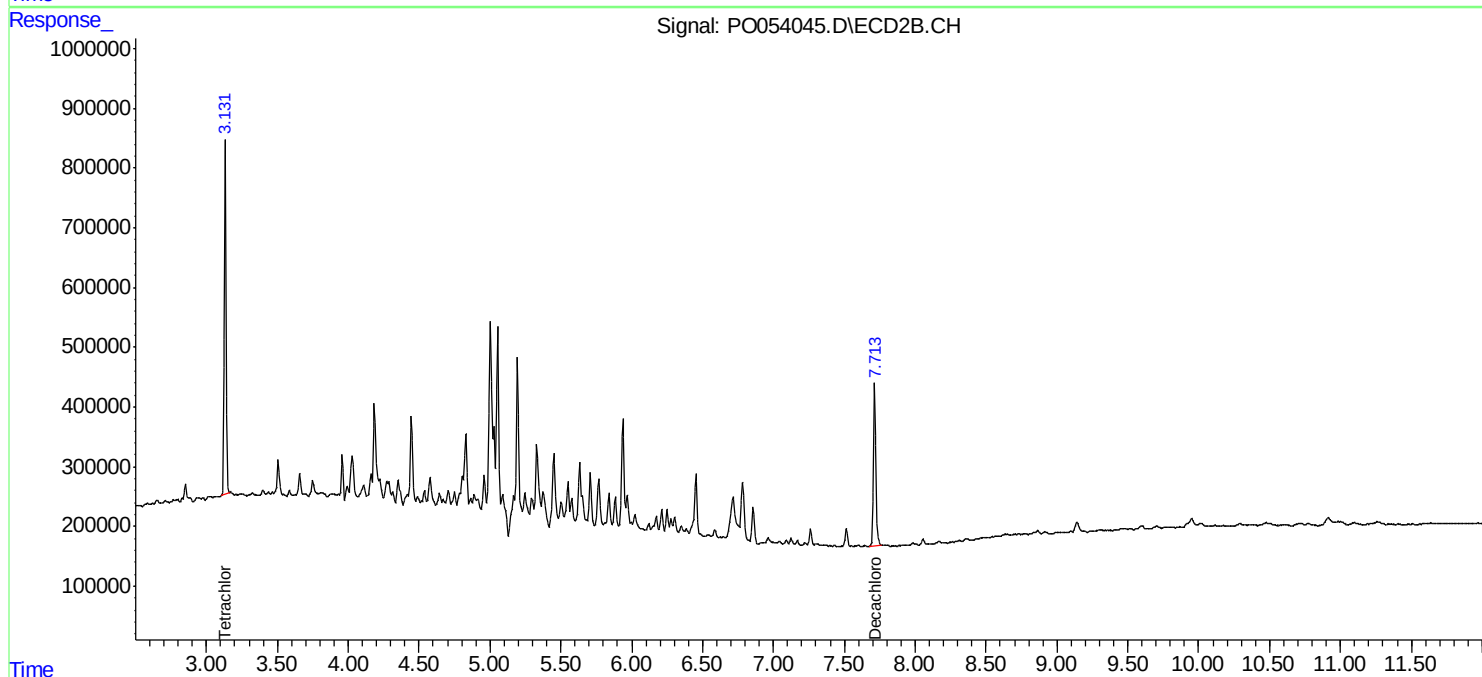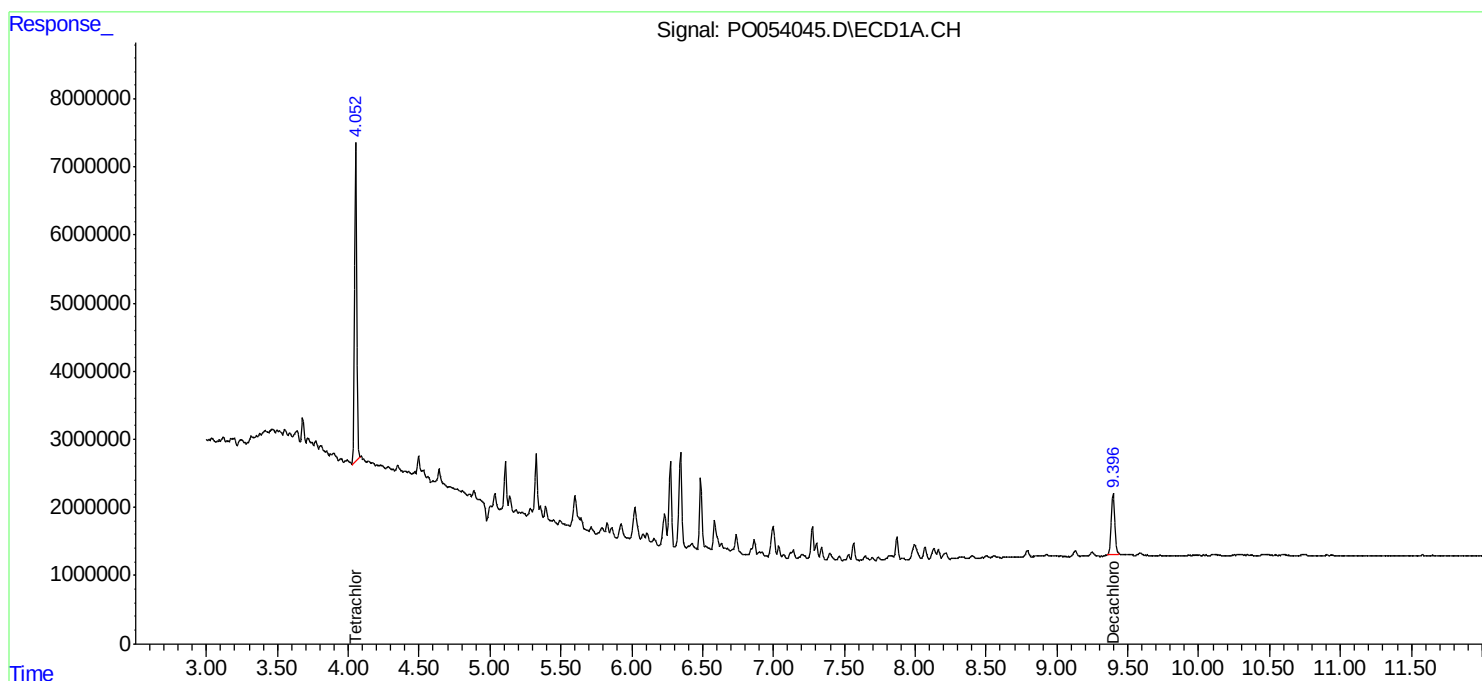

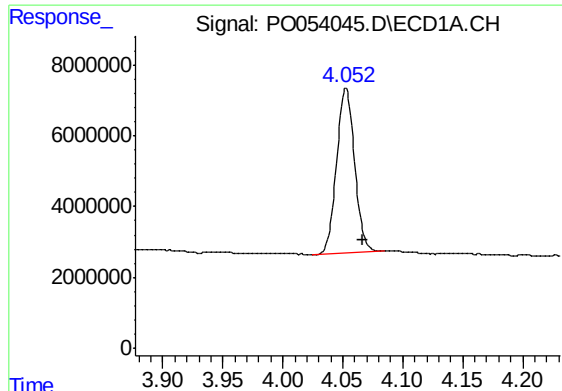


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.014 min
Response: 48837018
Conc: 16.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-15


Manual Integrations
APPROVED

Sohil
2/28/2019 1:57:18 PM

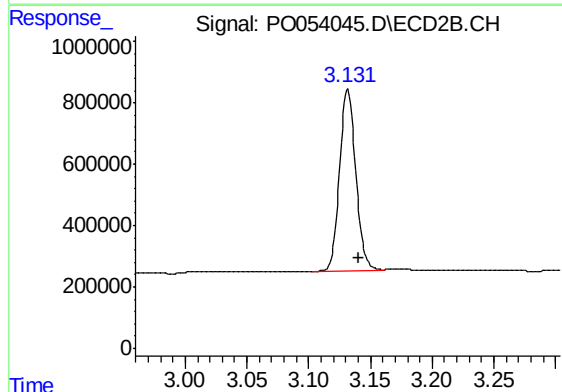


#1 Tetrachloro-m-xylene

R.T.: 3.132 min
Delta R.T.: -0.009 min
Response: 5398689
Conc: 20.23 ng/ml

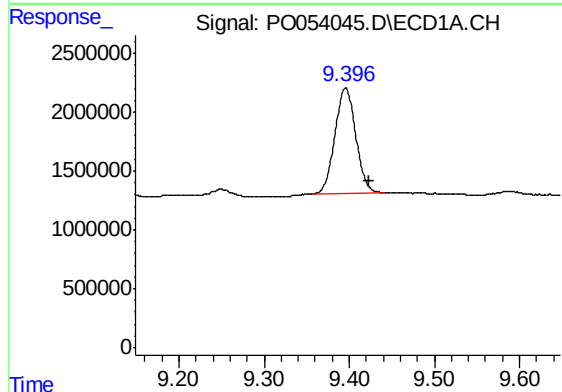

#2 Decachlorobiphenyl

R.T.: 9.396 min
Delta R.T.: -0.028 min
Response: 15151726
Conc: 12.07 ng/ml m

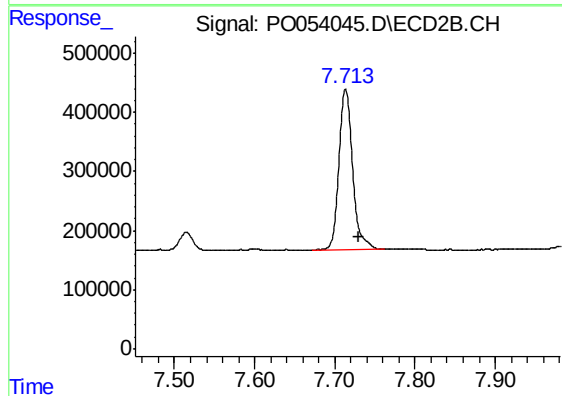

#2 Decachlorobiphenyl

R.T.: 7.714 min
Delta R.T.: -0.016 min
Response: 3227260
Conc: 10.77 ng/ml