

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
 Data File : P0054051.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2019 21:38
 Operator : SM/SJ
 Sample : K1597-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 02:26:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 19 03:40:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.051	3.130	51822845	4773701	17.280	17.890
2) SA Decachlor...	9.394	7.711	9479364	2423268	7.549	8.087

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022519\
Data File : P0054051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2019 21:38
Operator : SM/SJ
Sample : K1597-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 02:26:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0021819.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 19 03:40:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

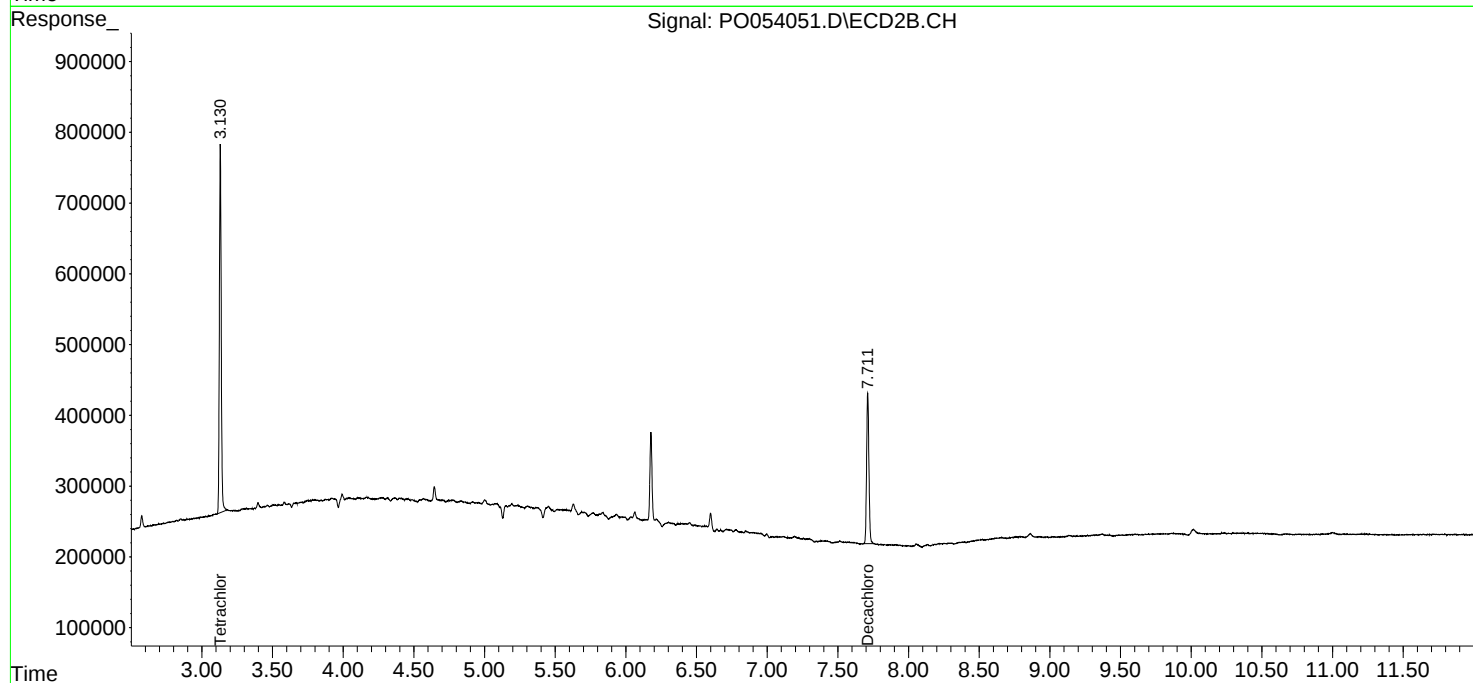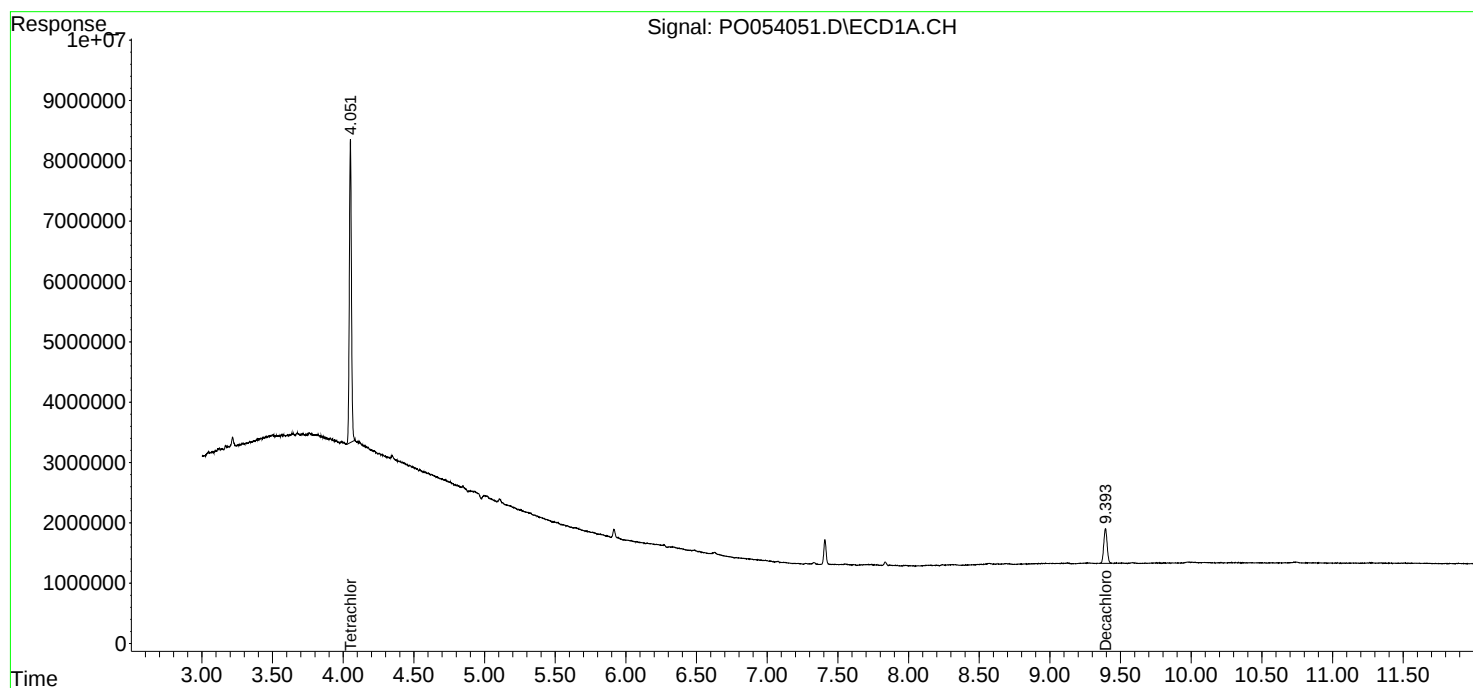


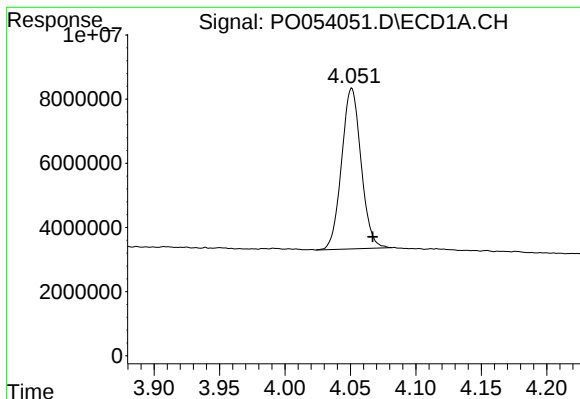

#1 Tetrachloro-m-xylene


R.T.: 4.051 min
Delta R.T.: -0.016 min
Response: 51822845
Conc: 17.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-23

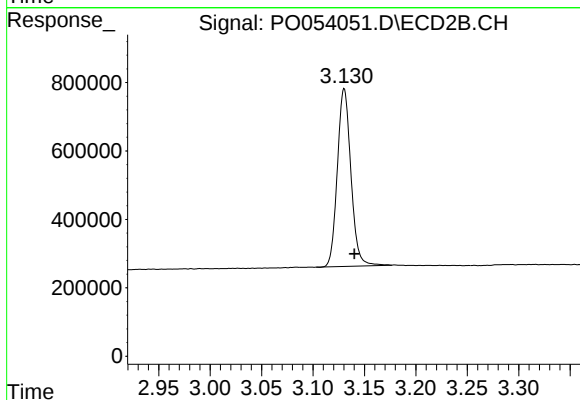


#1 Tetrachloro-m-xylene

R.T.: 3.130 min
Delta R.T.: -0.010 min
Response: 4773701
Conc: 17.89 ng/ml

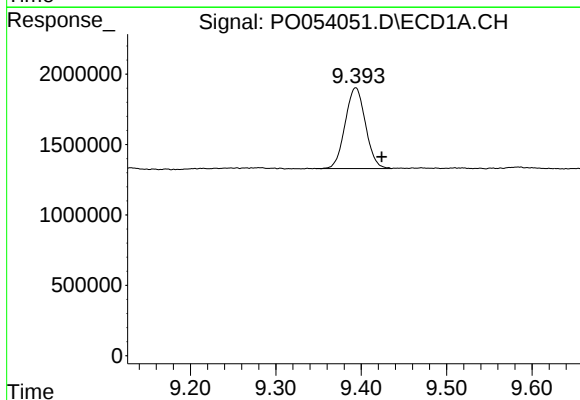

#2 Decachlorobiphenyl

R.T.: 9.394 min
Delta R.T.: -0.030 min
Response: 9479364
Conc: 7.55 ng/ml

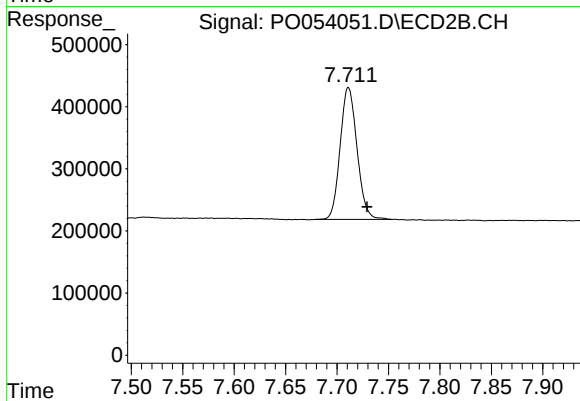

#2 Decachlorobiphenyl

R.T.: 7.711 min
Delta R.T.: -0.018 min
Response: 2423268
Conc: 8.09 ng/ml