

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022520\
 Data File : P0066814.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Feb 2020 14:39
 Operator : DD\AJ
 Sample : L1367-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-022420

Manual Integrations
 APPROVED

Sohil
 2/27/2020 2:34:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 00:36:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 14:58:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.405	913518	1163499	21.740m	21.541
2) SA Decachlor...	9.596	8.289	832935	901238	20.296	16.218

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022520\
Data File : P0066814.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Feb 2020 14:39
Operator : DD\AJ
Sample : L1367-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-022420


Manual Integrations
APPROVED

Sohil
2/27/2020 2:34:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 00:36:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 14:58:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

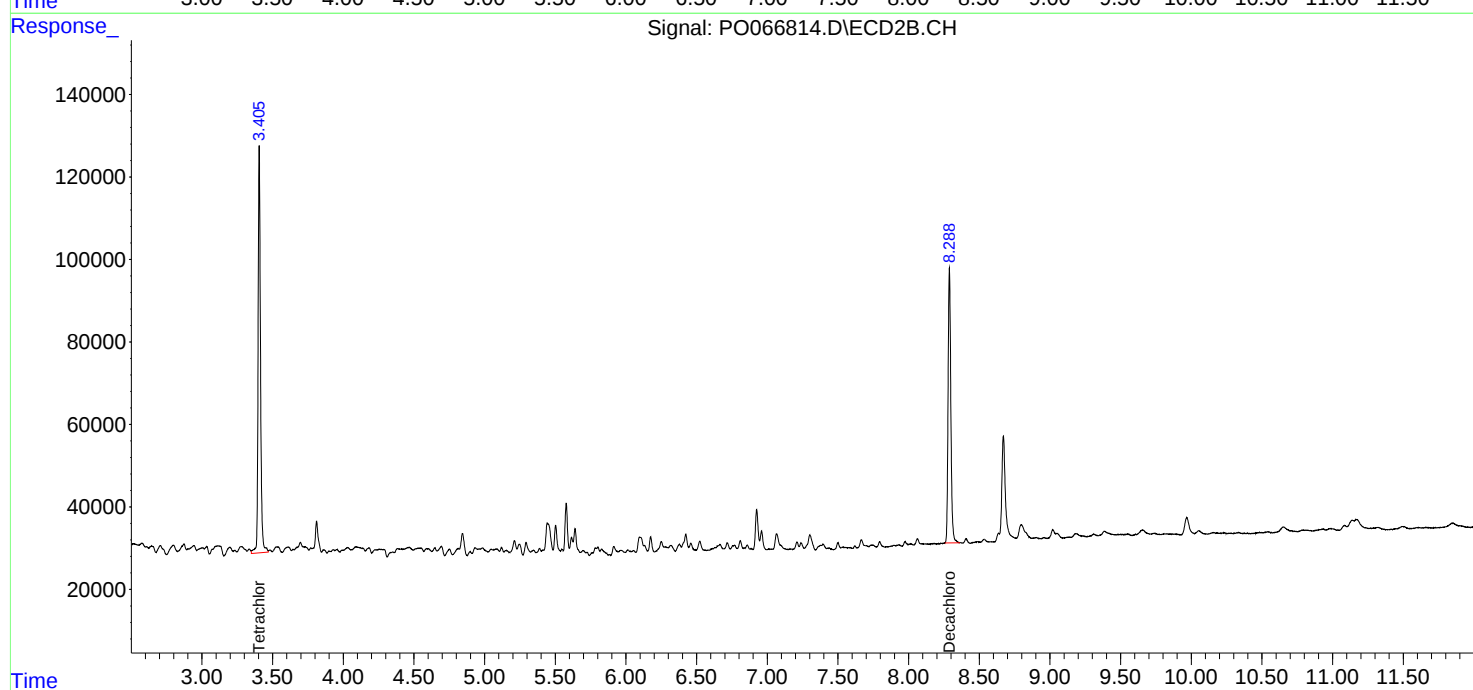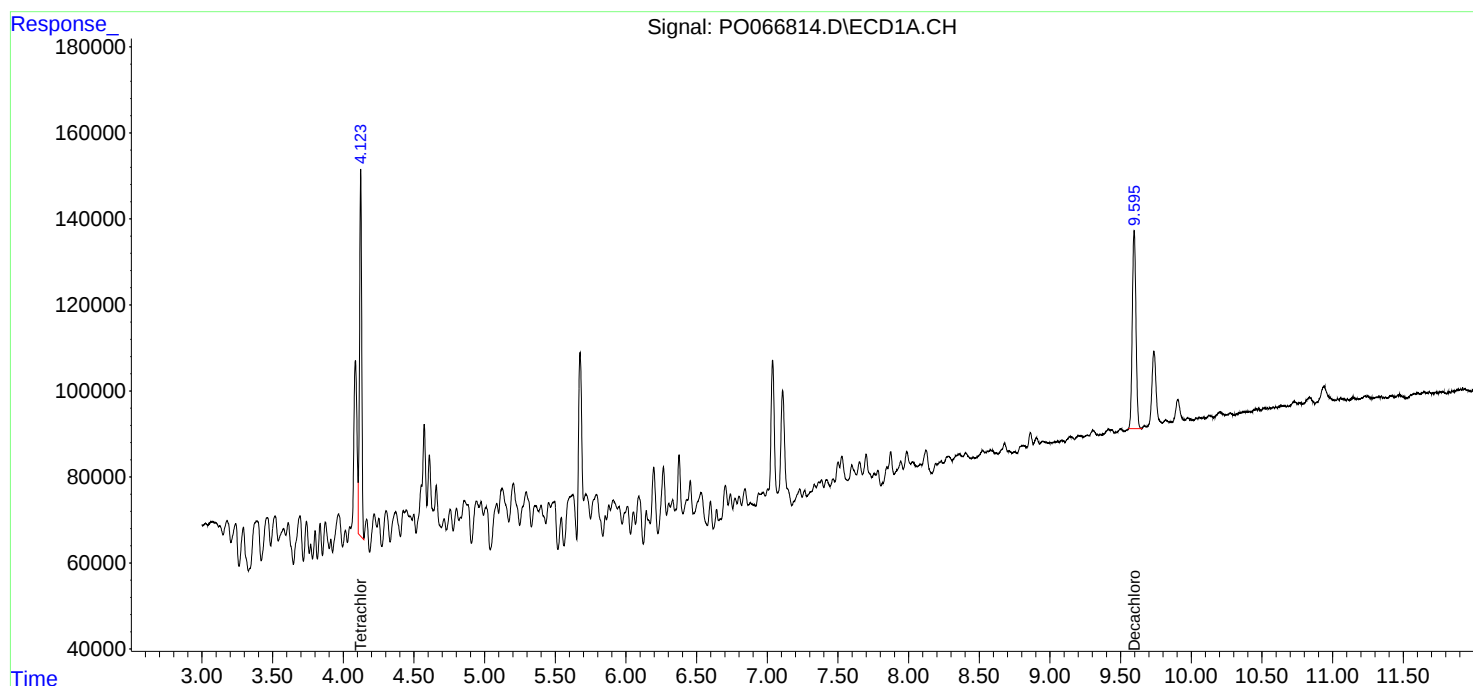

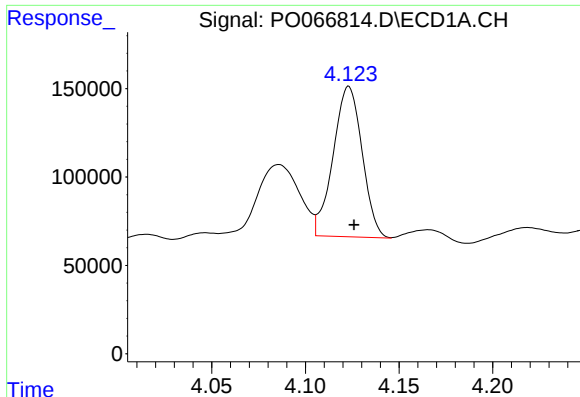


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: -0.003 min
Response: 913518
Conc: 21.74 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-02-022420


Manual Integrations
APPROVED

Sohil
2/27/2020 2:34:52 PM

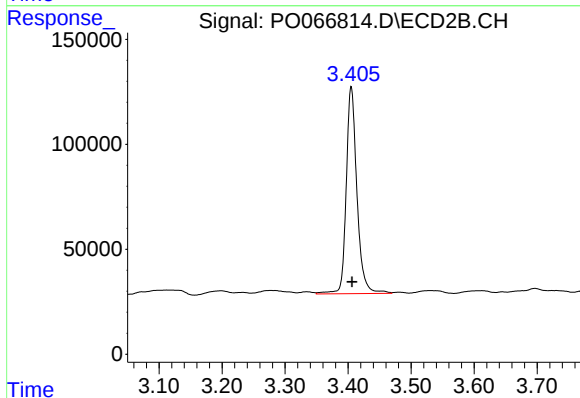


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: -0.002 min
Response: 1163499
Conc: 21.54 ng/ml

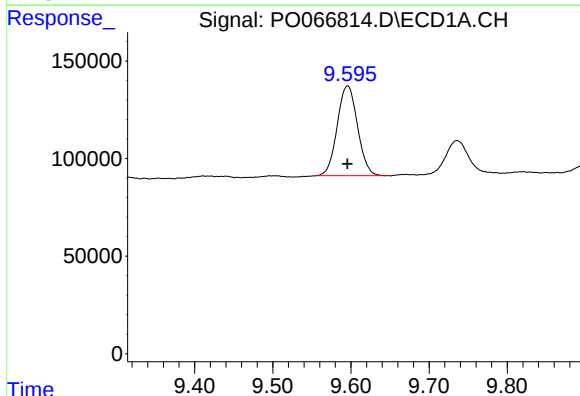

#2 Decachlorobiphenyl

R.T.: 9.596 min
Delta R.T.: 0.000 min
Response: 832935
Conc: 20.30 ng/ml

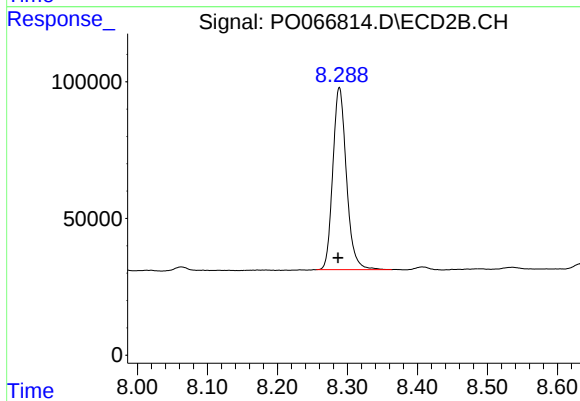

#2 Decachlorobiphenyl

R.T.: 8.289 min
Delta R.T.: 0.002 min
Response: 901238
Conc: 16.22 ng/ml