

Data Path : P:\HPCHEM1\ECD_0\Data\P0022618\
 Data File : P0042632.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Feb 2018 17:27
 Operator : SM/UA
 Sample : J1630-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 BPS1-SB4001-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 00:07:31 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.095	3.343	4818355	9152314	19.451	24.767 #
2)	SA Decachlor...	9.472	8.126	5148713	8125211	20.372	21.070
Target Compounds							
6)	L1 AR-1016-4	0.000	4.828	0	933720	N.D.	84.080 #
20)	L4 AR-1242-5	0.000	4.828	0	933720	N.D.	161.484 #
21)	L5 AR-1248-1	0.000	4.828	0	933720	N.D.	85.412 #
27)	L6 AR-1254-2	6.620	0.000	436843	0	50.227	N.D. #
28)	L6 AR-1254-3	6.620	0.000	436843	0	28.185	N.D. #
29)	L6 AR-1254-4	0.000	5.977	0	1381795	N.D.	70.913 #
32)	L7 AR-1260-2	0.000	5.977	0	1381795	N.D.	41.135 #
36)	L8 AR-1262-1	0.000	5.977	0	1381795	N.D.	62.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO022618\
Data File : PO042632.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2018 17:27
Operator : SM/UA
Sample : J1630-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 00:07:31 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

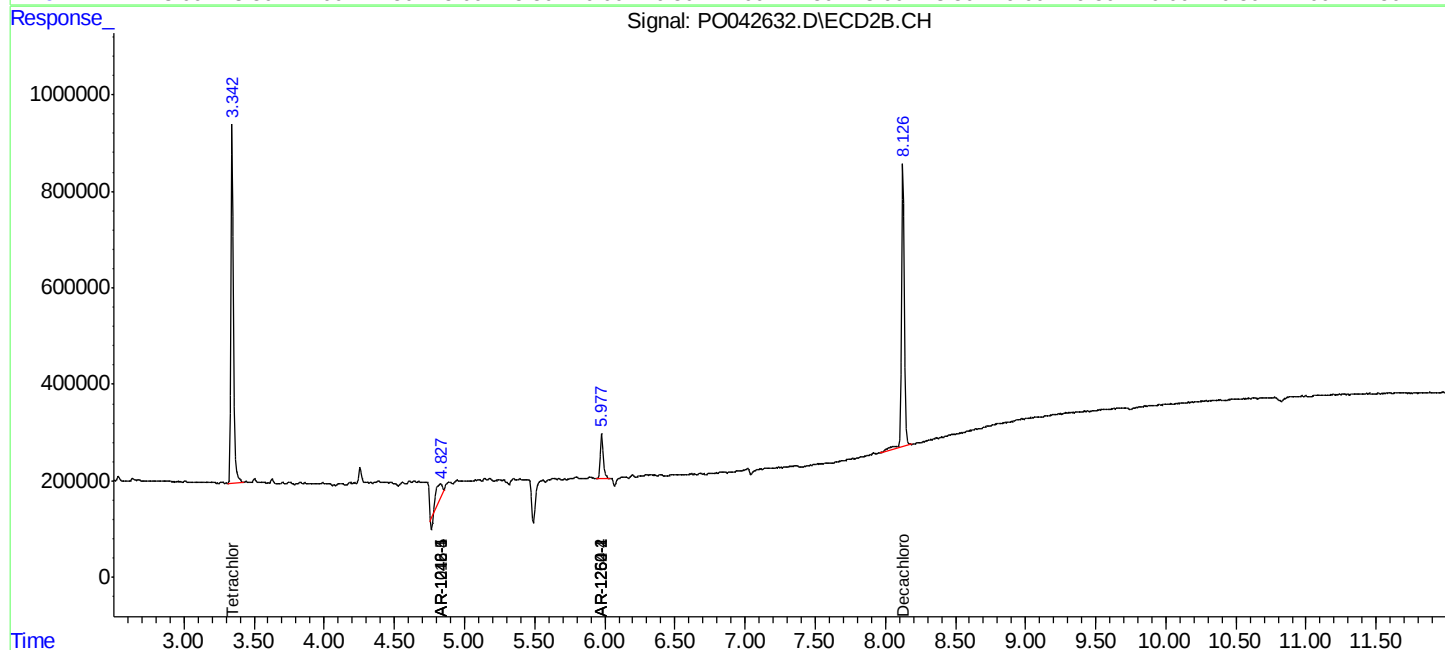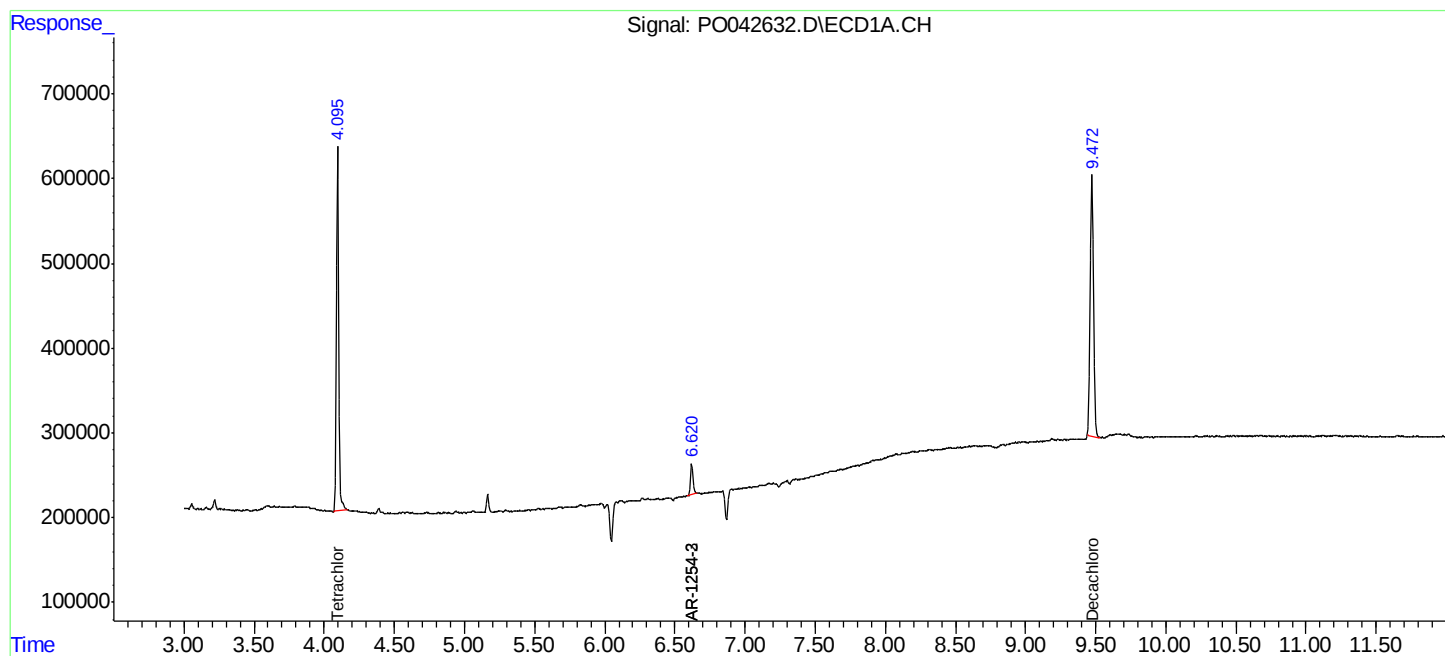


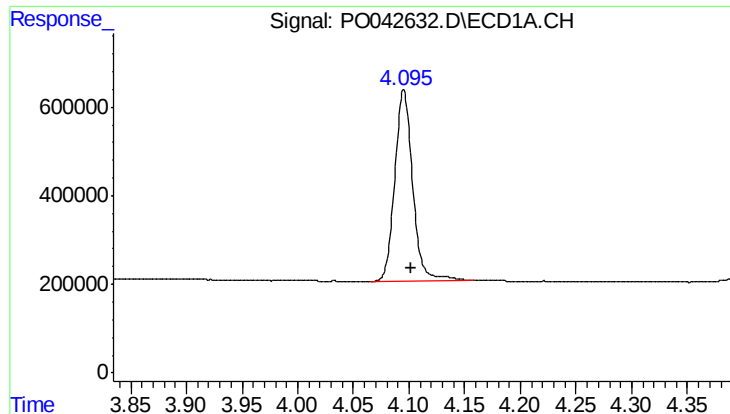

#1 Tetrachloro-m-xylene


R.T.: 4.095 min
Delta R.T.: -0.006 min
Response: 4818355
Conc: 19.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

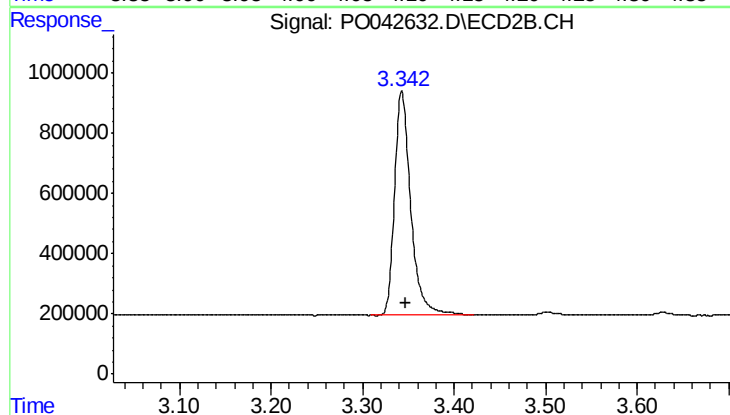


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: -0.005 min
Response: 9152314
Conc: 24.77 ng/ml

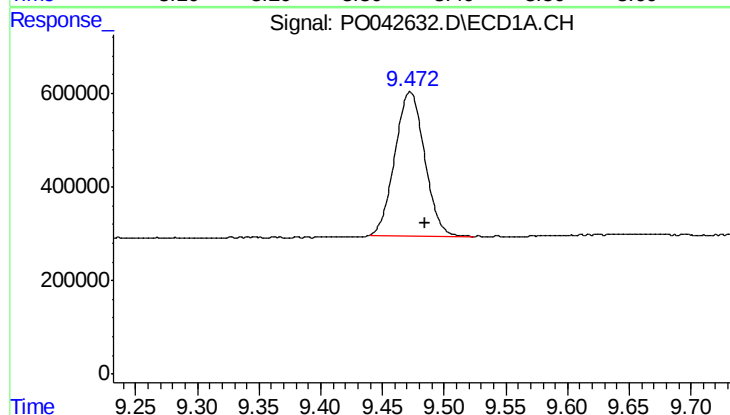


#2 Decachlorobiphenyl

R.T.: 9.472 min
Delta R.T.: -0.012 min
Response: 5148713
Conc: 20.37 ng/ml

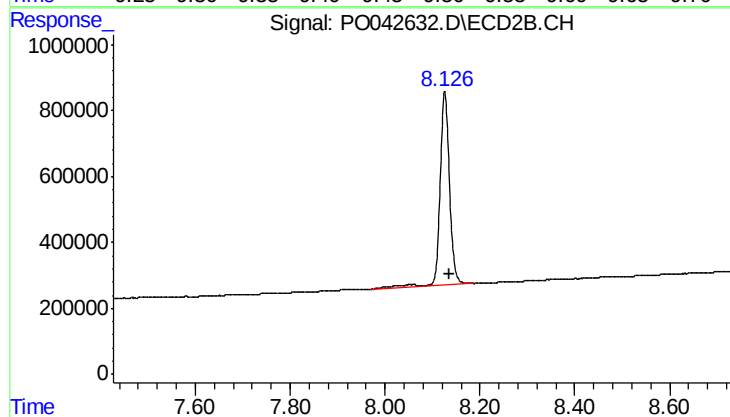

#2 Decachlorobiphenyl


R.T.: 8.126 min
Delta R.T.: -0.011 min
Response: 8125211
Conc: 21.07 ng/ml

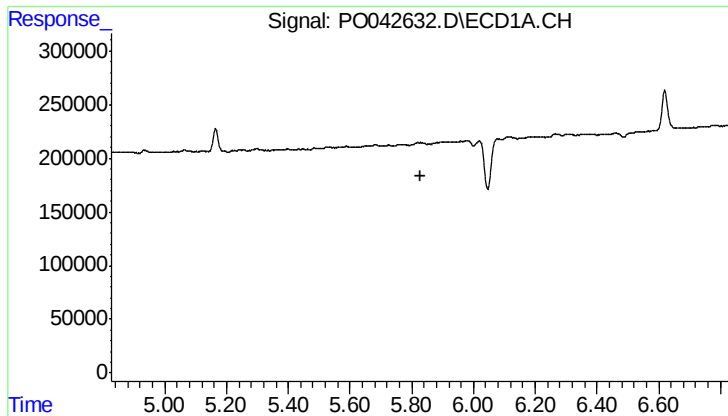

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

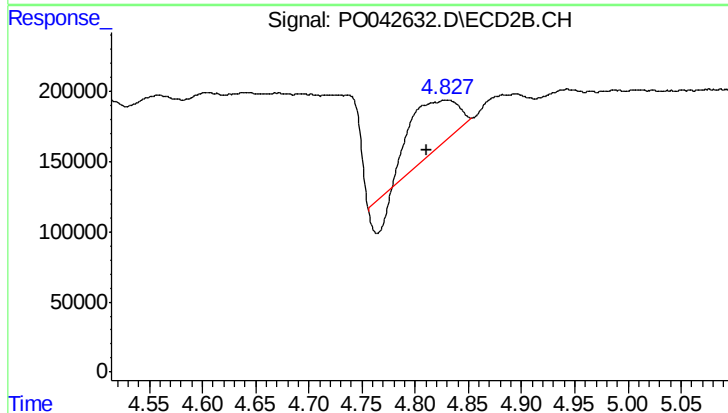


#6 AR-1016-4

R.T.: 4.828 min
Delta R.T.: 0.017 min
Response: 933720
Conc: 84.08 ng/ml

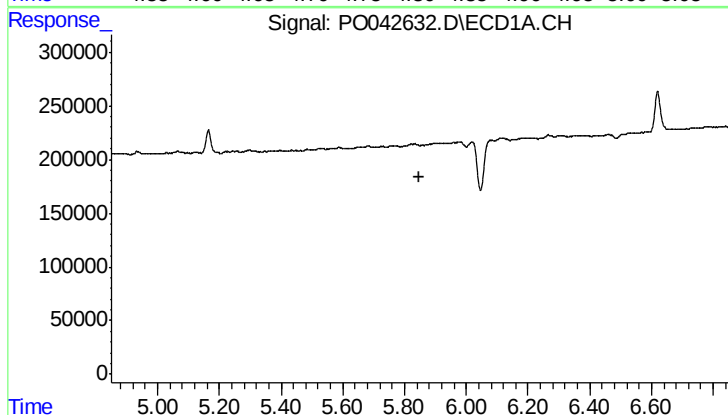


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.850 min
Response: 0
Conc: N.D.

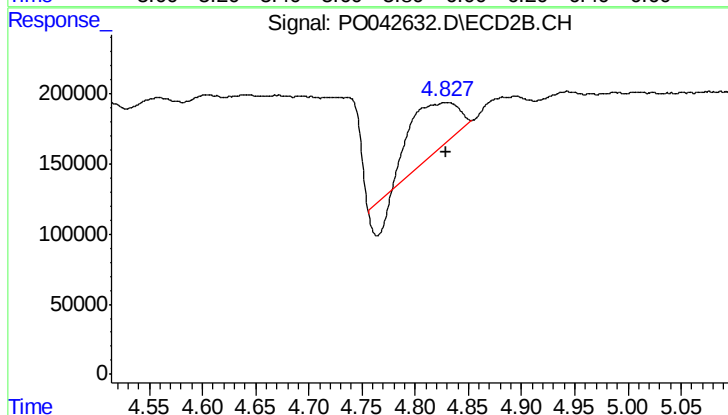

#20 AR-1242-5


R.T.: 4.828 min
Delta R.T.: 0.000 min
Response: 933720
Conc: 161.48 ng/ml

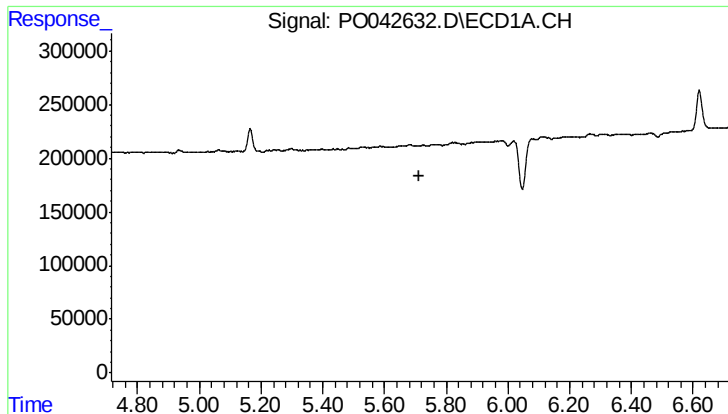

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.715 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

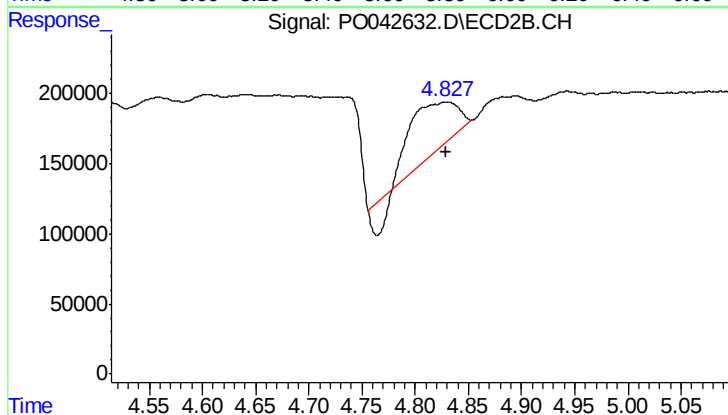


#21 AR-1248-1

R.T.: 4.828 min
Delta R.T.: -0.002 min
Response: 933720
Conc: 85.41 ng/ml

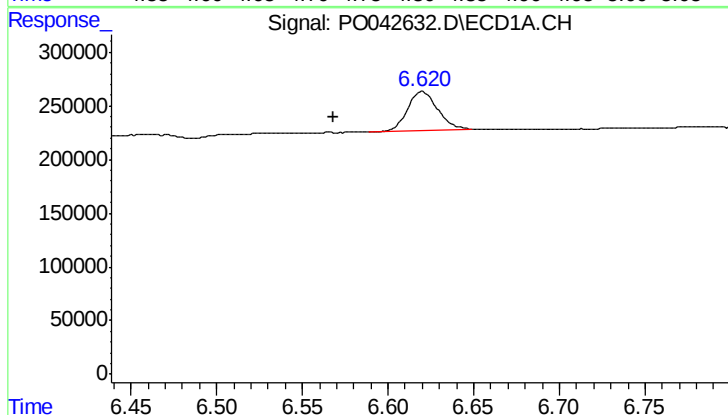


#27 AR-1254-2

R.T.: 6.620 min
Delta R.T.: 0.052 min
Response: 436843
Conc: 50.23 ng/ml

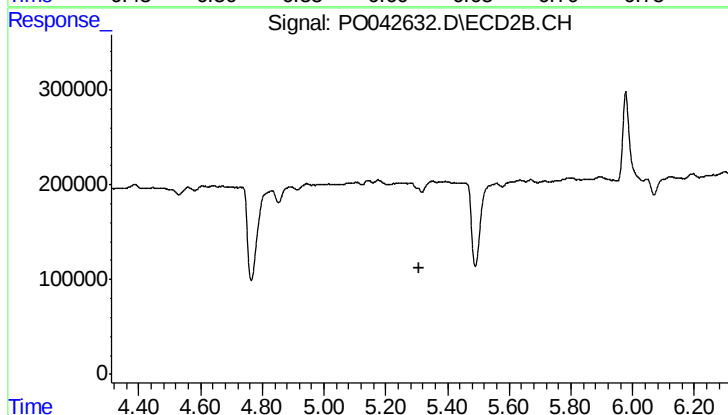

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.310 min
Response: 0
Conc: N.D.

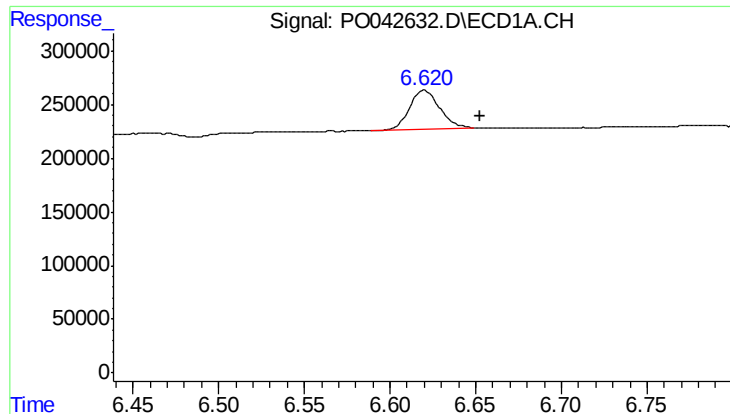

#28 AR-1254-3


R.T.: 6.620 min
Delta R.T.: -0.032 min
Response: 436843
Conc: 28.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

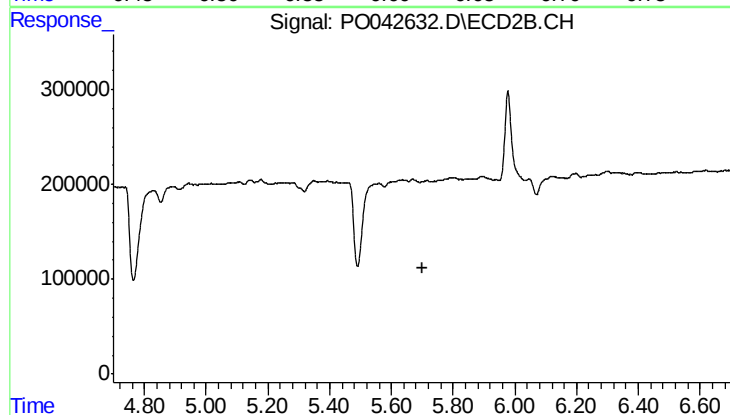


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 5.699 min
Response: 0
Conc: N.D.

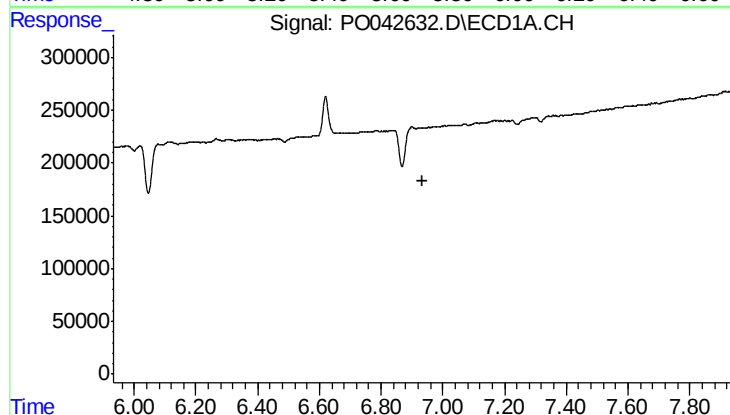


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 6.933 min
Response: 0
Conc: N.D.

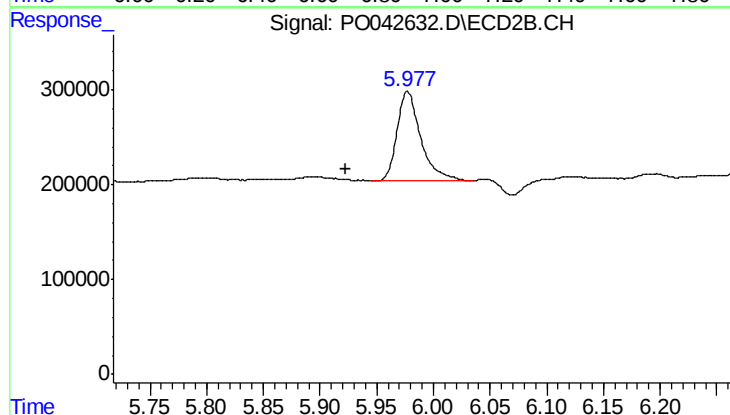

#29 AR-1254-4


R.T.: 5.977 min
Delta R.T.: 0.054 min
Response: 1381795
Conc: 70.91 ng/ml

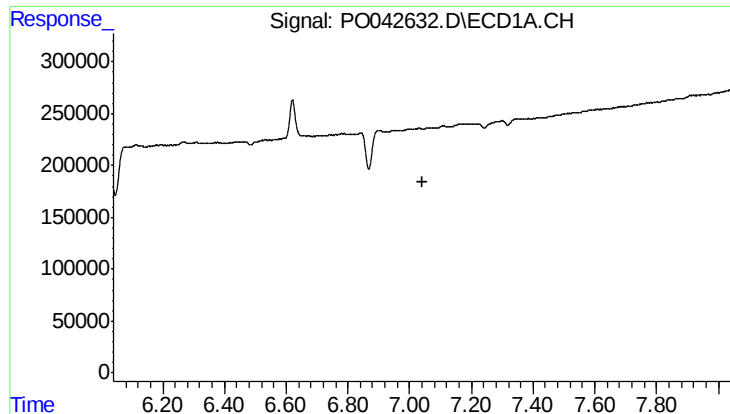

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-2022

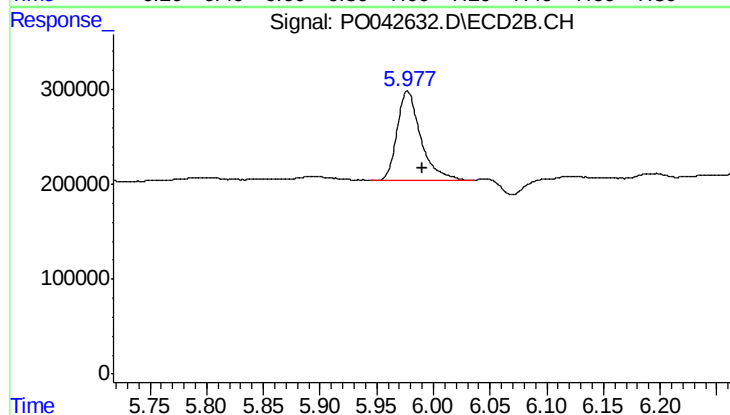


#32 AR-1260-2

R.T.: 5.977 min
Delta R.T.: -0.014 min
Response: 1381795
Conc: 41.13 ng/ml

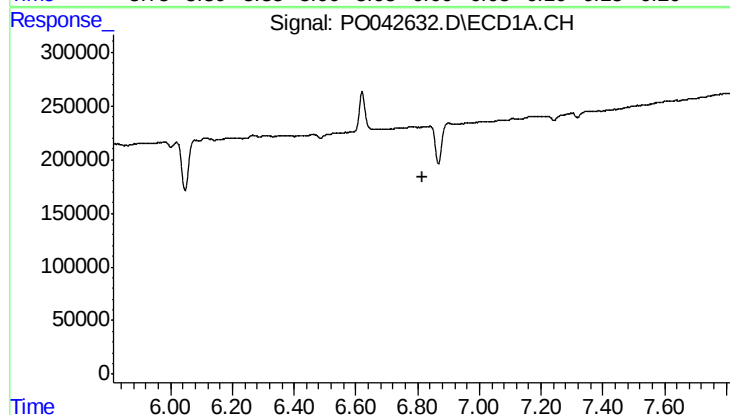

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.814 min
Response: 0
Conc: N.D.

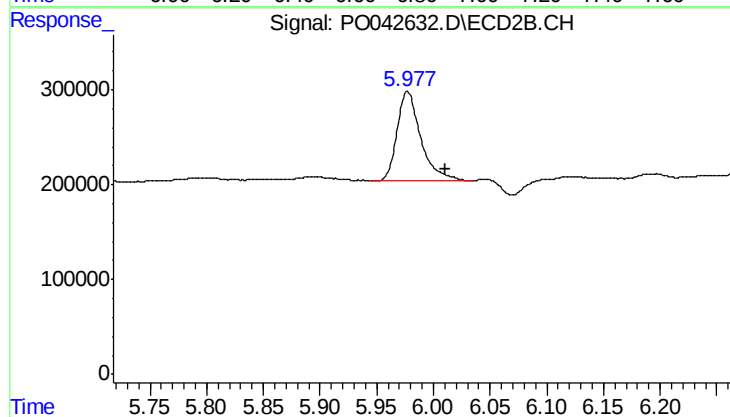

#36 AR-1262-1

R.T.: 5.977 min
Delta R.T.: -0.034 min
Response: 1381795
Conc: 62.21 ng/ml