

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
Data File : P0042631.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2018 17:12
Operator : SM/UA
Sample : J1630-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-1517

Manual Integrations
APPROVED

ugo
2/28/2018 5:09:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:35:19 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.095	3.344	4817098	9373123	19.446m	25.365 #
2) SA Decachlor...	9.473	8.126	5026122	7488246	19.887m	19.419

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
Data File : P0042631.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2018 17:12
Operator : SM/UA
Sample : J1630-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-1517


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:35:19 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

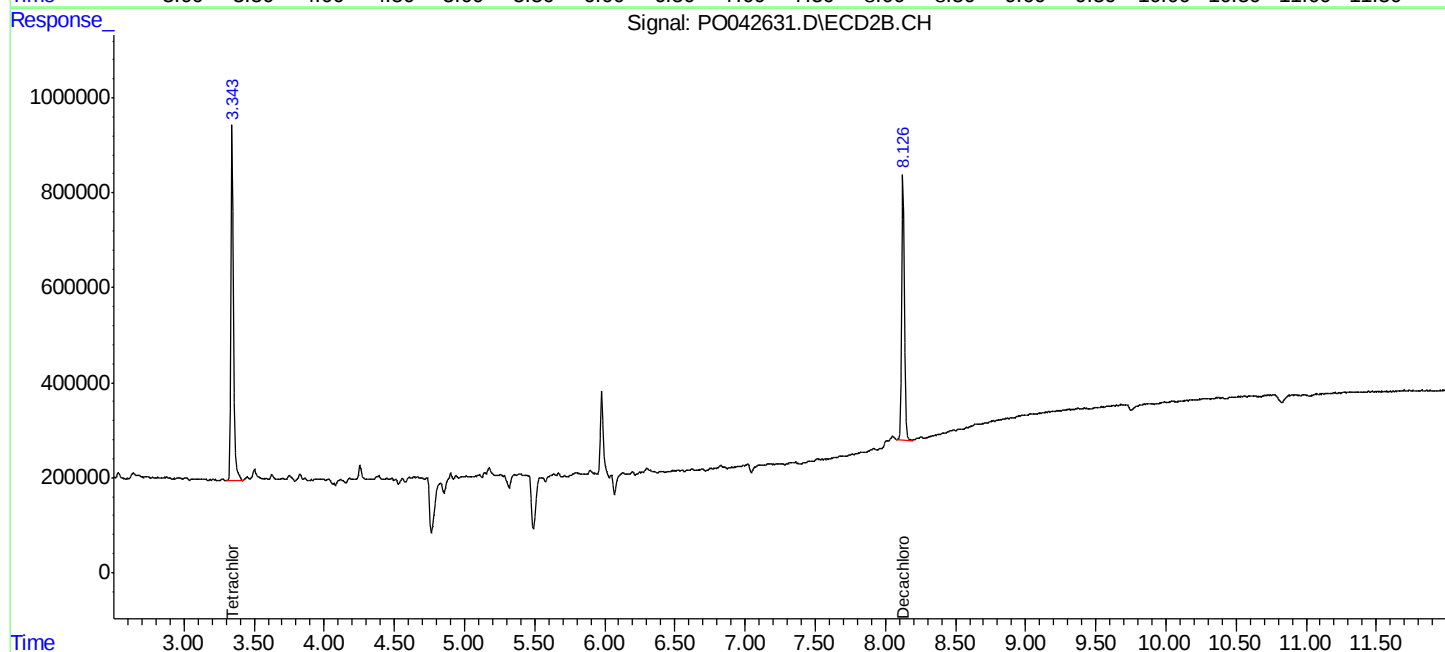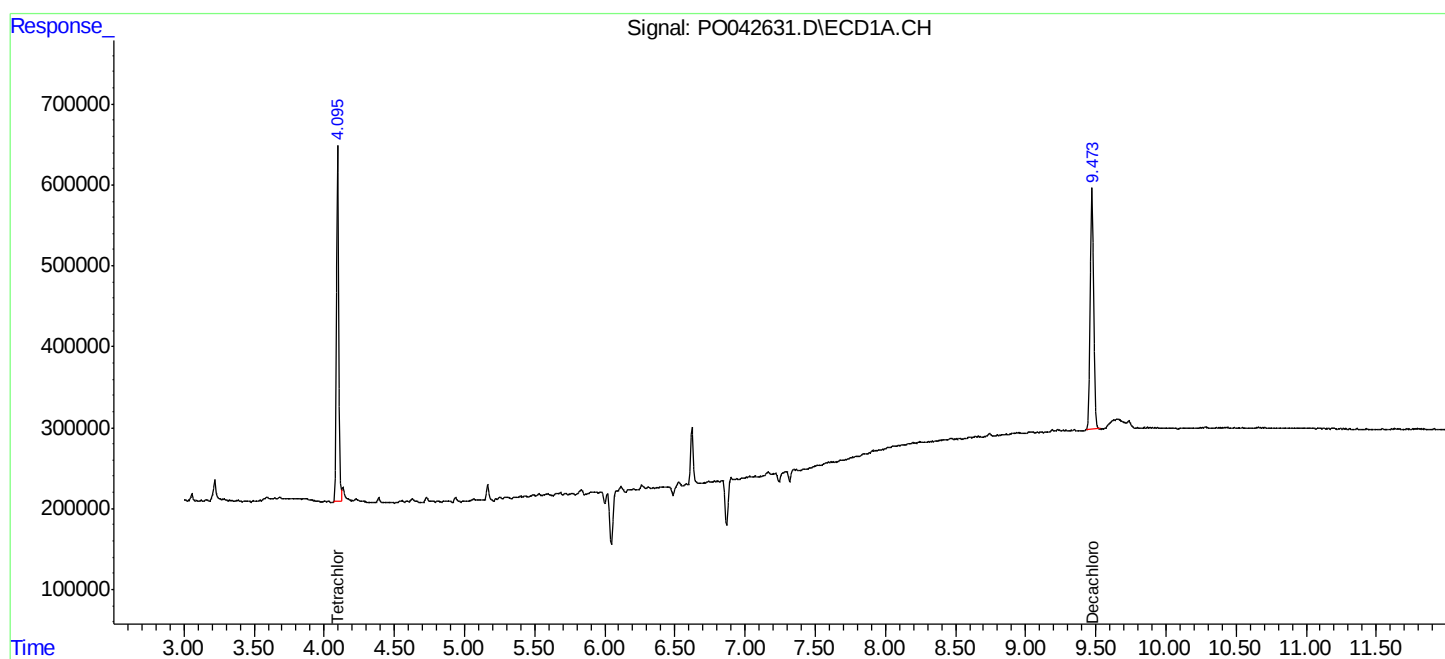

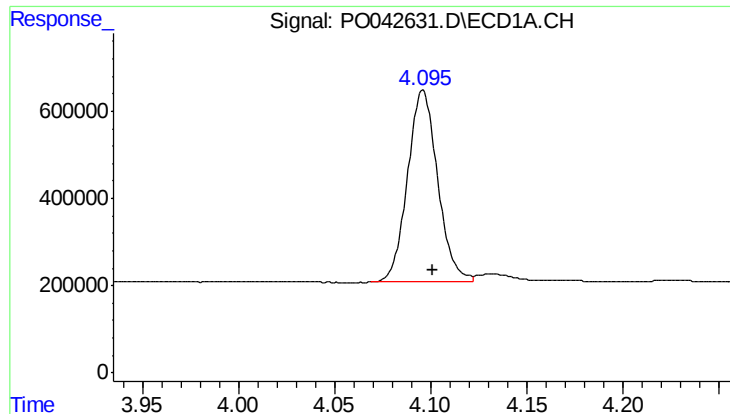


#1 Tetrachloro-m-xylene

R.T.: 4.095 min
Delta R.T.: -0.006 min
Response: 4817098
Conc: 19.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4001-1517


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:22 PM

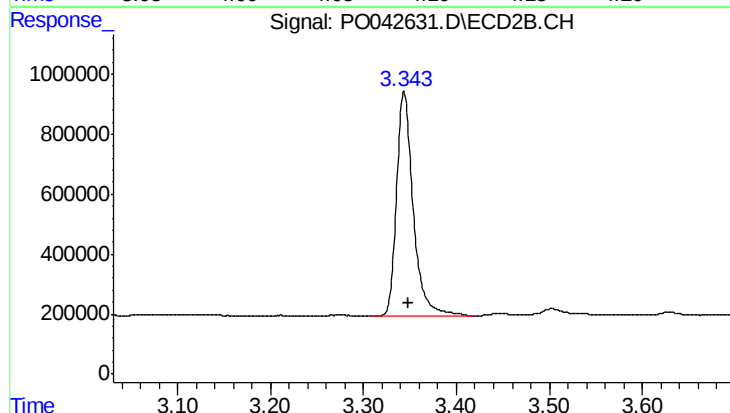


#1 Tetrachloro-m-xylene

R.T.: 3.344 min
Delta R.T.: -0.004 min
Response: 9373123
Conc: 25.36 ng/ml

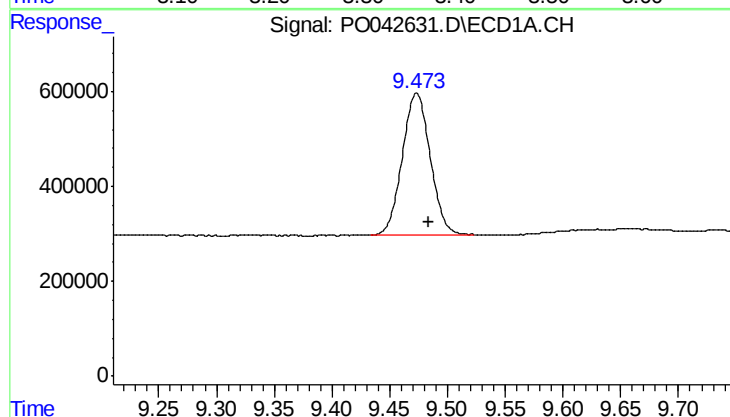

#2 Decachlorobiphenyl

R.T.: 9.473 min
Delta R.T.: -0.011 min
Response: 5026122
Conc: 19.89 ng/ml m

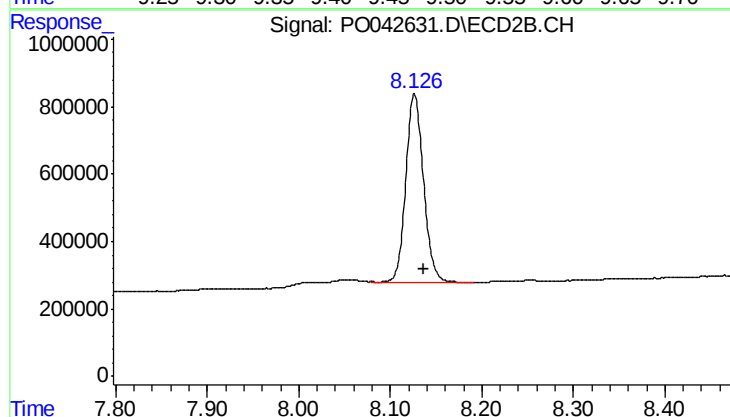

#2 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.010 min
Response: 7488246
Conc: 19.42 ng/ml