

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
 Data File : P0042635.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Feb 2018 18:12
 Operator : SM/UA
 Sample : J1630-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BPS1-SB4006-2022

Manual Integrations
 APPROVED

ugo
 2/28/2018 5:09:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:41:55 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.096	3.344	5345323	9240227	21.578	25.005
2) SA Decachlor...	9.472	8.126	4679794	6750333	18.517m	17.505m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
Data File : P0042635.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2018 18:12
Operator : SM/UA
Sample : J1630-05
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4006-2022


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:41:55 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

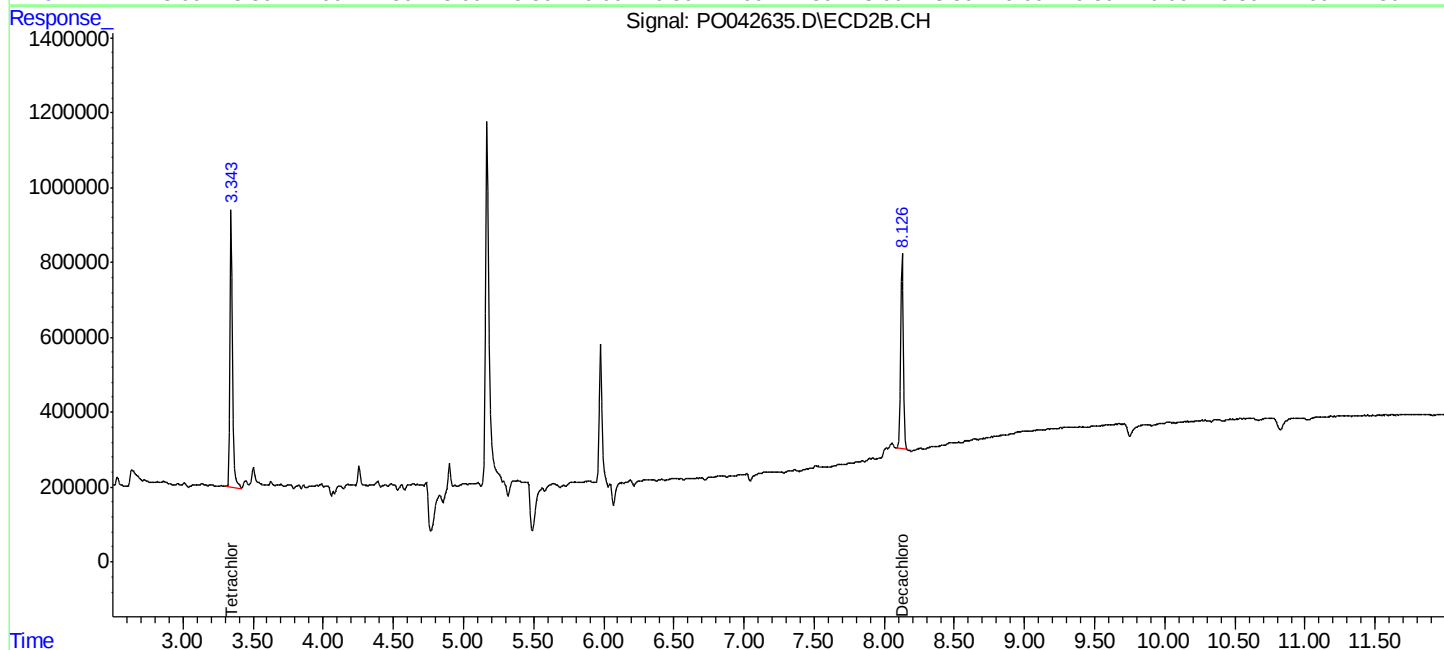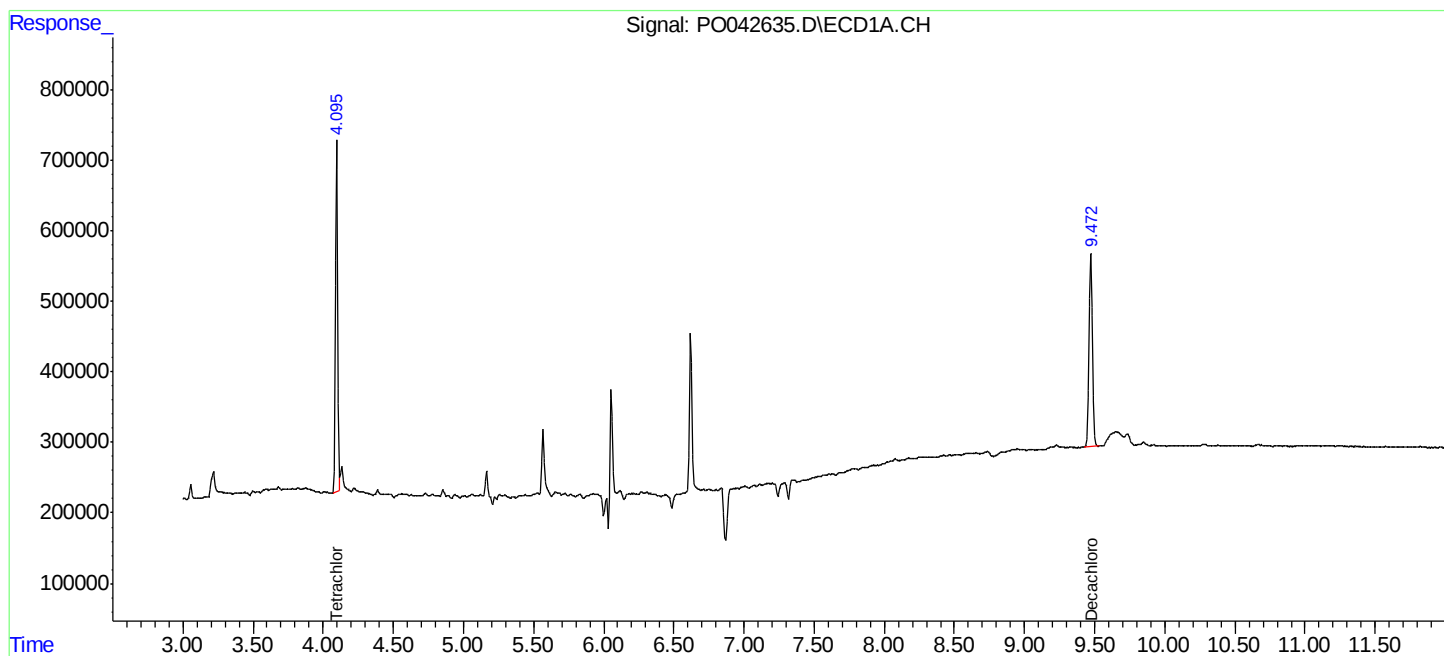

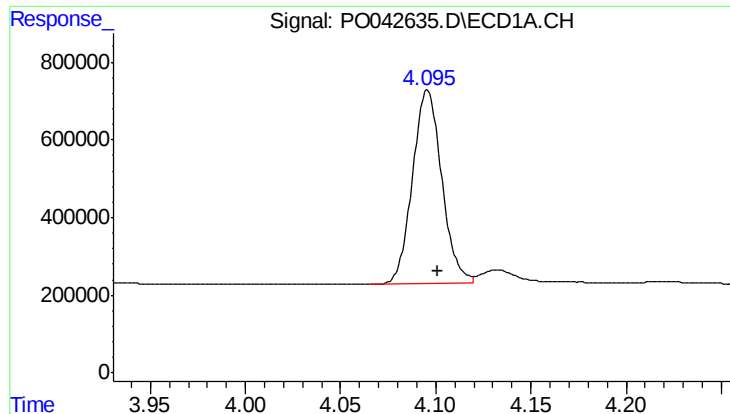


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.006 min
Response: 5345323
Conc: 21.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4006-2022


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:32 PM

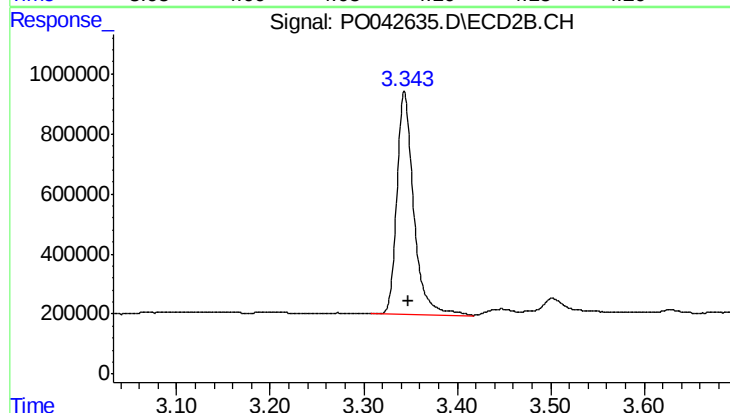


#1 Tetrachloro-m-xylene

R.T.: 3.344 min
Delta R.T.: -0.004 min
Response: 9240227
Conc: 25.01 ng/ml

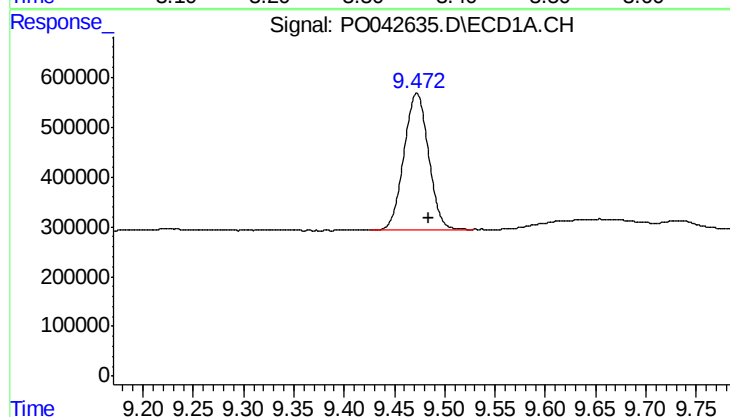

#2 Decachlorobiphenyl

R.T.: 9.472 min
Delta R.T.: -0.012 min
Response: 4679794
Conc: 18.52 ng/ml m

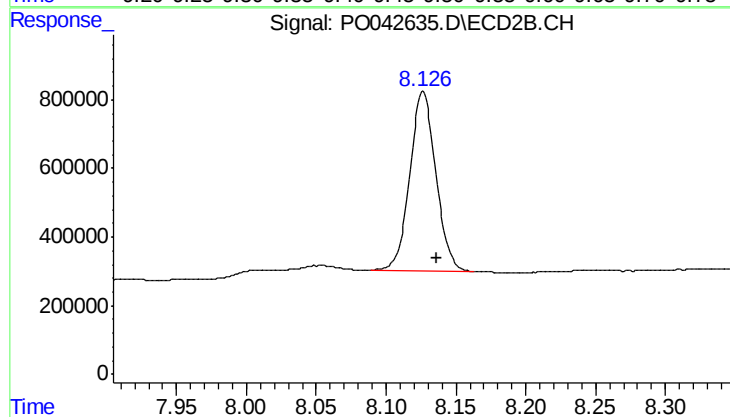

#2 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.010 min
Response: 6750333
Conc: 17.51 ng/ml m