

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
 Data File : P0042637.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Feb 2018 18:42
 Operator : SM/UA
 Sample : J1630-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BPS1-SB4003-1517

Manual Integrations
 APPROVED

ugo
 2/28/2018 5:09:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:51:04 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.094	3.343	4980925	9875439	20.107m	26.724 #
2) SA Decachlor...	9.481	8.126	6706108	25785980	26.535m	66.869m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0022618\
Data File : P0042637.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2018 18:42
Operator : SM/UA
Sample : J1630-07
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-1517


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:51:04 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

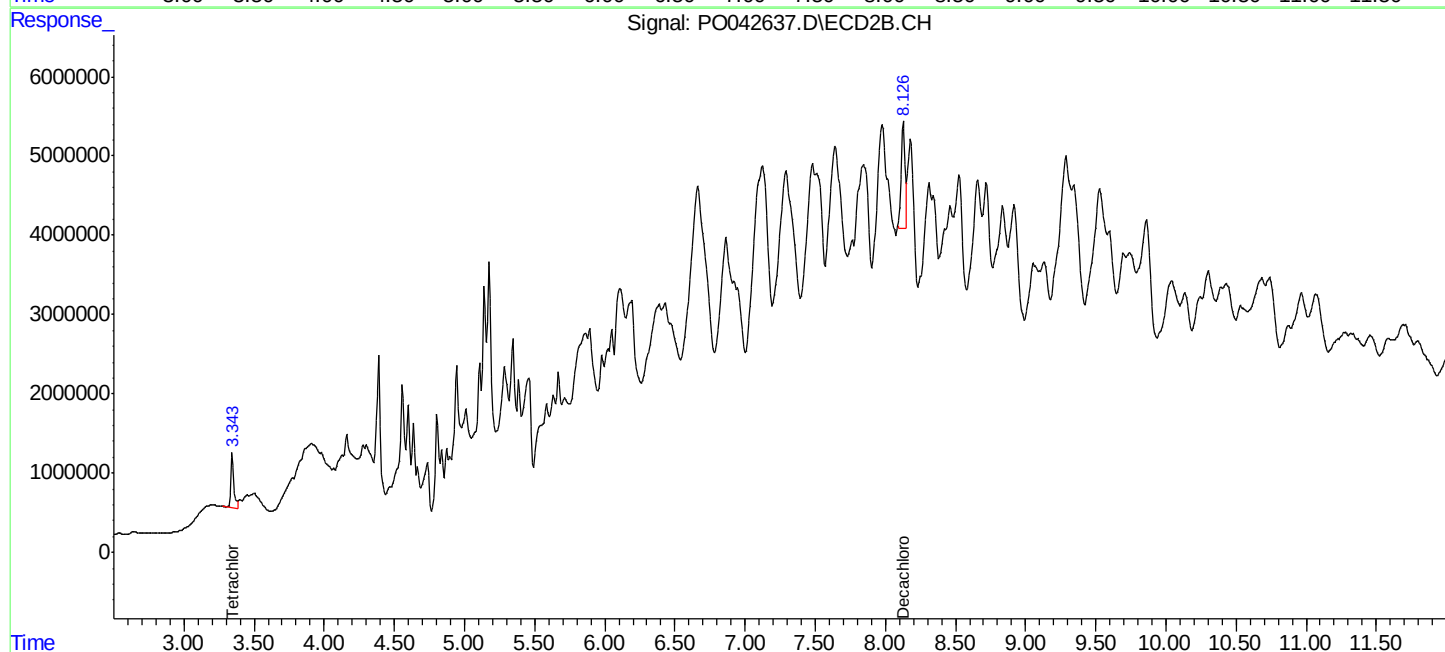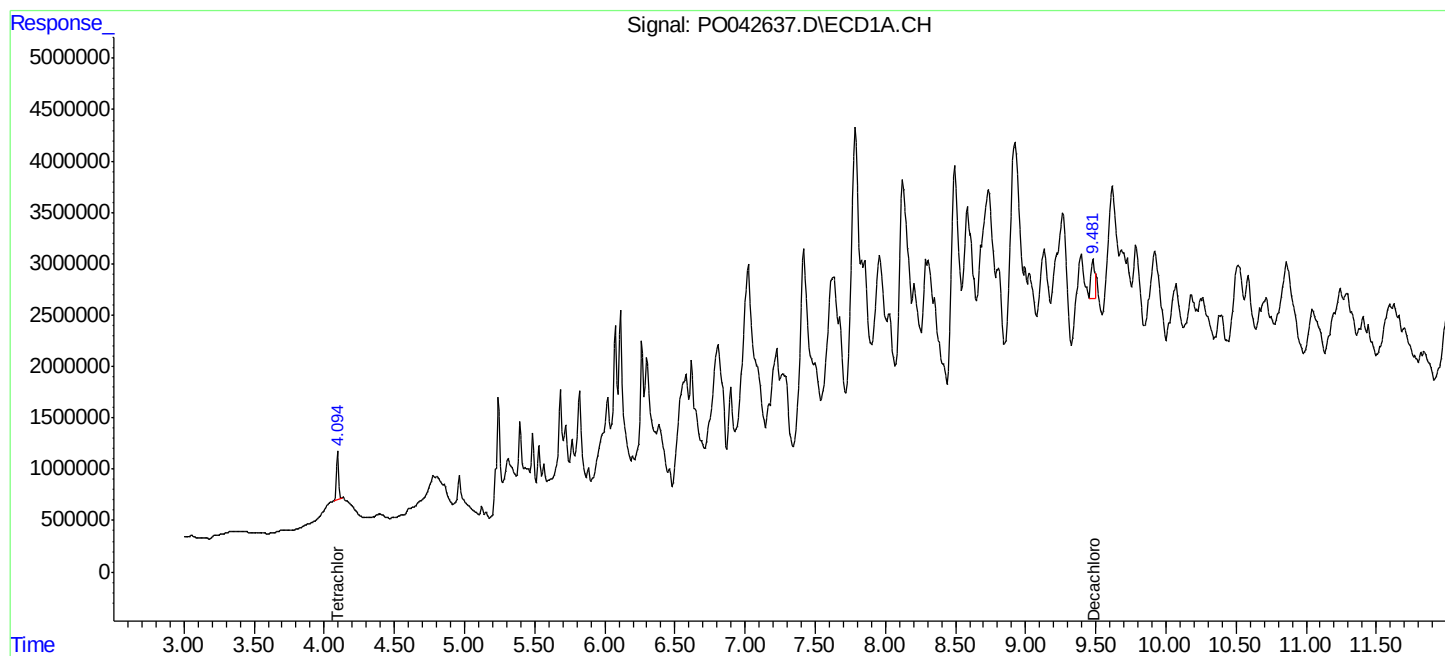

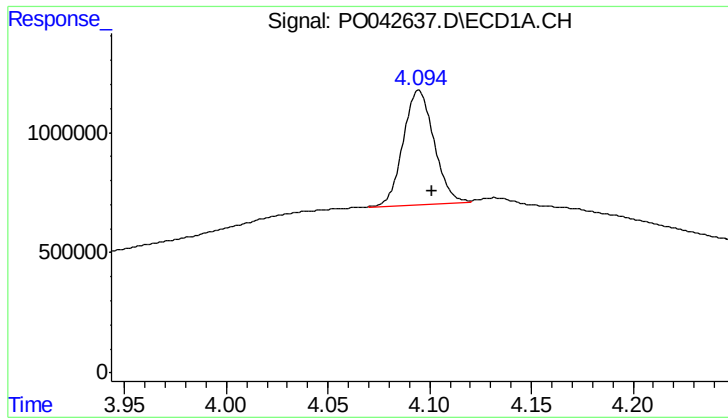


#1 Tetrachloro-m-xylene

R.T.: 4.094 min
Delta R.T.: -0.007 min
Response: 4980925
Conc: 20.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-1517


Manual Integrations
APPROVED

ugo
2/28/2018 5:09:36 PM

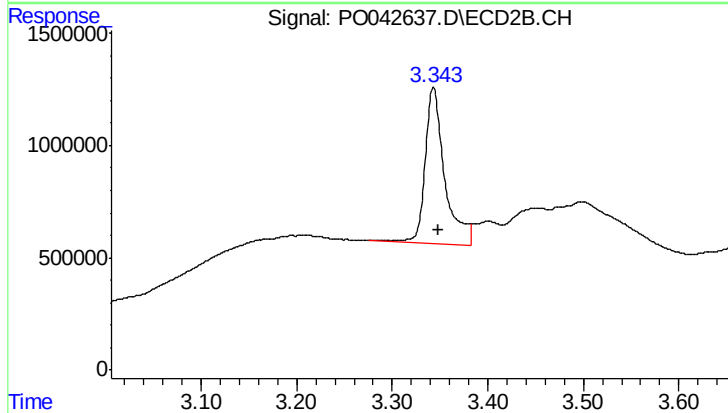


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: -0.005 min
Response: 9875439
Conc: 26.72 ng/ml

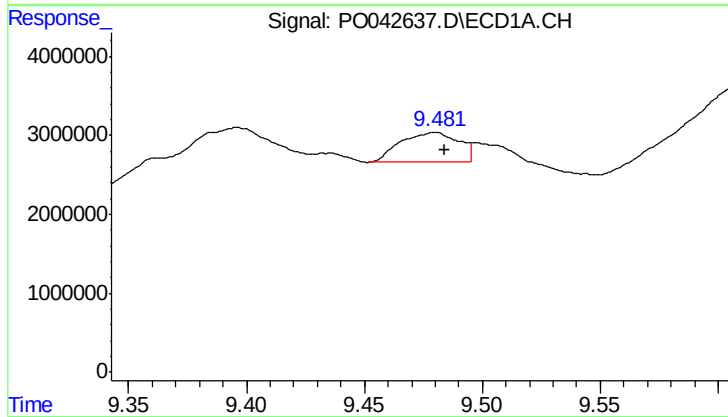

#2 Decachlorobiphenyl

R.T.: 9.481 min
Delta R.T.: -0.004 min
Response: 6706108
Conc: 26.53 ng/ml m

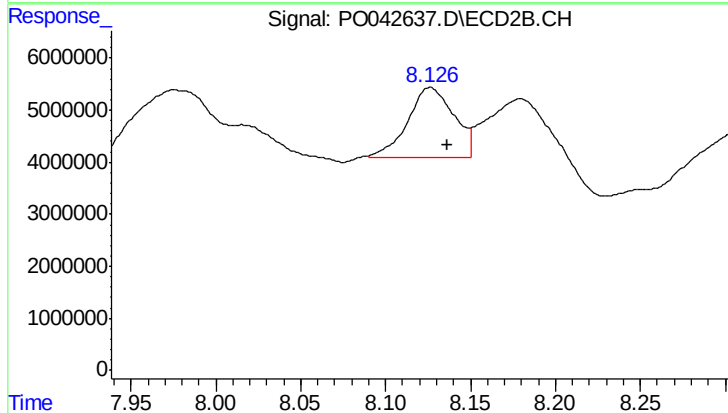

#2 Decachlorobiphenyl

R.T.: 8.126 min
Delta R.T.: -0.011 min
Response: 25785980
Conc: 66.87 ng/ml m