

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022619\
Data File : P0054055.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2019 12:56
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 04:26:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.053	3.131	41374715	4724298	19.291	18.428
2) SA Decachlor...	9.390	7.710	19951929	5078841	18.283	19.116

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022619\
Data File : P0054055.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Feb 2019 12:56
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 04:26:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

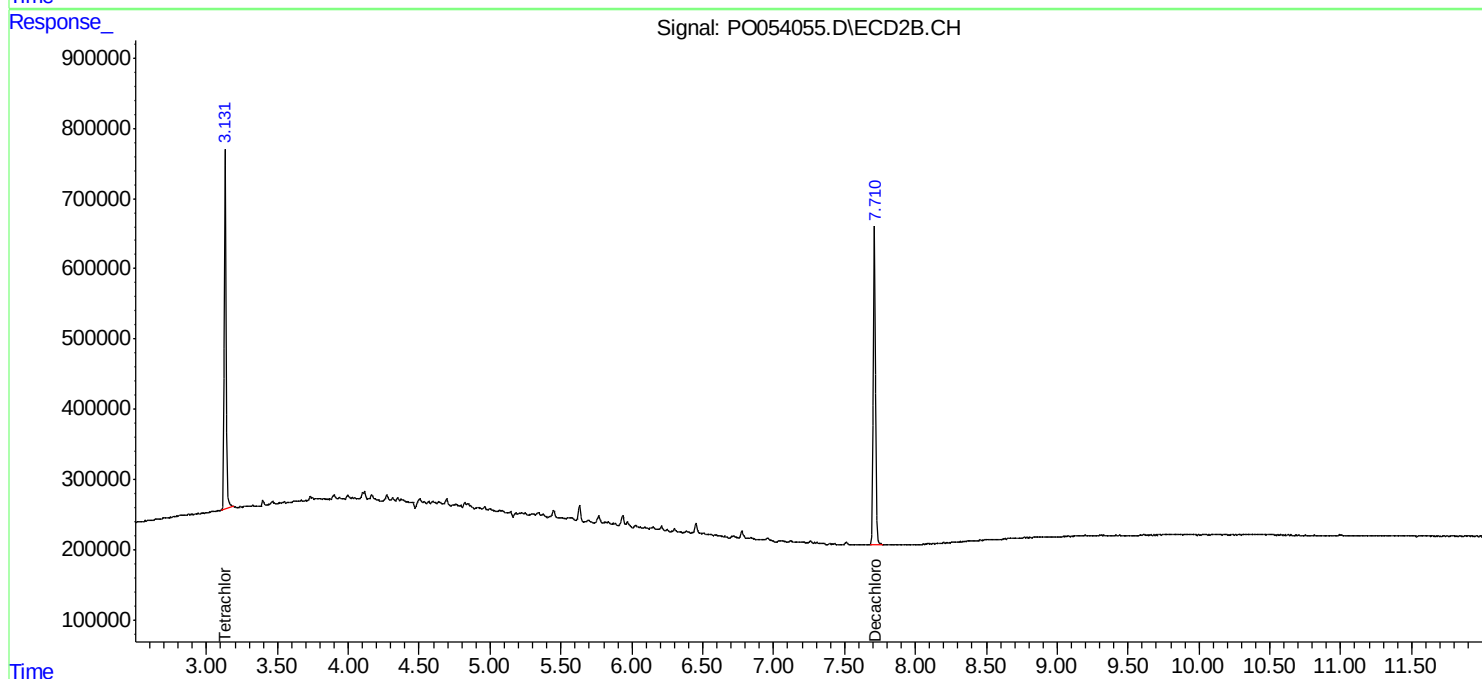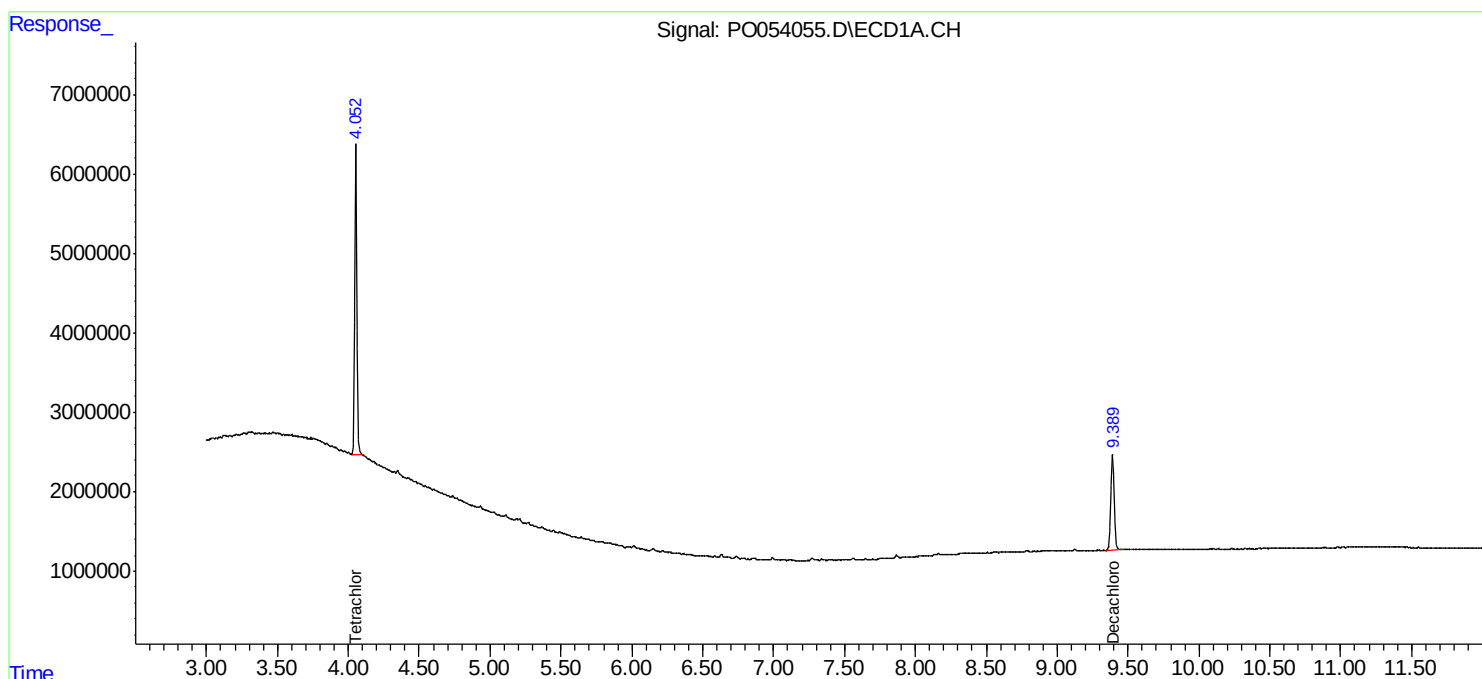


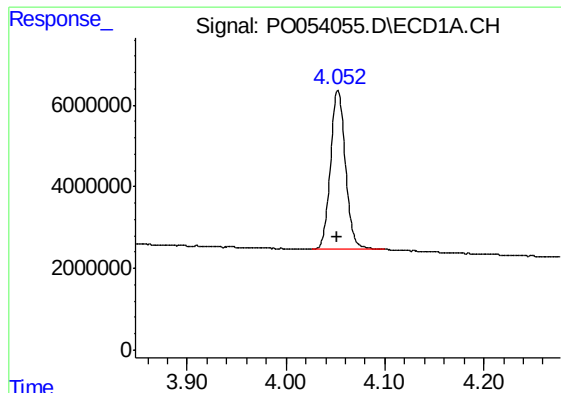

#1 Tetrachloro-m-xylene


R.T.: 4.053 min
Delta R.T.: 0.002 min
Response: 41374715
Conc: 19.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

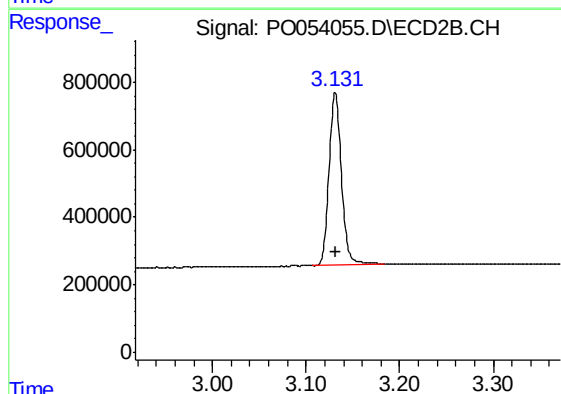


#1 Tetrachloro-m-xylene

R.T.: 3.131 min
Delta R.T.: 0.000 min
Response: 4724298
Conc: 18.43 ng/ml

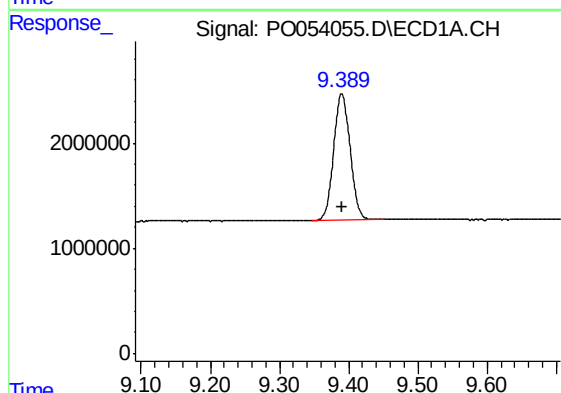

#2 Decachlorobiphenyl

R.T.: 9.390 min
Delta R.T.: 0.000 min
Response: 19951929
Conc: 18.28 ng/ml

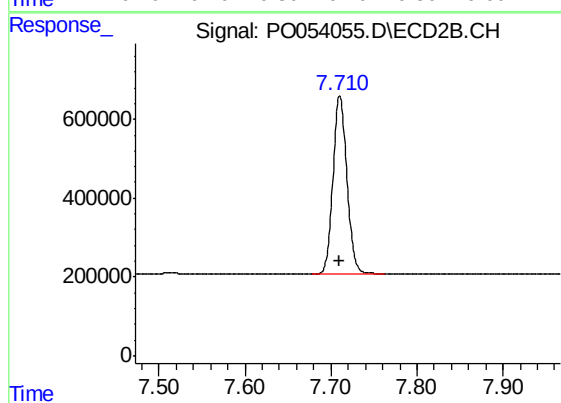

#2 Decachlorobiphenyl

R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 5078841
Conc: 19.12 ng/ml