

Data Path : P:\HPCHEM1\ECD 0\Data\P0022718\
Data File : P0042656.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2018 10:45
Operator : SM/UA
Sample : J1397-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-022318-D

Manual Integrations
APPROVED

ugo
3/2/2018 4:50:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 11:20:56 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.093	3.342	4701842	7036102	18.980	19.041
2) SA Decachlor...	9.463	8.122	3790613	4493744	14.999m	11.653

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0022718\
Data File : P0042656.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2018 10:45
Operator : SM/UA
Sample : J1397-15
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CL-02-022318-D


Manual Integrations
APPROVED

ugo
3/2/2018 4:50:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 11:20:56 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

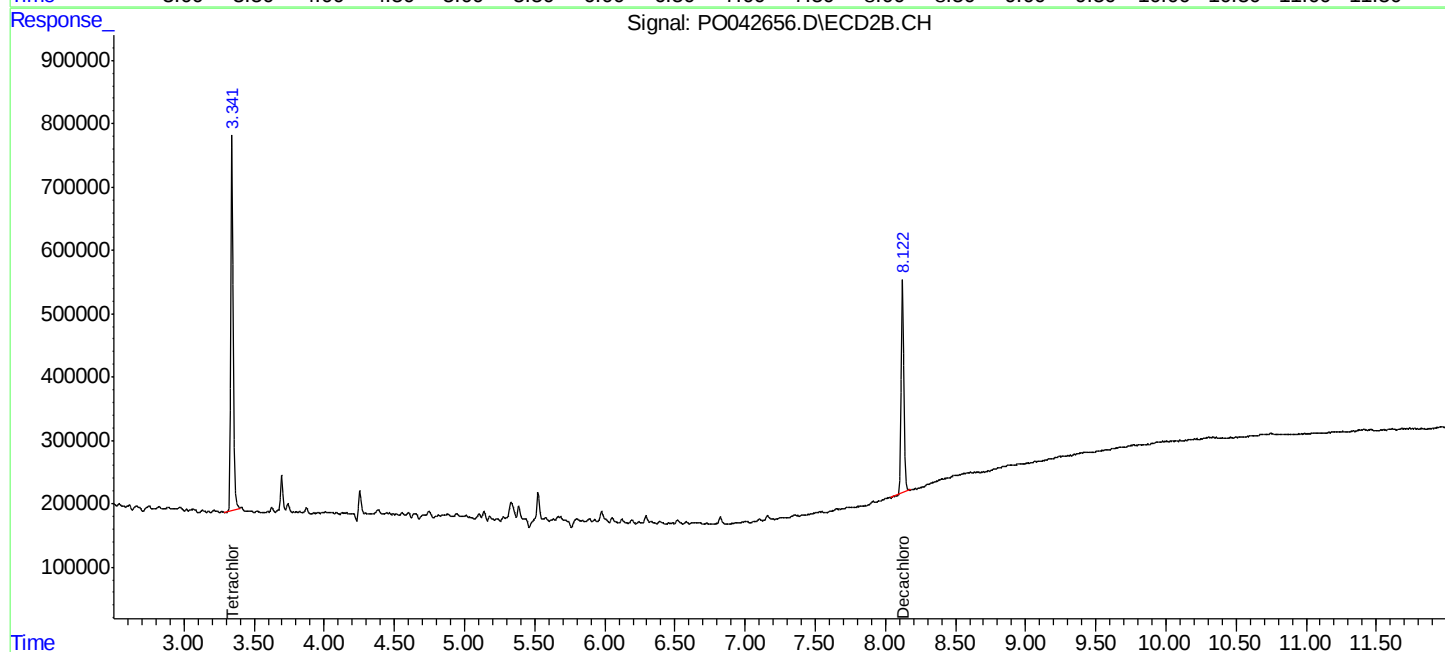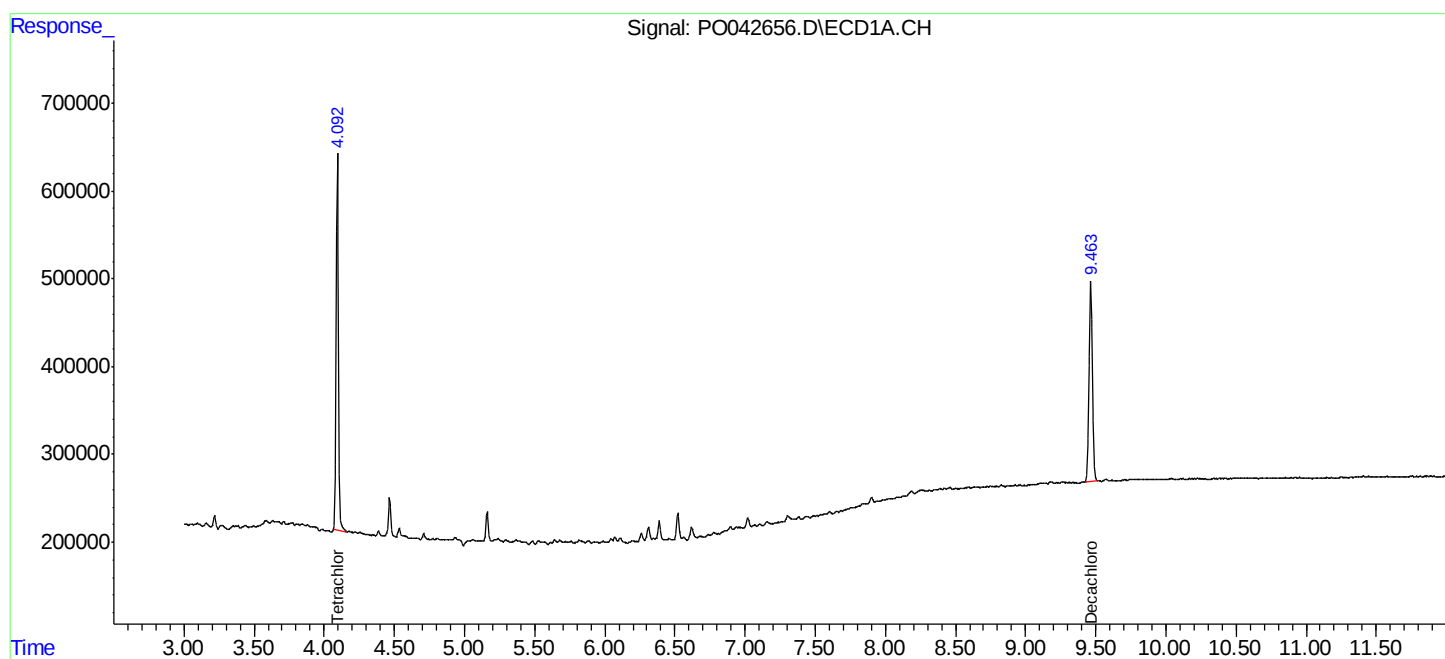

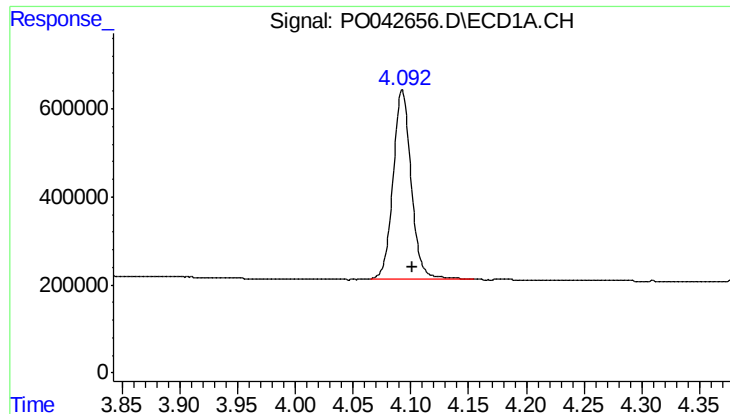


#1 Tetrachloro-m-xylene

R.T.: 4.093 min
Delta R.T.: -0.009 min
Response: 4701842
Conc: 18.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-022318-D


Manual Integrations
APPROVED

ugo
3/2/2018 4:50:32 PM

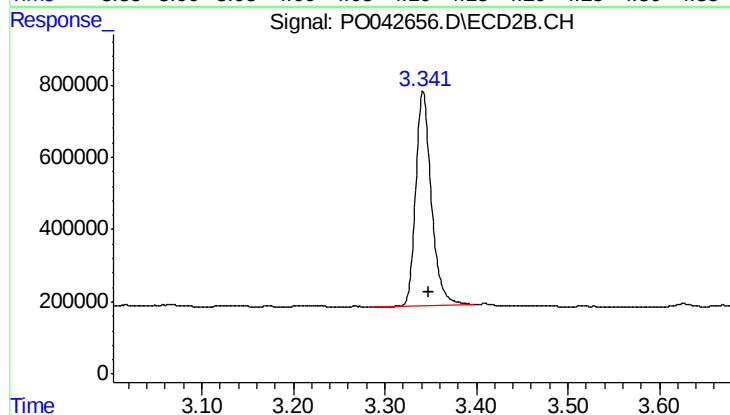


#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: -0.006 min
Response: 7036102
Conc: 19.04 ng/ml

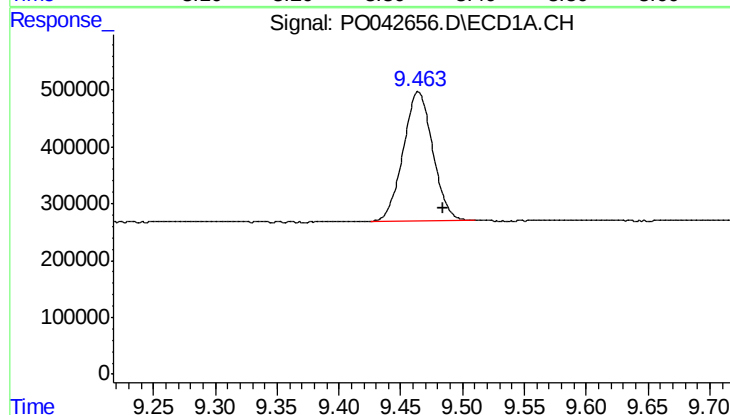

#2 Decachlorobiphenyl

R.T.: 9.463 min
Delta R.T.: -0.021 min
Response: 3790613
Conc: 15.00 ng/ml m

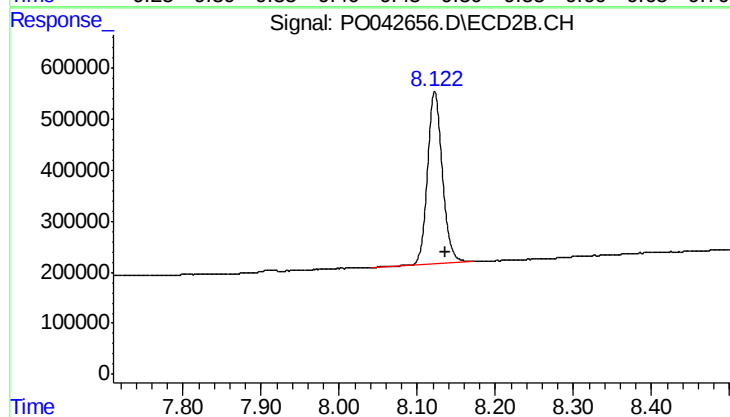

#2 Decachlorobiphenyl

R.T.: 8.122 min
Delta R.T.: -0.014 min
Response: 4493744
Conc: 11.65 ng/ml