

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022819\
 Data File : P0054121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2019 10:17
 Operator : SM/SJ
 Sample : K1353-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-02-022619-ARE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 23:50:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.051	3.127	24566753	3697942	11.454	14.424 #
2) SA Decachlor...	9.385	7.705	12784409	2629529	11.715	9.897

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022819\
Data File : P0054121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2019 10:17
Operator : SM/SJ
Sample : K1353-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PL-02-022619-ARE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 23:50:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

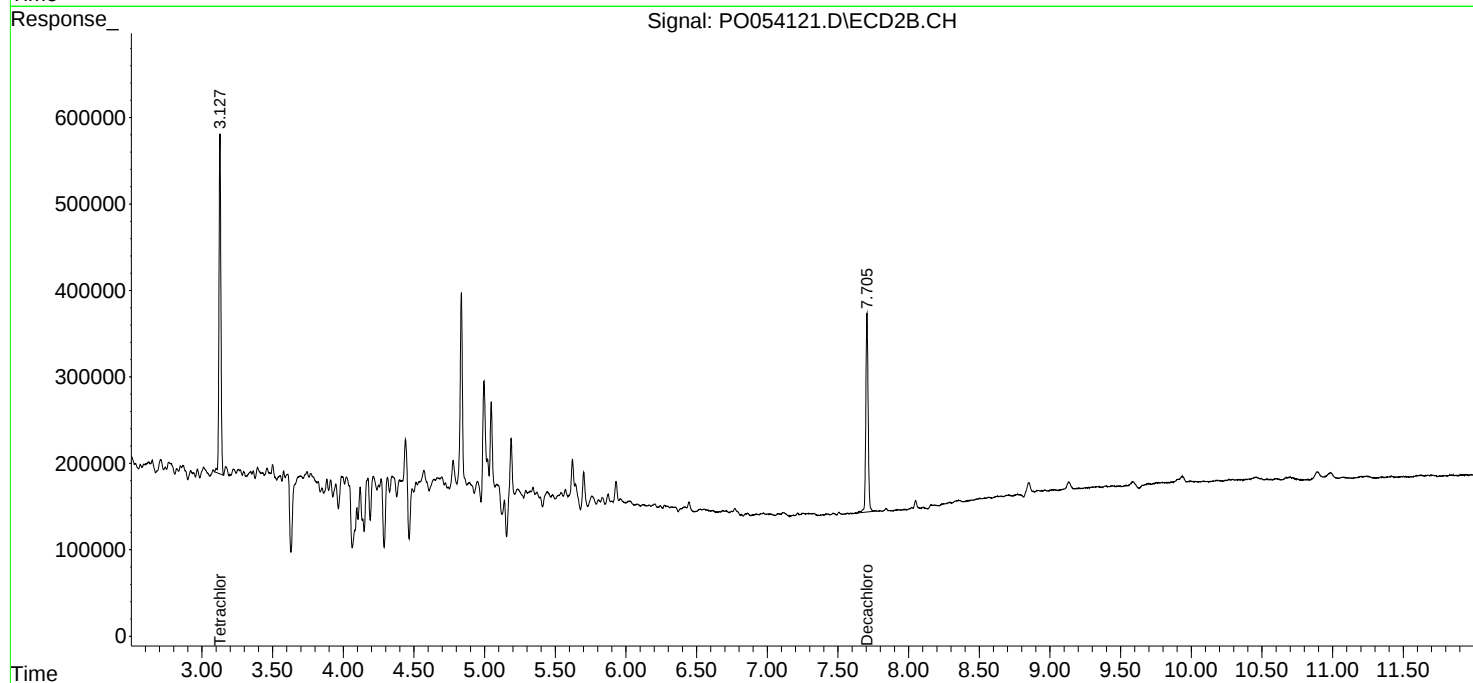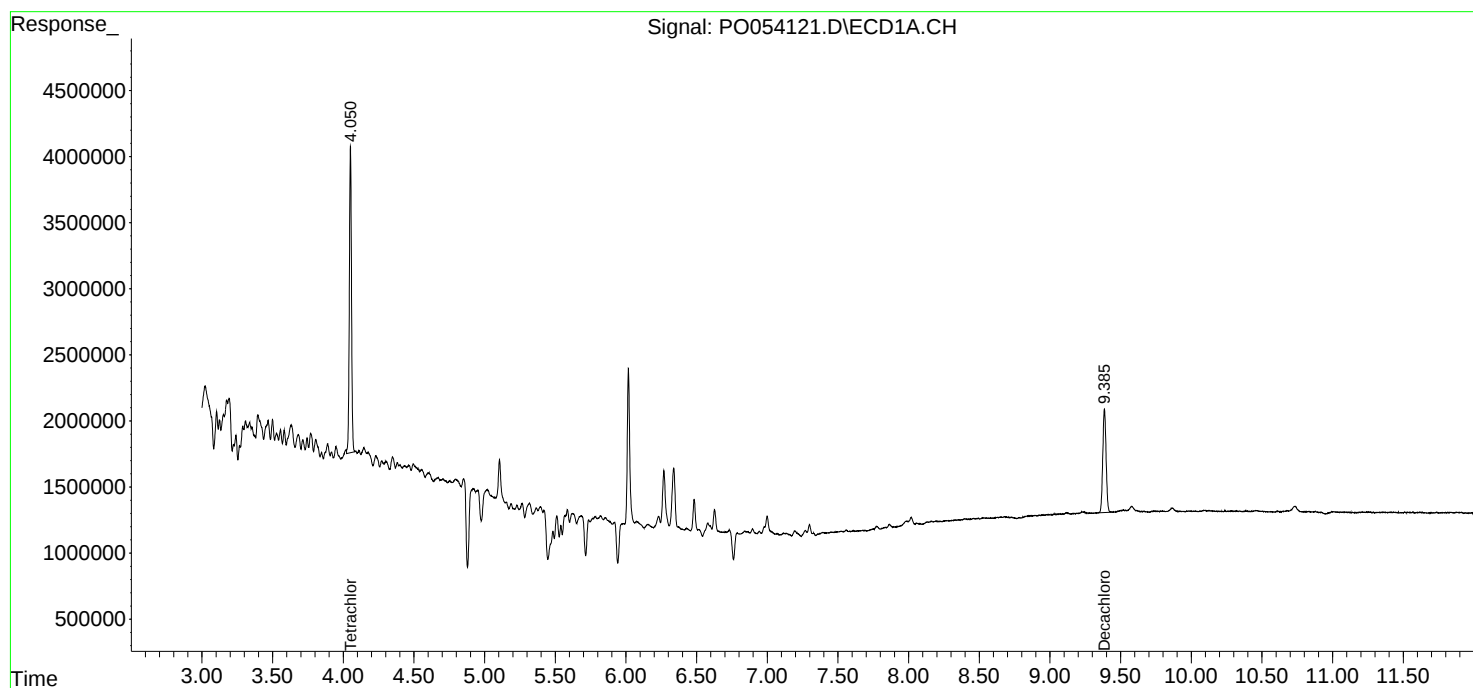


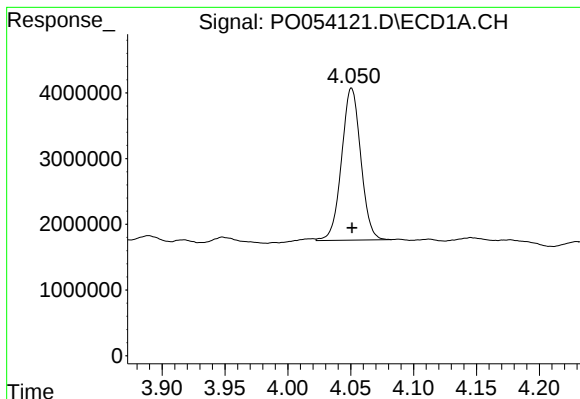

#1 Tetrachloro-m-xylene


R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 24566753
Conc: 11.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-02-022619-ARE

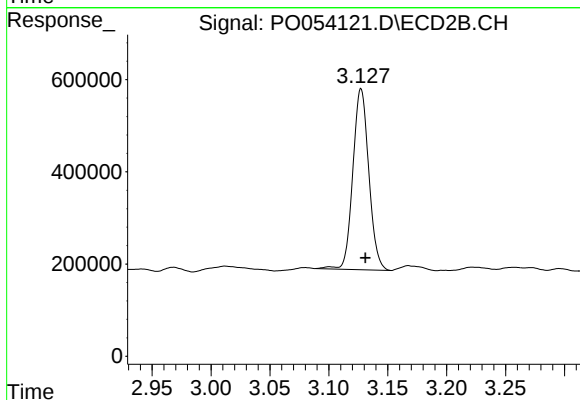


#1 Tetrachloro-m-xylene

R.T.: 3.127 min
Delta R.T.: -0.004 min
Response: 3697942
Conc: 14.42 ng/ml

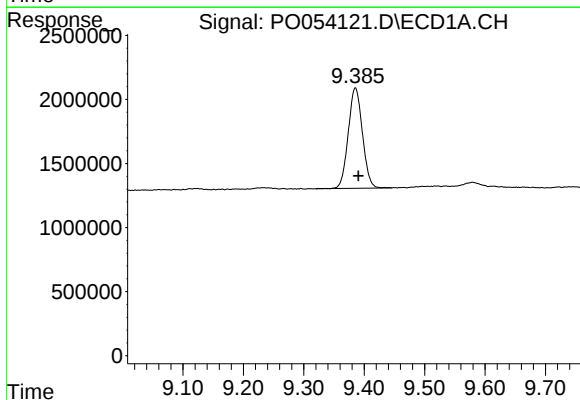

#2 Decachlorobiphenyl

R.T.: 9.385 min
Delta R.T.: -0.005 min
Response: 12784409
Conc: 11.71 ng/ml

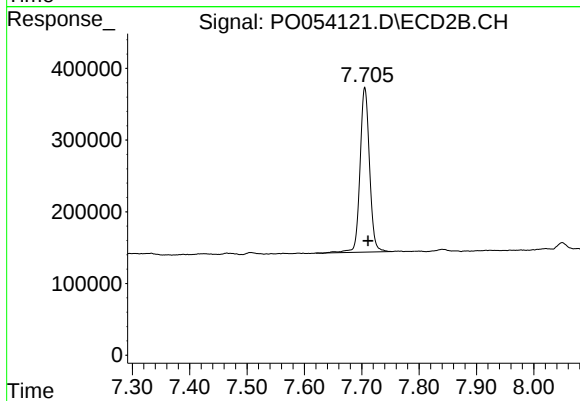

#2 Decachlorobiphenyl

R.T.: 7.705 min
Delta R.T.: -0.005 min
Response: 2629529
Conc: 9.90 ng/ml