

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022819\
 Data File : P0054161.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 00:52
 Operator : SM/SJ
 Sample : K1652-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-DAY-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 02:48:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.042	3.126	78494455	6695455	36.598	26.116 #
2) SA Decachlor...	9.369	7.698	19137112	4840826	17.536	18.220

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022819\
Data File : PO054161.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 00:52
Operator : SM/SJ
Sample : K1652-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-DAY-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 02:48:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

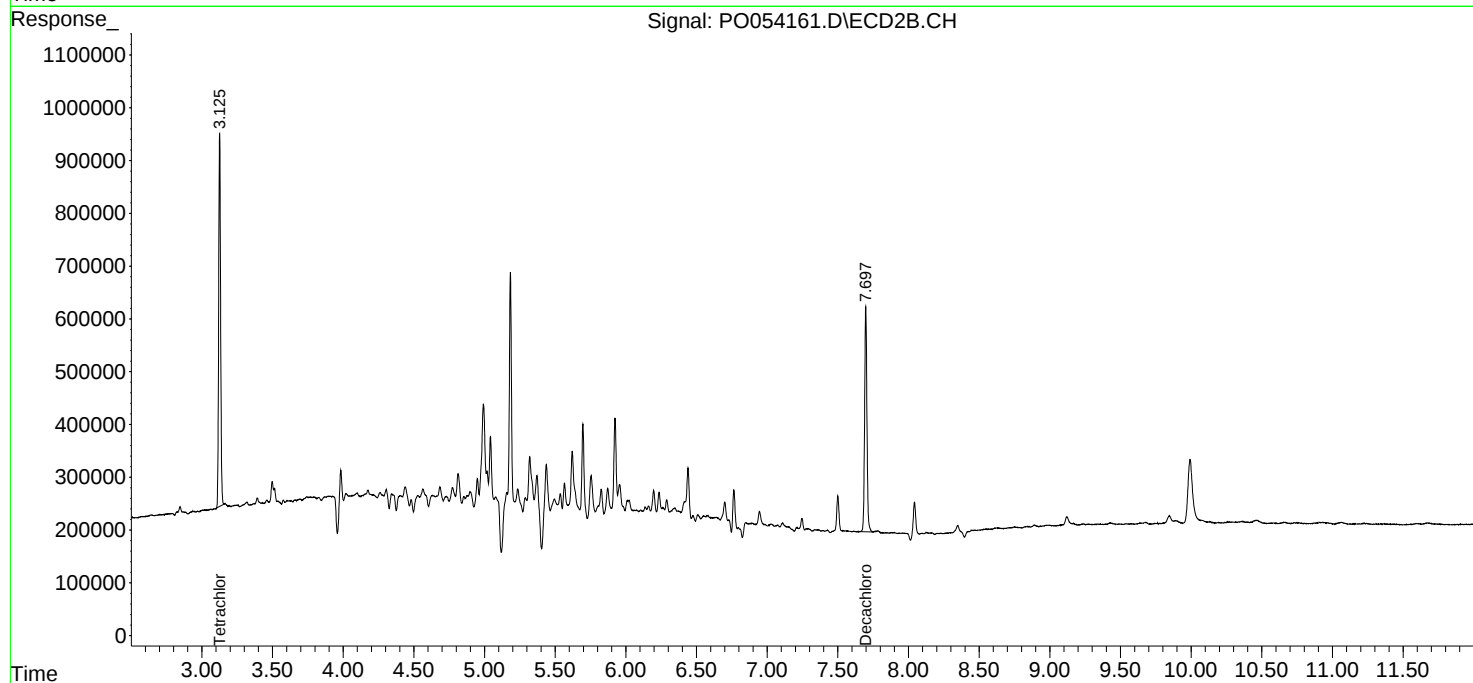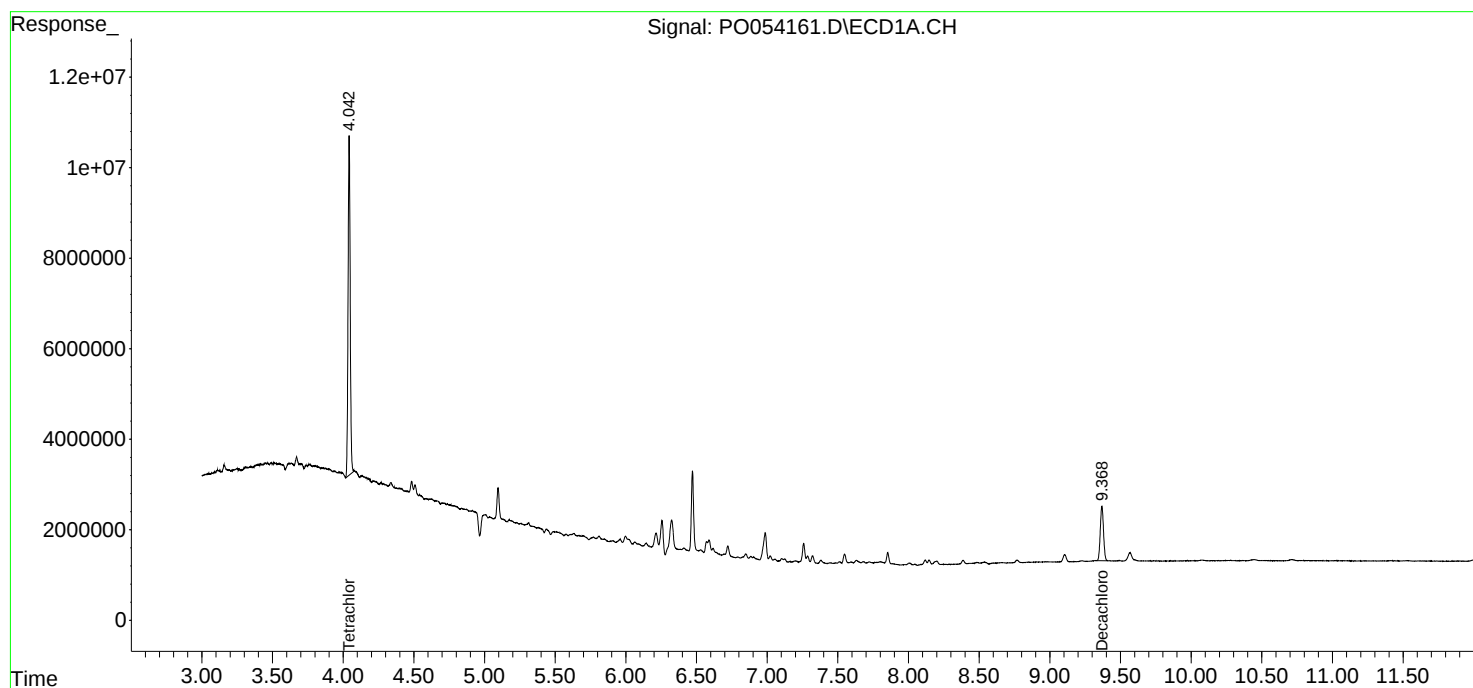


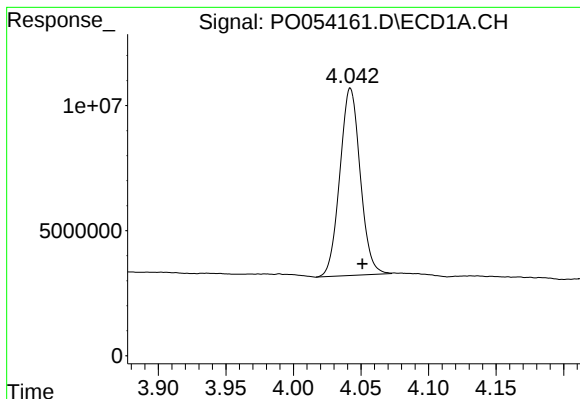

#1 Tetrachloro-m-xylene


R.T.: 4.042 min
Delta R.T.: -0.009 min
Response: 78494455
Conc: 36.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-DAY-2

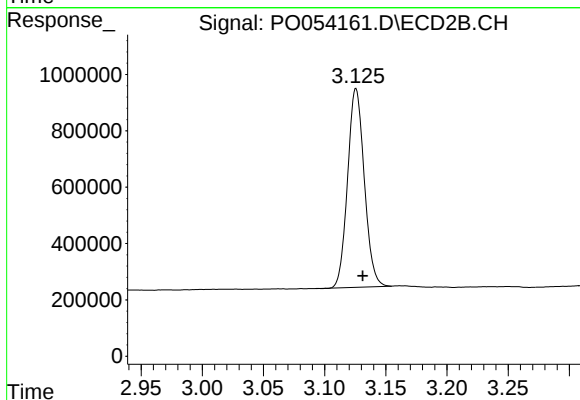


#1 Tetrachloro-m-xylene

R.T.: 3.126 min
Delta R.T.: -0.006 min
Response: 6695455
Conc: 26.12 ng/ml

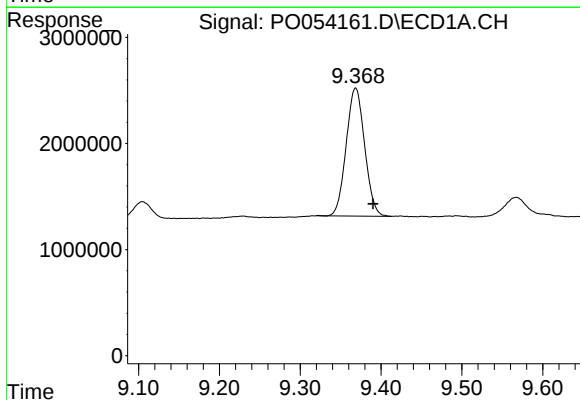

#2 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.022 min
Response: 19137112
Conc: 17.54 ng/ml

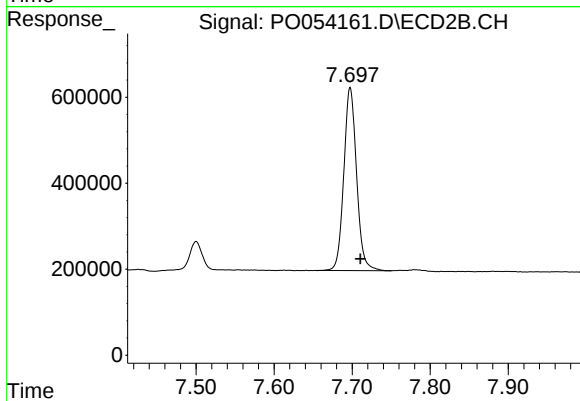

#2 Decachlorobiphenyl

R.T.: 7.698 min
Delta R.T.: -0.013 min
Response: 4840826
Conc: 18.22 ng/ml