

Data Path : P:\HPCHEM1\ECD 0\Data\P0030118\
 Data File : P0042677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2018 8:20
 Operator : SM/UA
 Sample : J1630-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BPS1-SB4003-2022

Manual Integrations
 APPROVED

ugo
 3/2/2018 4:51:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 09:19:20 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 26 14:24:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.094	3.342	5277645	7618490	21.305	20.617
2) SA Decachlor...	9.469	8.124	5423017	7959744	21.458m	20.641
Target Compounds						
21) L5 AR-1248-1	5.720	4.837	1480556	2237207	204.738	204.648
22) L5 AR-1248-2	5.882	4.941	894744	6350579	142.724	653.111 #
23) L5 AR-1248-3	6.110	5.137	5440344	7351551	594.935	433.452m#
24) L5 AR-1248-4	6.110	5.176	5440344	8902951	607.099	659.359
25) L5 AR-1248-5	6.299	5.668	3264454	2911523	546.458	377.852 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO030118\
Data File : PO042677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2018 8:20
Operator : SM/UA
Sample : J1630-08
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-2022


Manual Integrations
APPROVED

ugo
3/2/2018 4:51:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 09:19:20 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

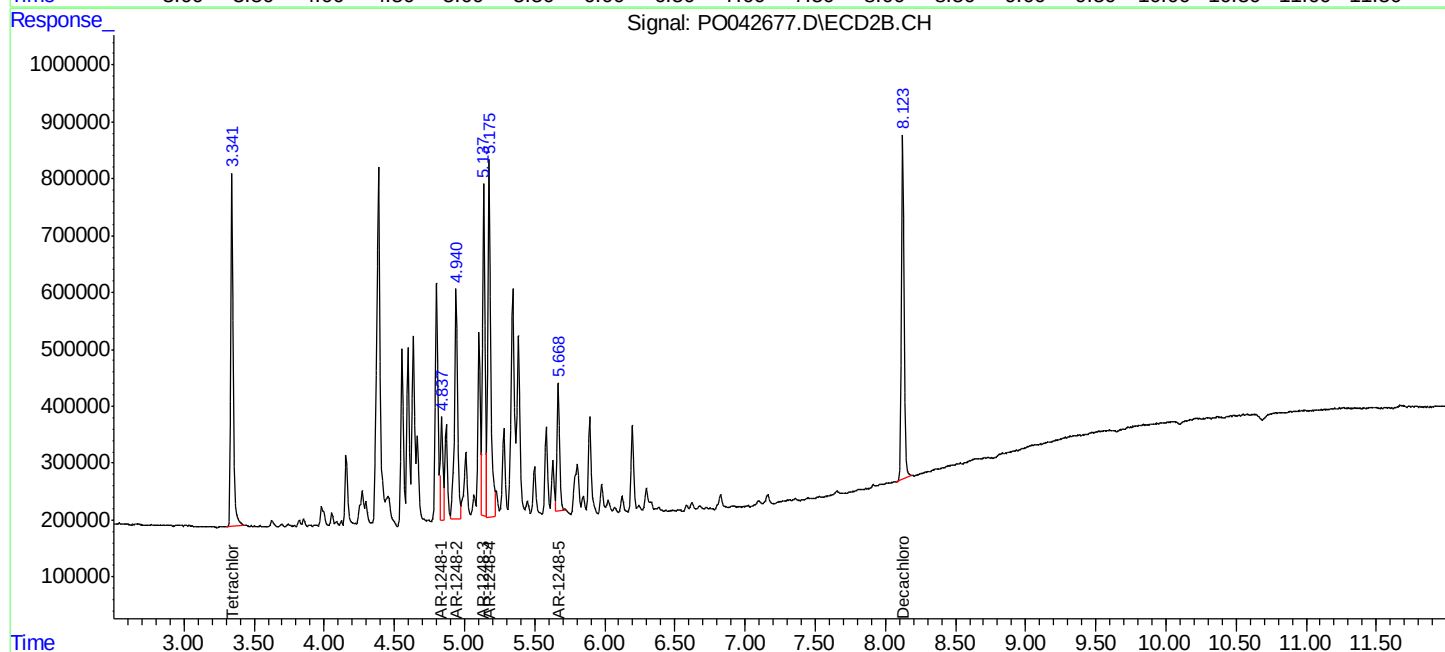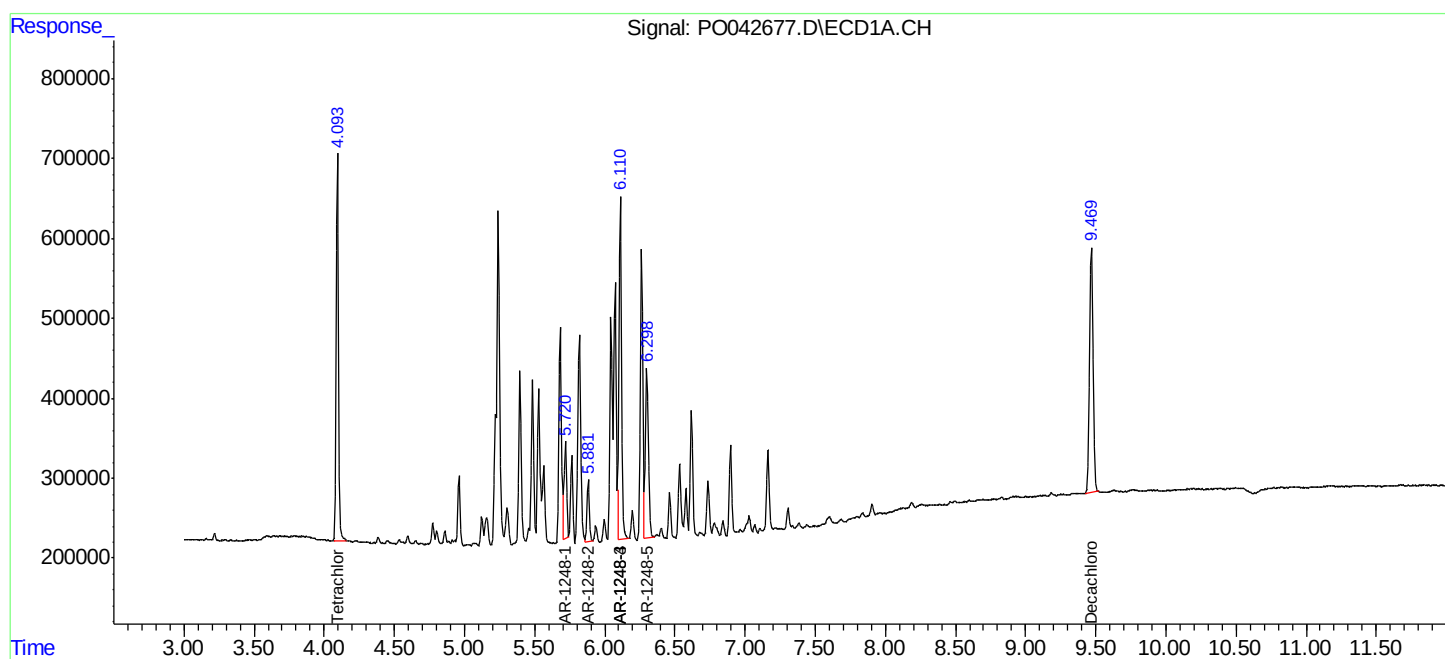

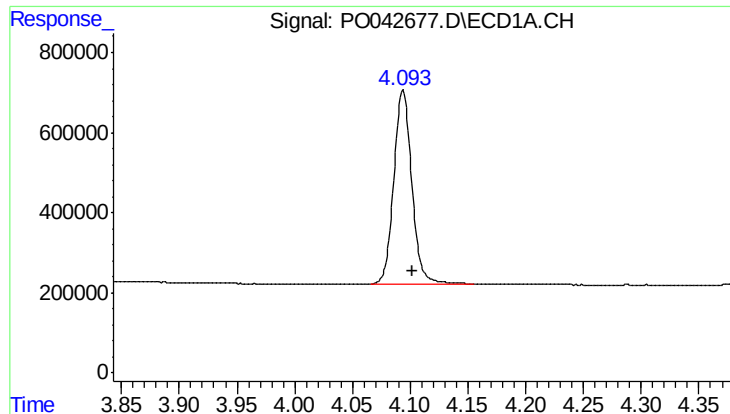


#1 Tetrachloro-m-xylene

R.T.: 4.094 min
Delta R.T.: -0.008 min
Response: 5277645
Conc: 21.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-2022


Manual Integrations
APPROVED

ugo
3/2/2018 4:51:56 PM

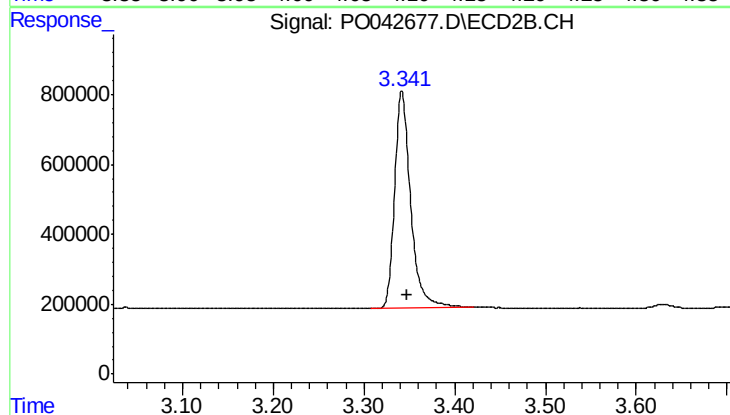


#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: -0.006 min
Response: 7618490
Conc: 20.62 ng/ml

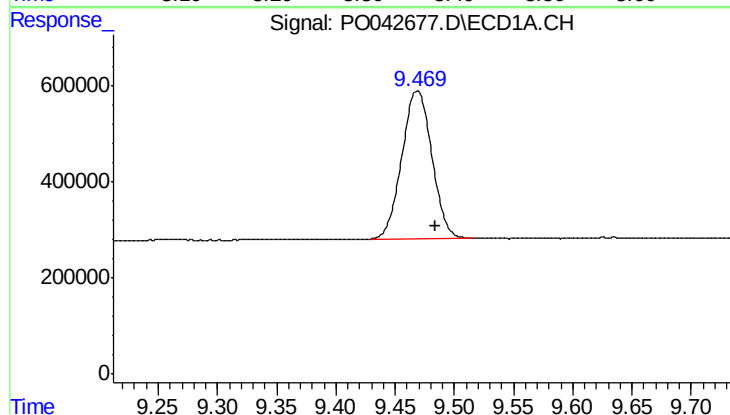


#2 Decachlorobiphenyl

R.T.: 9.469 min
Delta R.T.: -0.015 min
Response: 5423017
Conc: 21.46 ng/ml m

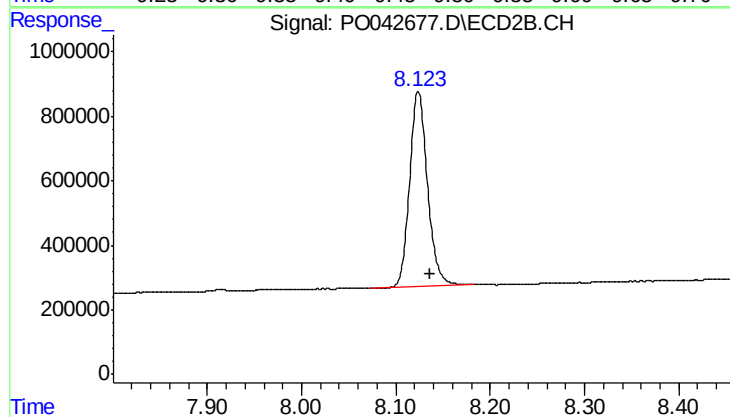

#2 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.013 min
Response: 7959744
Conc: 20.64 ng/ml

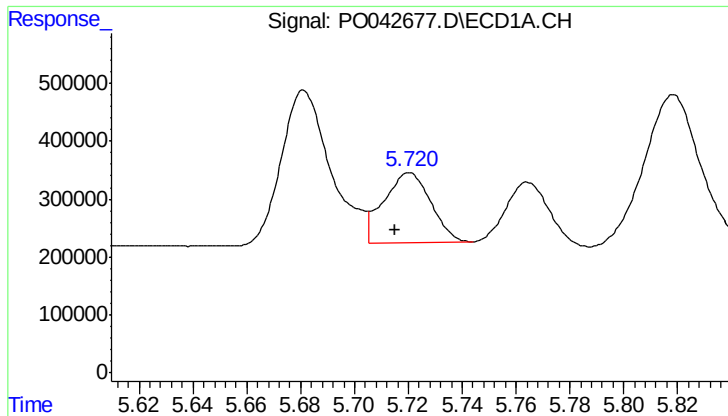


#21 AR-1248-1

R.T.: 5.720 min
Delta R.T.: 0.005 min
Response: 1480556
Conc: 204.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-2022


Manual Integrations
APPROVED

ugo
3/2/2018 4:51:56 PM

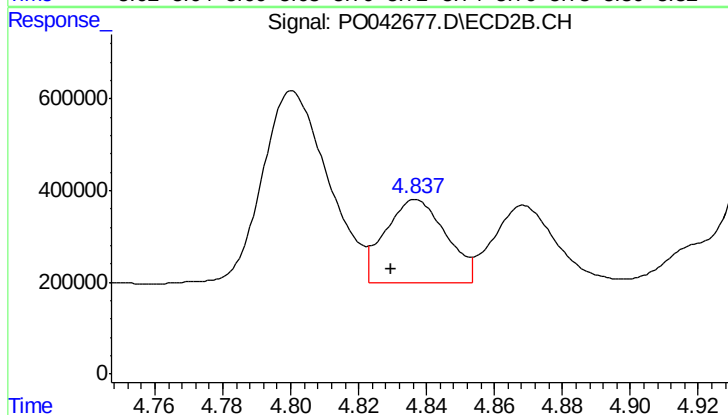


#21 AR-1248-1

R.T.: 4.837 min
Delta R.T.: 0.007 min
Response: 2237207
Conc: 204.65 ng/ml

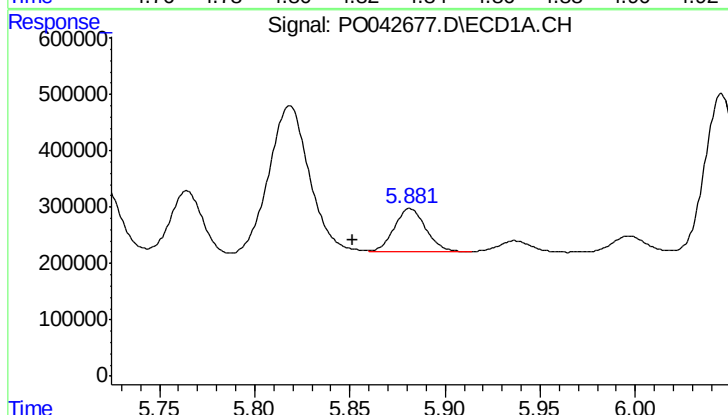


#22 AR-1248-2

R.T.: 5.882 min
Delta R.T.: 0.030 min
Response: 894744
Conc: 142.72 ng/ml

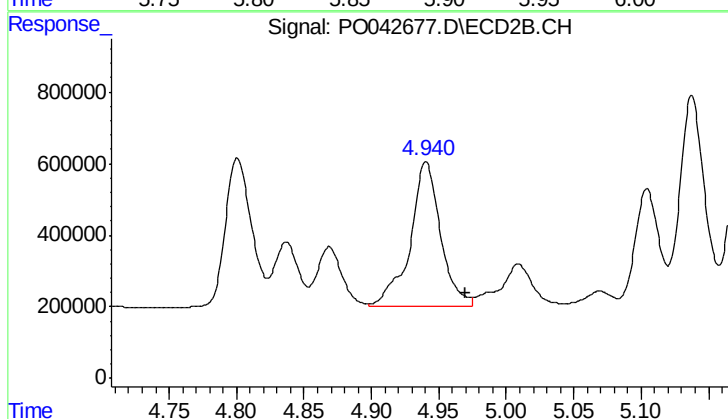

#22 AR-1248-2

R.T.: 4.941 min
Delta R.T.: -0.029 min
Response: 6350579
Conc: 653.11 ng/ml

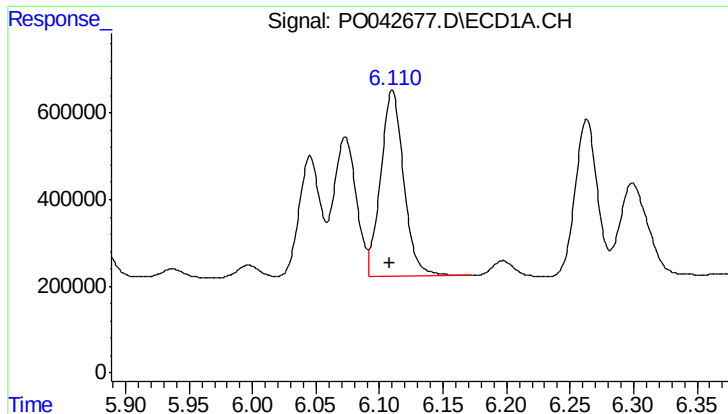


#23 AR-1248-3

R.T.: 6.110 min
Delta R.T.: 0.002 min
Response: 5440344
Conc: 594.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-2022


Manual Integrations
APPROVED

ugo
3/2/2018 4:51:56 PM

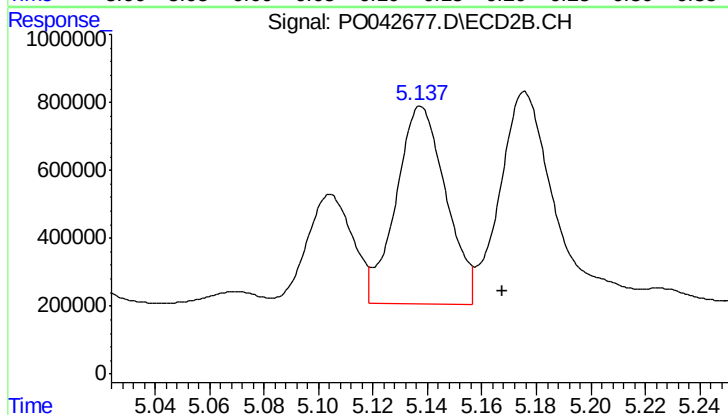


#23 AR-1248-3

R.T.: 5.137 min
Delta R.T.: -0.030 min
Response: 7351551
Conc: 433.45 ng/ml m

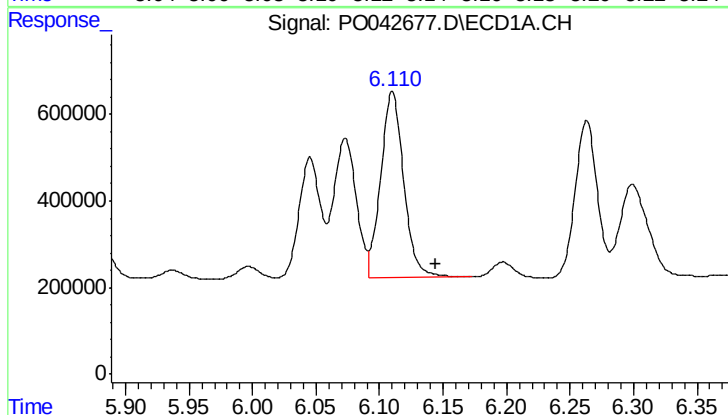


#24 AR-1248-4

R.T.: 6.110 min
Delta R.T.: -0.035 min
Response: 5440344
Conc: 607.10 ng/ml

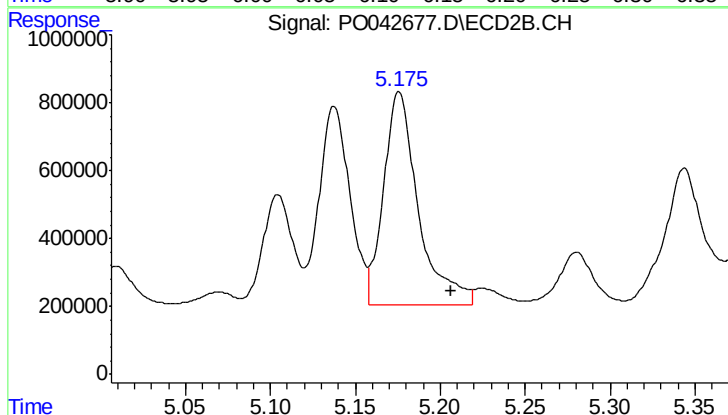

#24 AR-1248-4

R.T.: 5.176 min
Delta R.T.: -0.031 min
Response: 8902951
Conc: 659.36 ng/ml

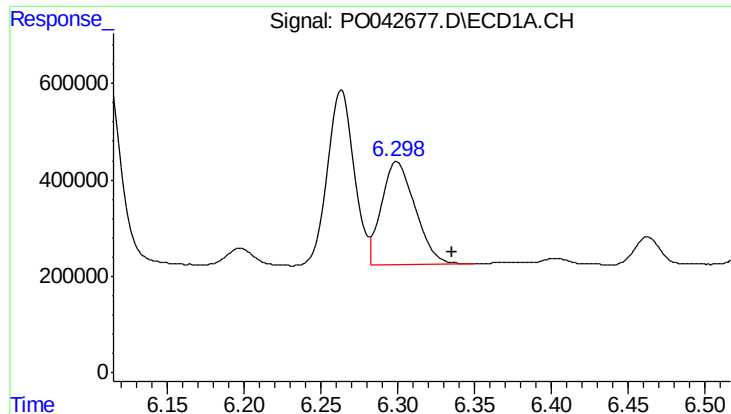


#25 AR-1248-5

R.T.: 6.299 min
Delta R.T.: -0.036 min
Response: 3264454
Conc: 546.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
BPS1-SB4003-2022

Manual Integrations
APPROVED

ugo
3/2/2018 4:51:56 PM

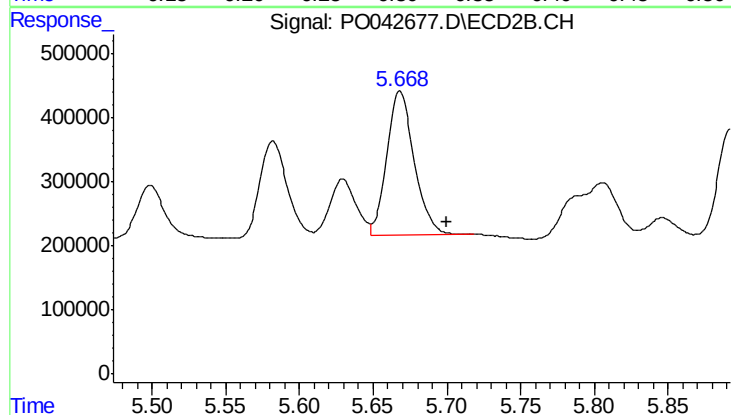

#25 AR-1248-5

R.T.: 5.668 min
Delta R.T.: -0.032 min
Response: 2911523
Conc: 377.85 ng/ml