

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030119\
Data File : P0054173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 13:38
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:58:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.044	3.121	48292364	4826932	22.516	18.828
2) SA Decachlor...	9.372	7.695	21647916	5257719	19.837	19.789

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030119\
Data File : P0054173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 13:38
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:58:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

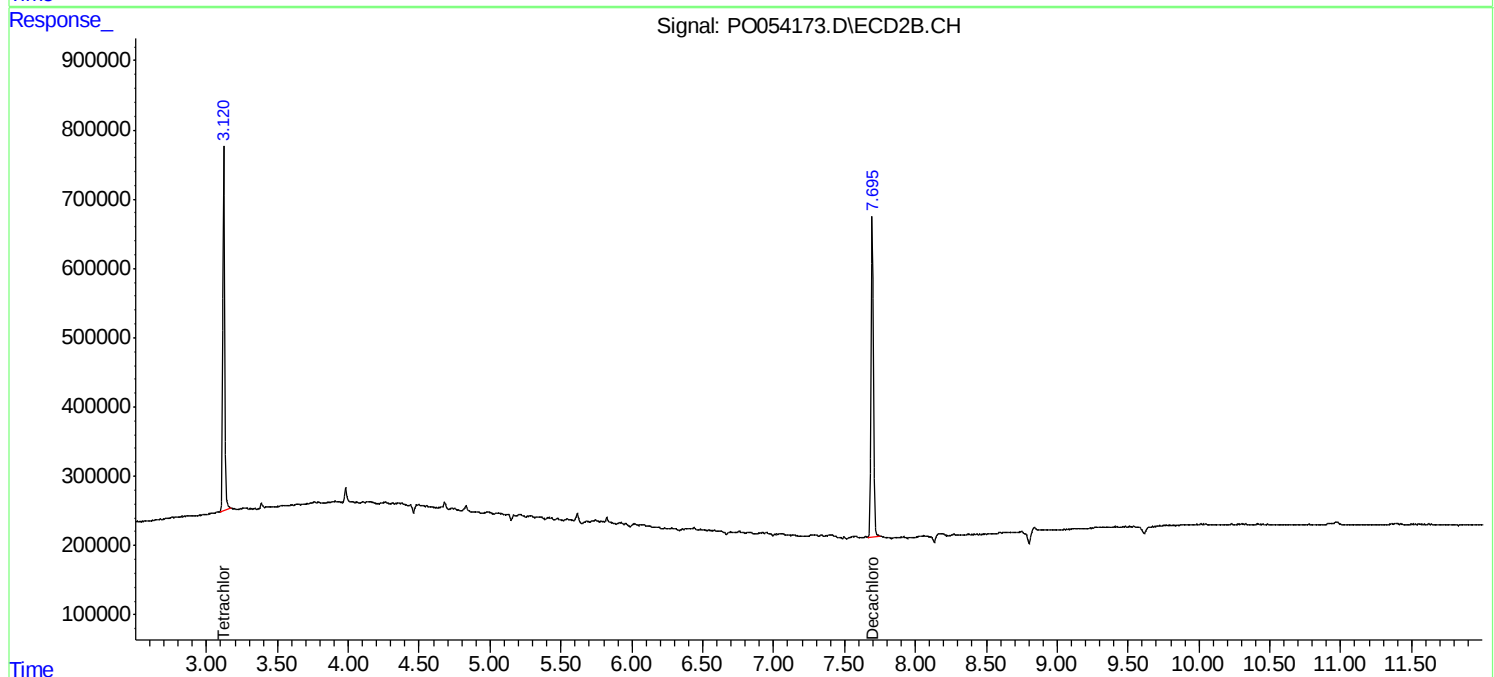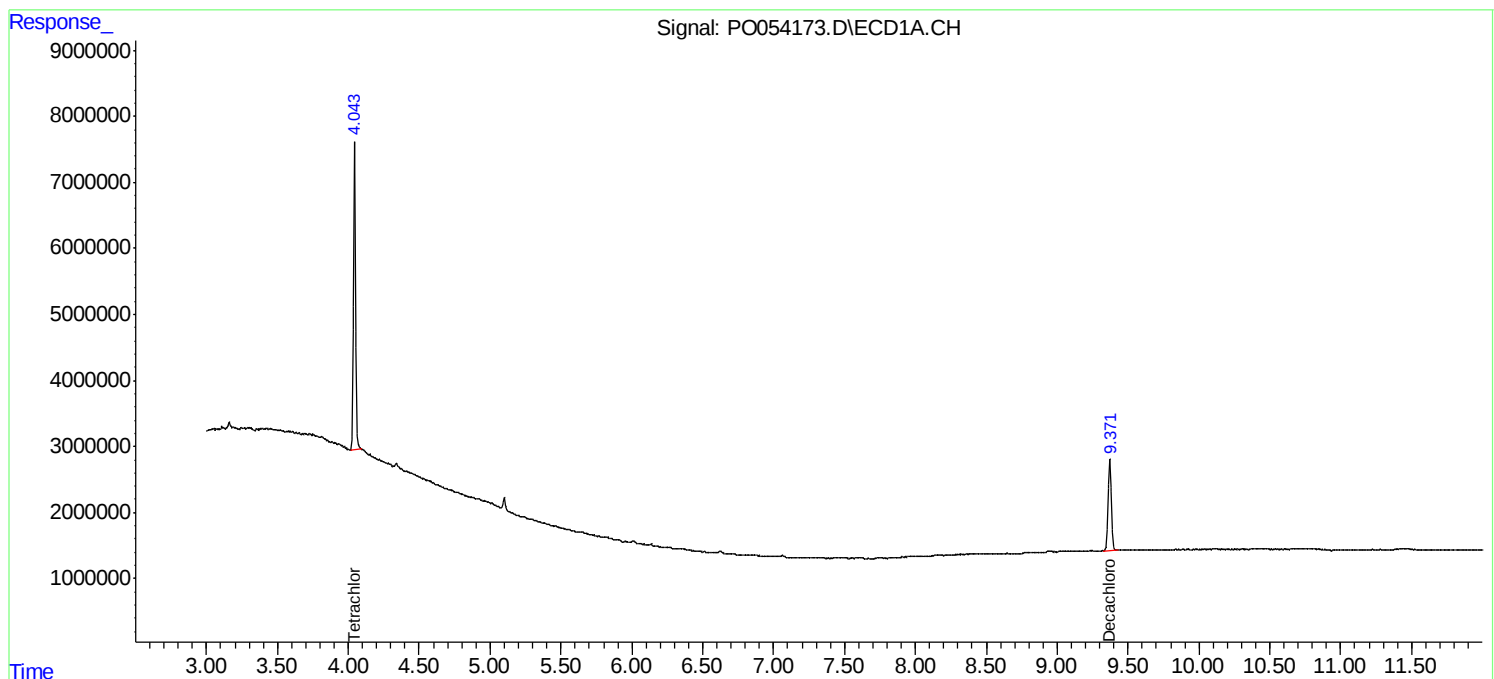


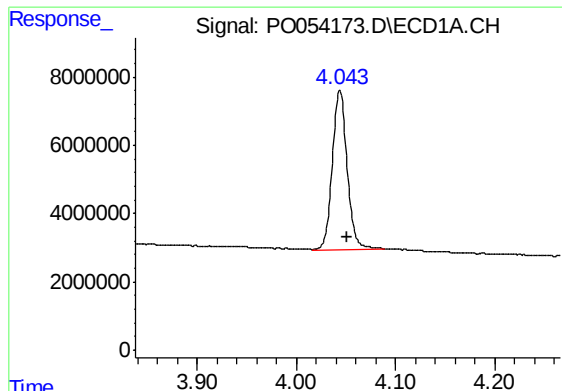

#1 Tetrachloro-m-xylene


R.T.: 4.044 min
Delta R.T.: -0.007 min
Response: 48292364
Conc: 22.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

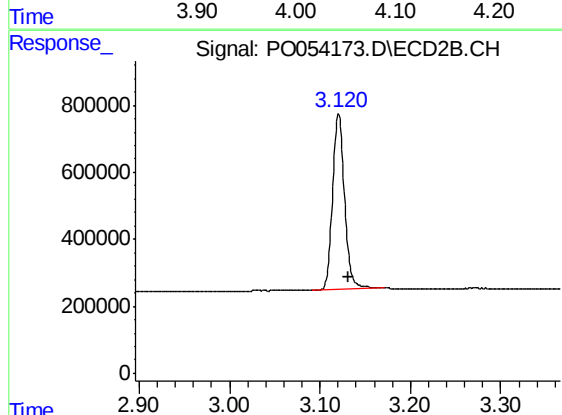


#1 Tetrachloro-m-xylene

R.T.: 3.121 min
Delta R.T.: -0.011 min
Response: 4826932
Conc: 18.83 ng/ml

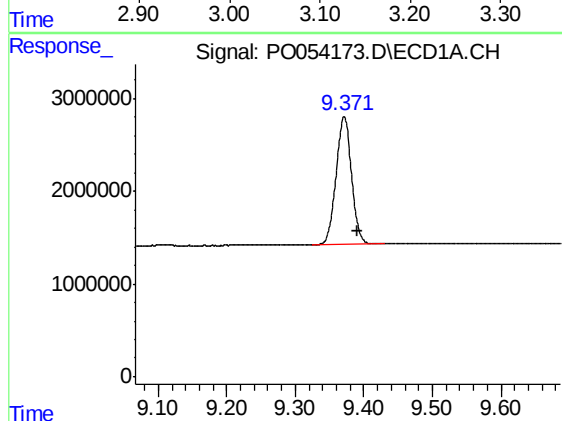

#2 Decachlorobiphenyl

R.T.: 9.372 min
Delta R.T.: -0.019 min
Response: 21647916
Conc: 19.84 ng/ml

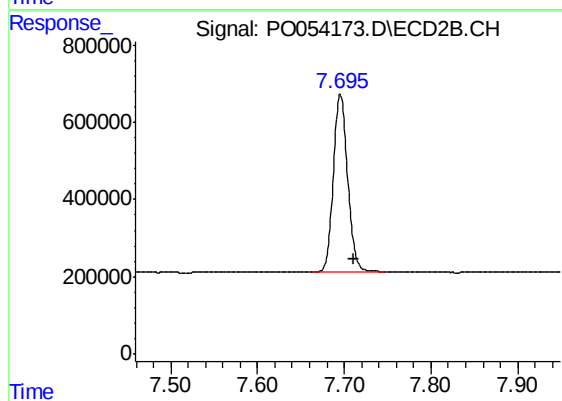

#2 Decachlorobiphenyl

R.T.: 7.695 min
Delta R.T.: -0.015 min
Response: 5257719
Conc: 19.79 ng/ml