

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030119\
Data File : P0054179.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 15:45
Operator : SM/SJ
Sample : K1647-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
44766

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:59:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.037	3.122	48846568	5117730	22.775	19.962
2) SA Decachlor...	9.362	7.693	16928590	4057060	15.512	15.270

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030119\
Data File : PO054179.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 15:45
Operator : SM/SJ
Sample : K1647-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
44766

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 23:59:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

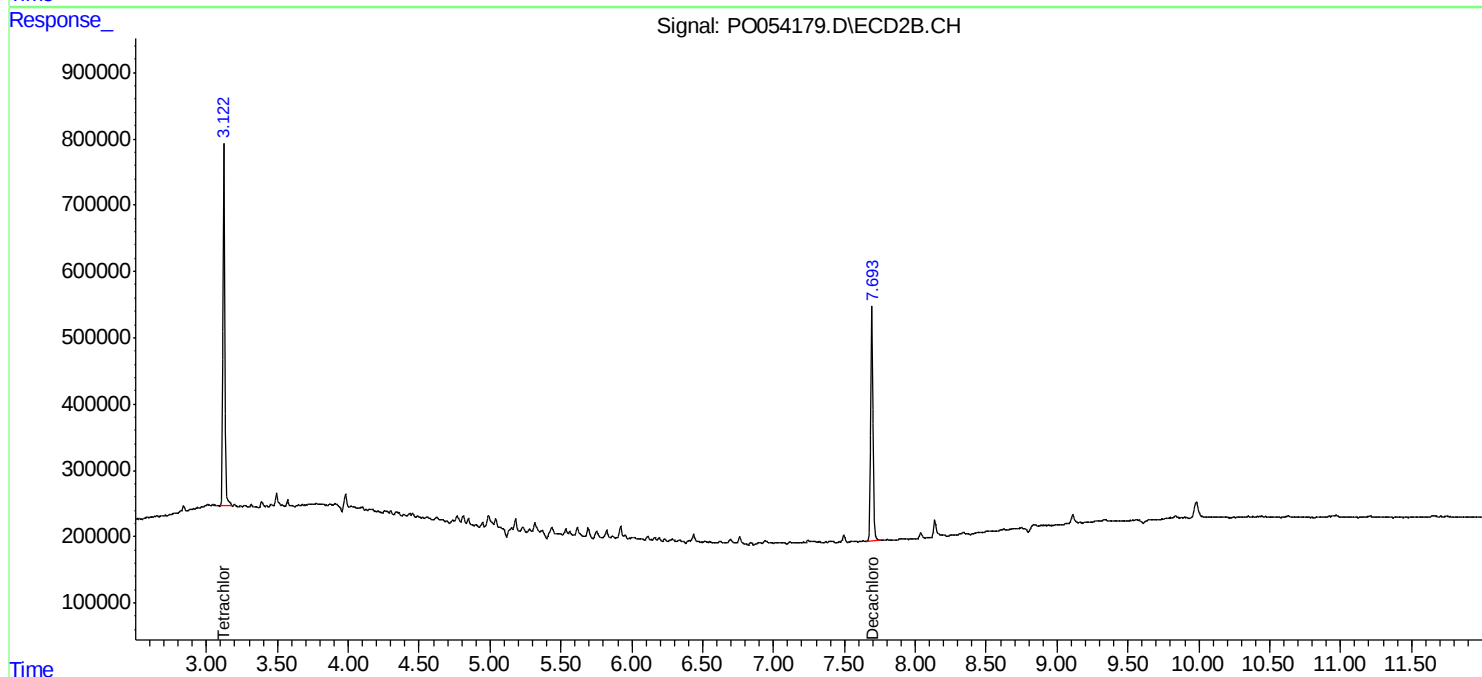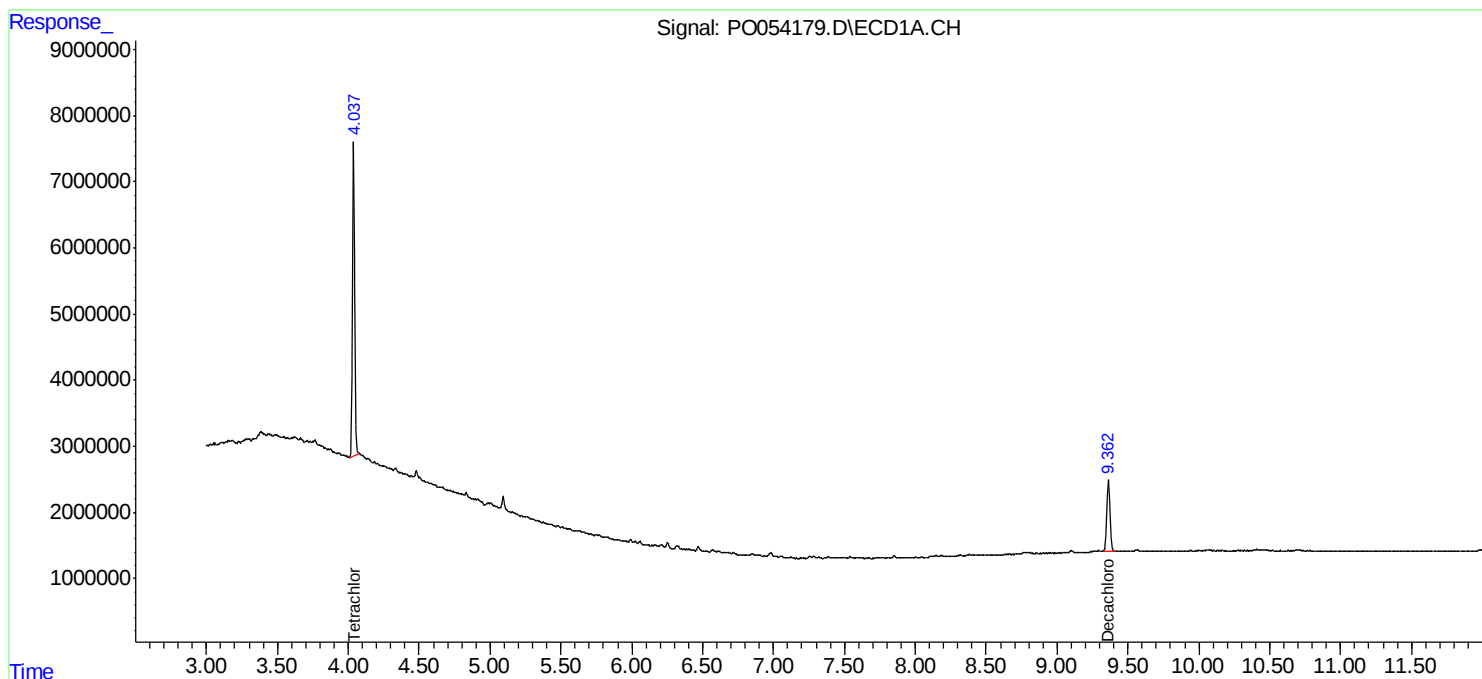


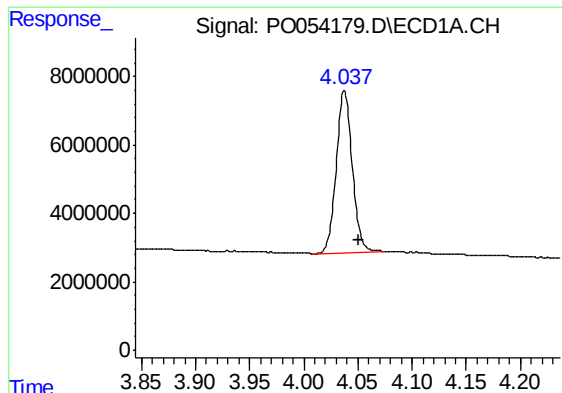

#1 Tetrachloro-m-xylene


R.T.: 4.037 min
Delta R.T.: -0.014 min
Response: 48846568
Conc: 22.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
44766

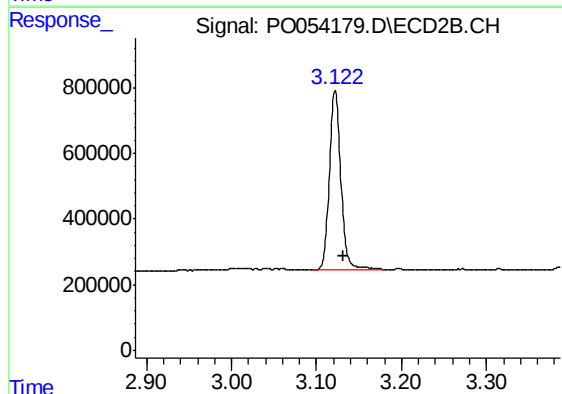


#1 Tetrachloro-m-xylene

R.T.: 3.122 min
Delta R.T.: -0.009 min
Response: 5117730
Conc: 19.96 ng/ml

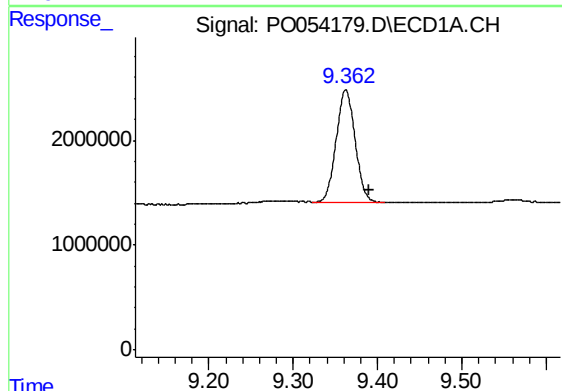

#2 Decachlorobiphenyl

R.T.: 9.362 min
Delta R.T.: -0.028 min
Response: 16928590
Conc: 15.51 ng/ml

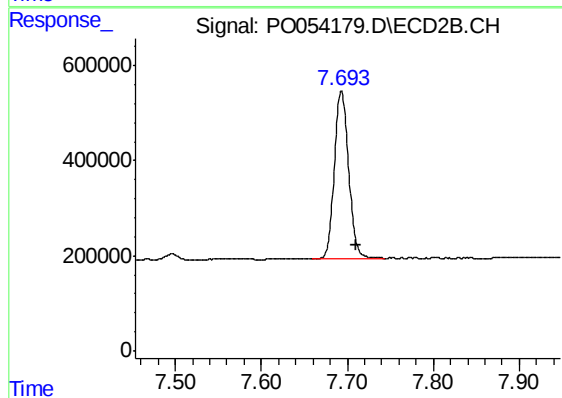

#2 Decachlorobiphenyl

R.T.: 7.693 min
Delta R.T.: -0.018 min
Response: 4057060
Conc: 15.27 ng/ml