

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030119\
 Data File : P0054196.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2019 20:33
 Operator : SM/SJ
 Sample : K1666-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PM-E

Manual Integrations
 APPROVED

Sohil
 3/4/2019 1:54:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:05:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 27 04:24:32 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.036	3.123	49480454	3922959	23.070m	15.302 #
2) SA Decachlor...	9.359	7.692	16252176	3656890	14.893	13.764

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030119\
Data File : PO054196.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2019 20:33
Operator : SM/SJ
Sample : K1666-05
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PM-E


Manual Integrations
APPROVED

Sohil
3/4/2019 1:54:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:05:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 27 04:24:32 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

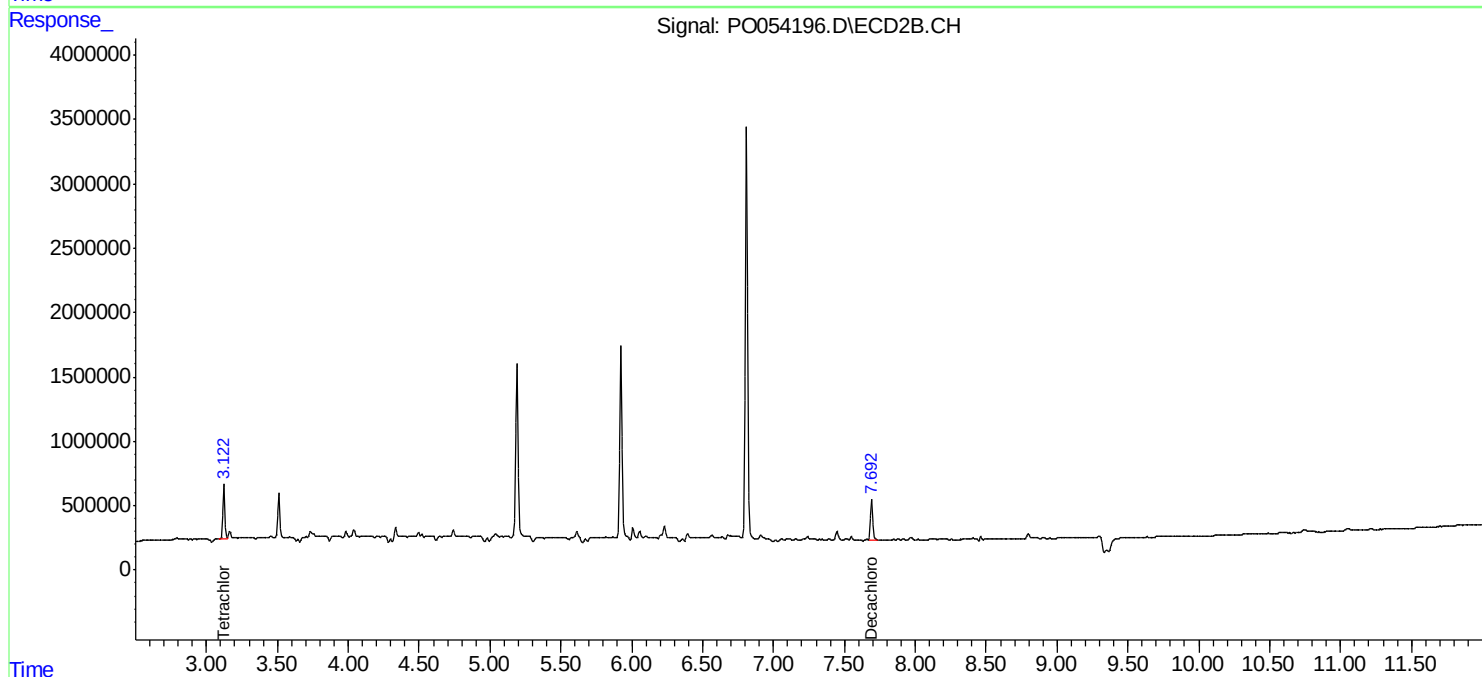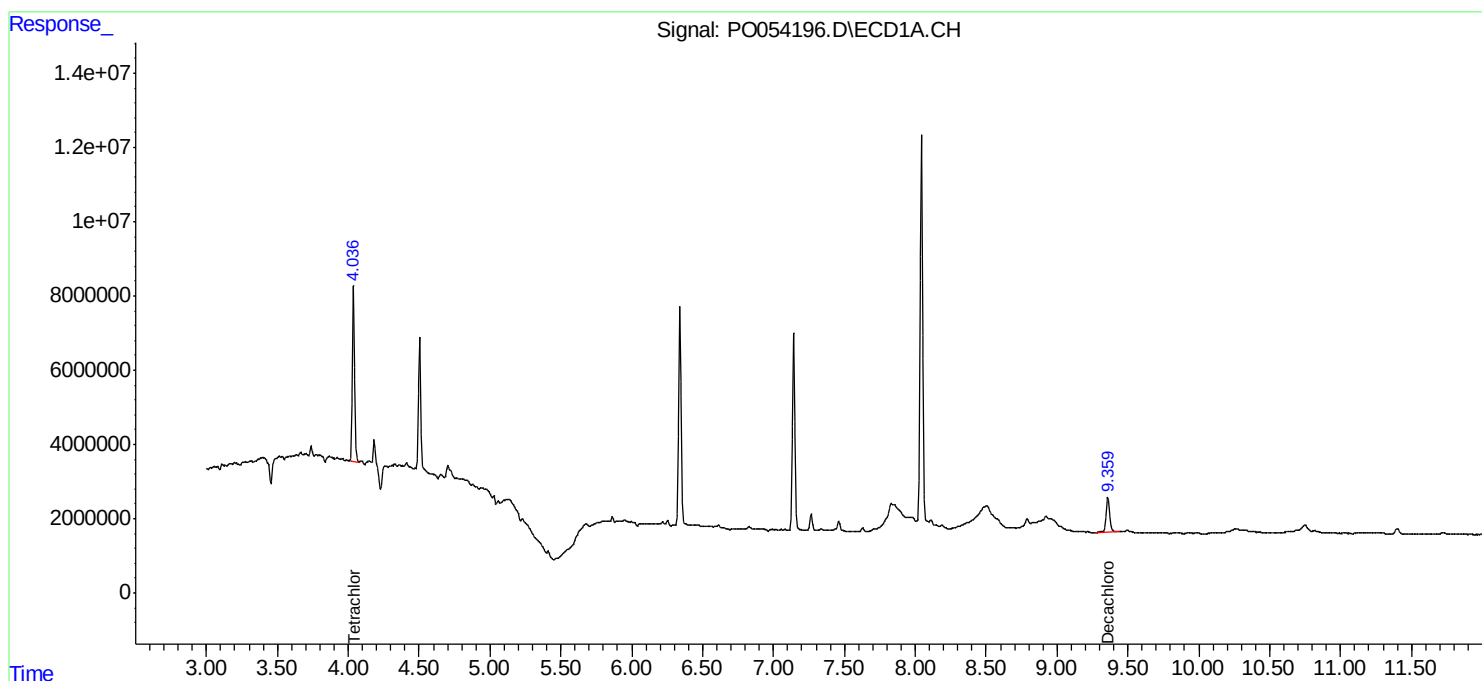

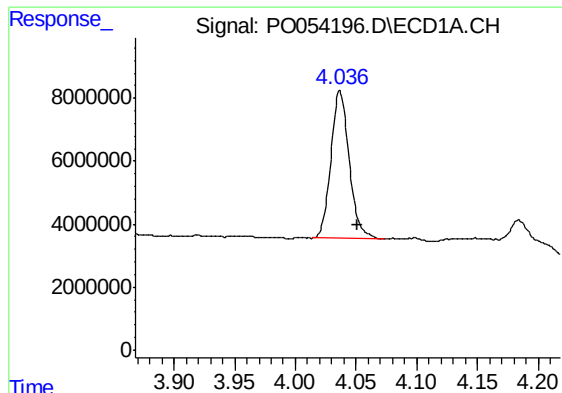


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: -0.015 min
Response: 49480454
Conc: 23.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PM-E


Manual Integrations
APPROVED

Sohil
3/4/2019 1:54:33 PM

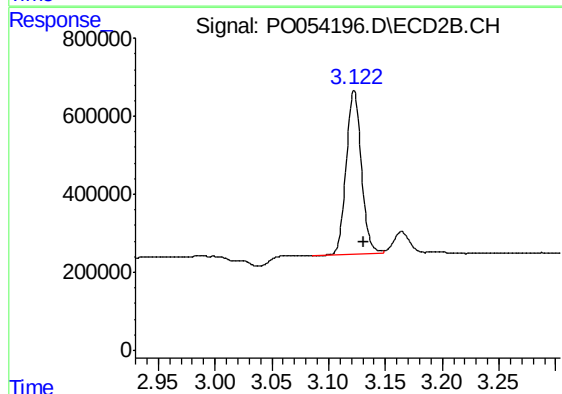


#1 Tetrachloro-m-xylene

R.T.: 3.123 min
Delta R.T.: -0.009 min
Response: 3922959
Conc: 15.30 ng/ml

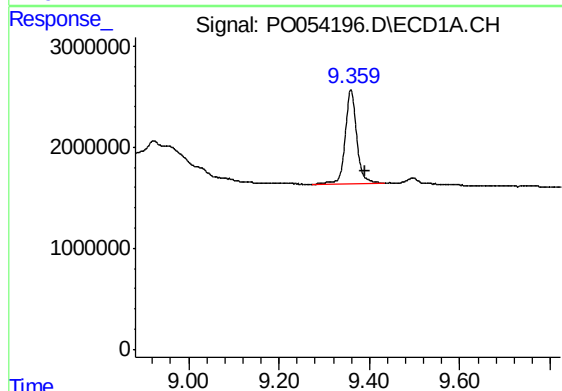

#2 Decachlorobiphenyl

R.T.: 9.359 min
Delta R.T.: -0.031 min
Response: 16252176
Conc: 14.89 ng/ml

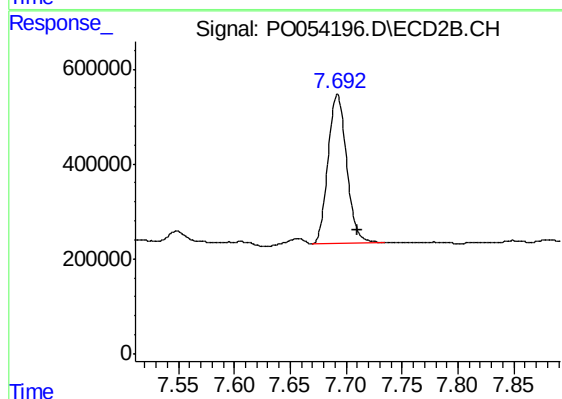

#2 Decachlorobiphenyl

R.T.: 7.692 min
Delta R.T.: -0.018 min
Response: 3656890
Conc: 13.76 ng/ml