

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
 Data File : P0066887.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2020 12:57
 Operator : DD\AJ
 Sample : L1738-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-G0-G1-G0A-G1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 14:20:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 26 14:12:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.121	3.402	991554	1026753	24.316	23.249
2) SA Decachlor...	9.594	8.285	1188896	1205515	24.372	23.965
Target Compounds						
9) L2 AR-1221-2	0.000	3.695	0	16074	N.D.	46.545 #
32) L7 AR-1260-2	0.000	6.091	0	15256	N.D.	4.871 #
33) L7 AR-1260-3	0.000	6.308	0	13259	N.D.	4.507 #
35) L7 AR-1260-5	0.000	7.012	0	8009	N.D.	1.291 #
37) L8 AR-1262-2	0.000	7.012	0	8009	N.D.	1.387 #
38) L8 AR-1262-3	0.000	7.241	0	24584	N.D.	10.171 #
39) L8 AR-1262-4	0.000	7.241	0	24584	N.D.	5.545 #
40) L8 AR-1262-5	0.000	7.852	0	9743	N.D.	4.800 #
41) L9 AR-1268-1	0.000	7.241	0	24584	N.D.	3.412 #
42) L9 AR-1268-2	0.000	7.241	0	24584	N.D.	3.693 #
43) L9 AR-1268-3	0.000	7.500	0	22421	N.D.	4.049 #
44) L9 AR-1268-4	0.000	7.852	0	9743	N.D.	4.004 #
45) L9 AR-1268-5	0.000	8.061	0	25803	N.D.	1.468 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
Data File : P0066887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2020 12:57
Operator : DD\AJ
Sample : L1738-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 14:20:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 26 14:12:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

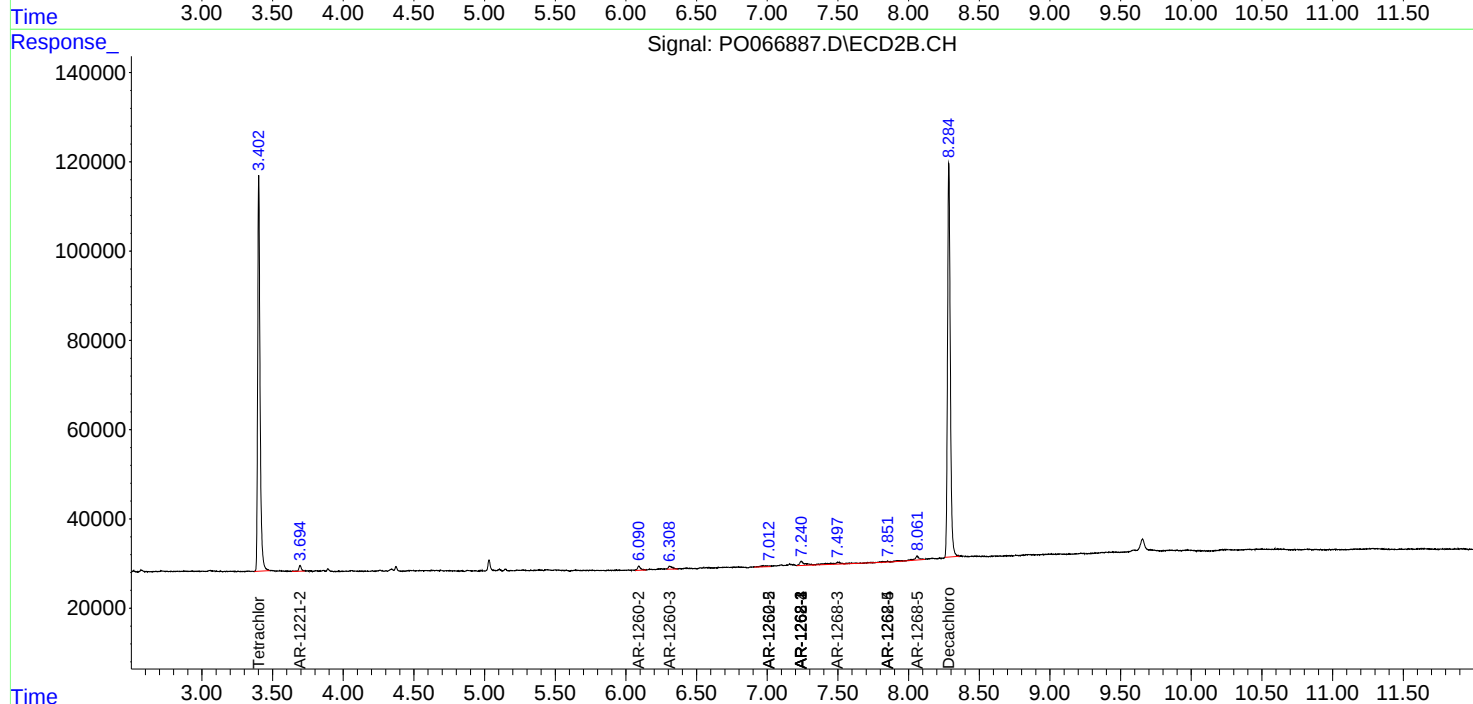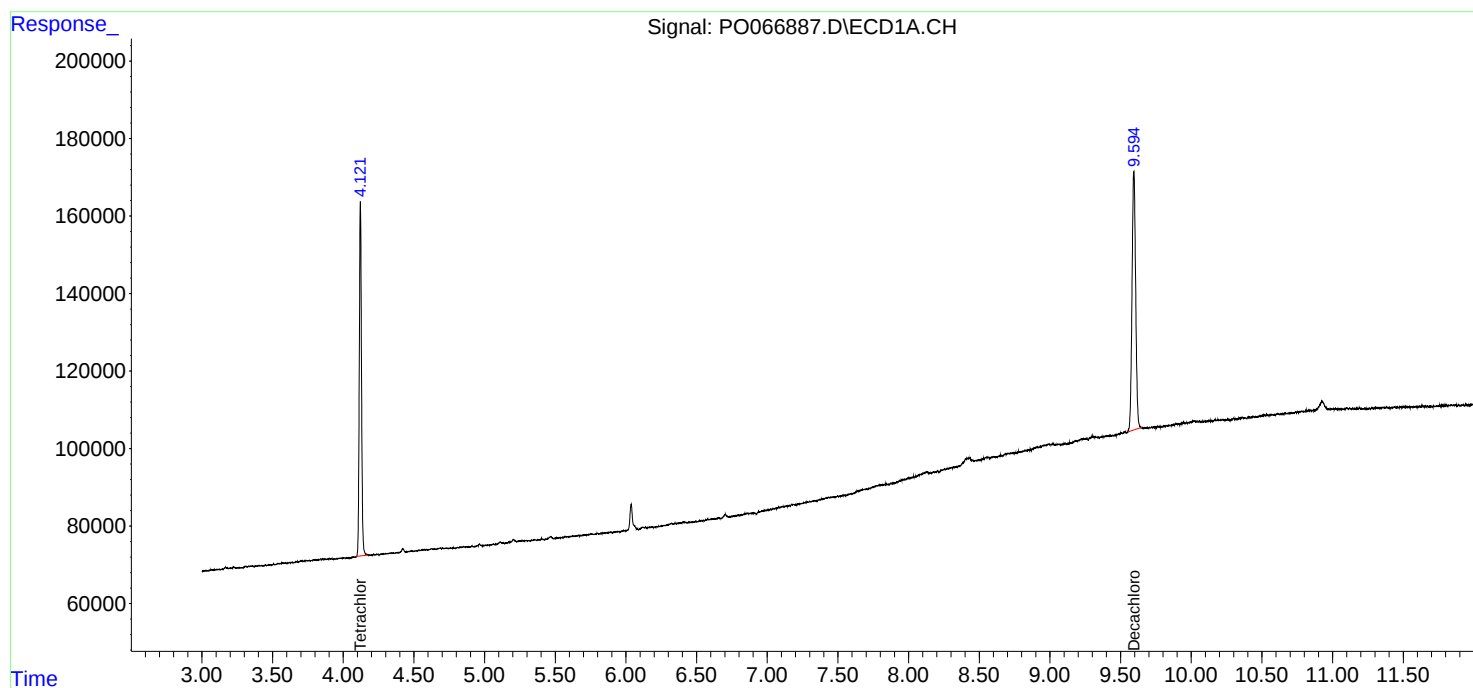


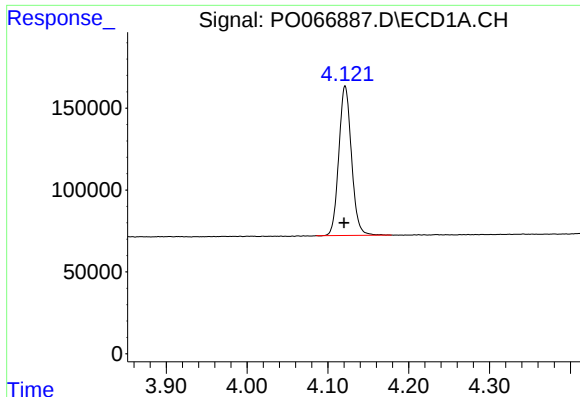

#1 Tetrachloro-m-xylene


R.T.: 4.121 min
Delta R.T.: 0.001 min
Response: 991554
Conc: 24.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

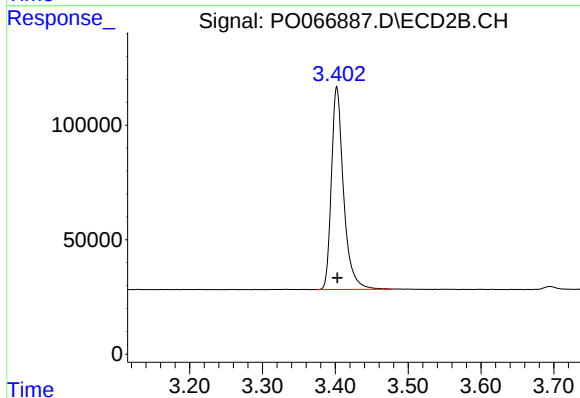


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 1026753
Conc: 23.25 ng/ml

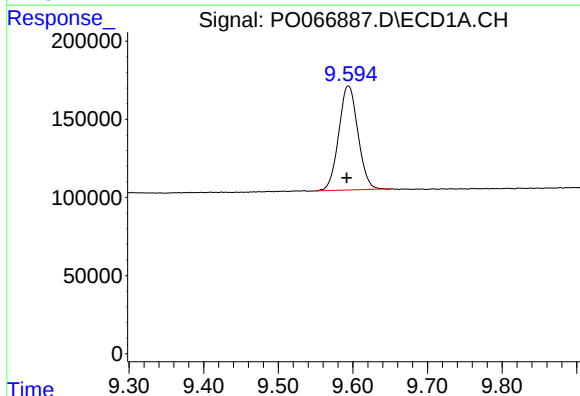


#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: 0.002 min
Response: 1188896
Conc: 24.37 ng/ml

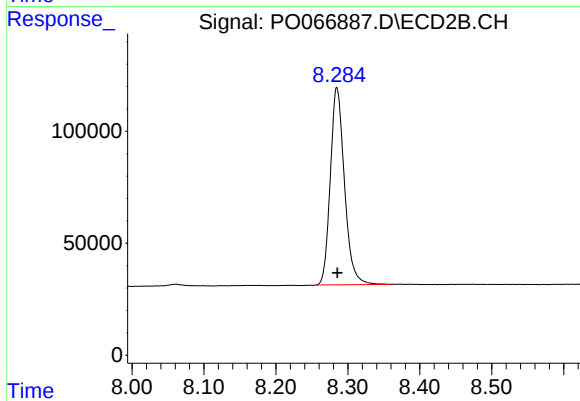

#2 Decachlorobiphenyl


R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 1205515
Conc: 23.96 ng/ml

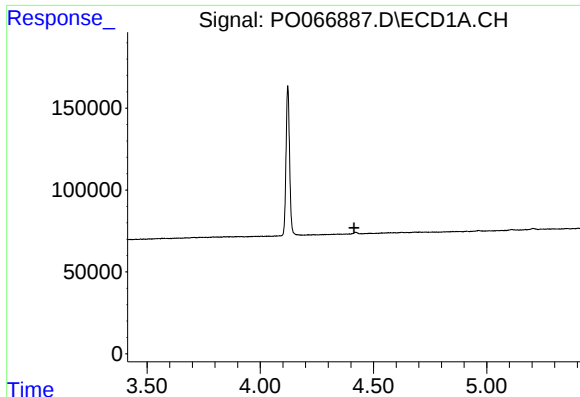

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

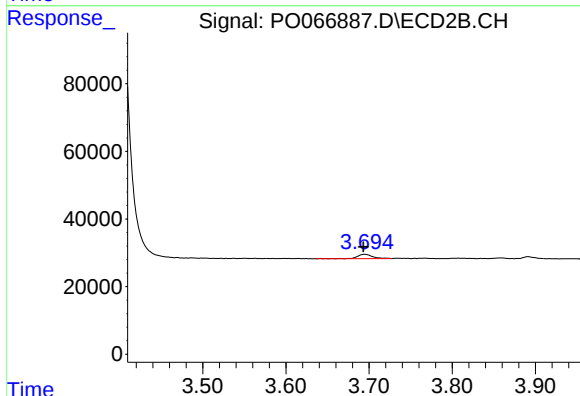


#9 AR-1221-2

R.T.: 3.695 min
Delta R.T.: 0.002 min
Response: 16074
Conc: 46.54 ng/ml

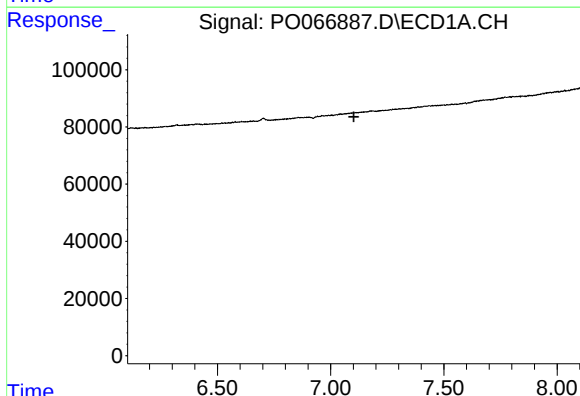


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.102 min
Response: 0
Conc: N.D.

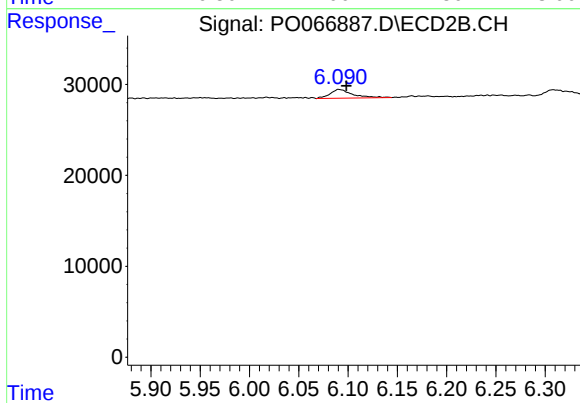

#32 AR-1260-2


R.T.: 6.091 min
Delta R.T.: -0.007 min
Response: 15256
Conc: 4.87 ng/ml

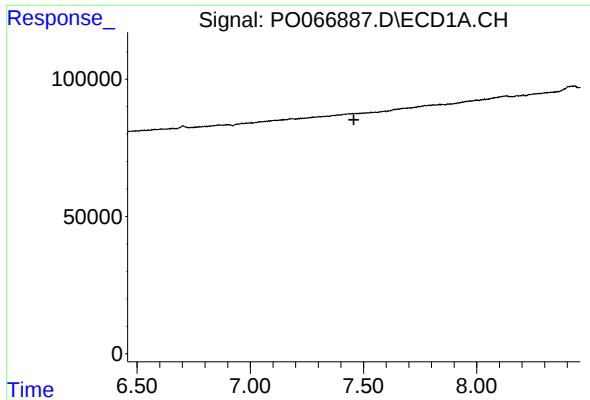

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

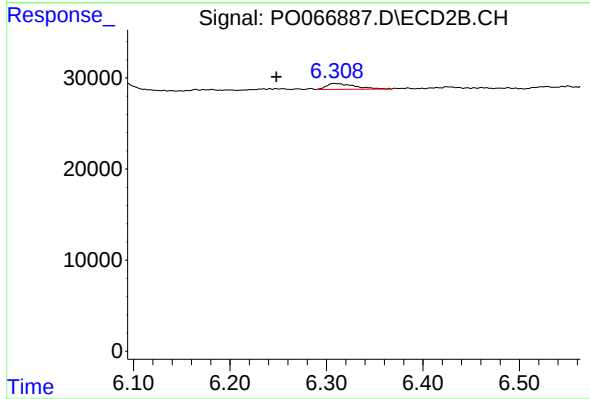


#33 AR-1260-3

R.T.: 6.308 min
Delta R.T.: 0.060 min
Response: 13259
Conc: 4.51 ng/ml

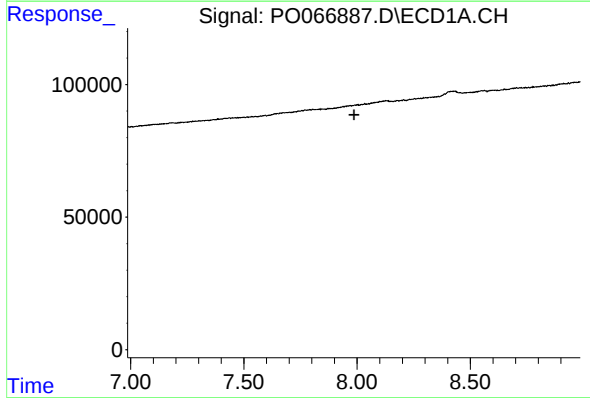


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.986 min
Response: 0
Conc: N.D.

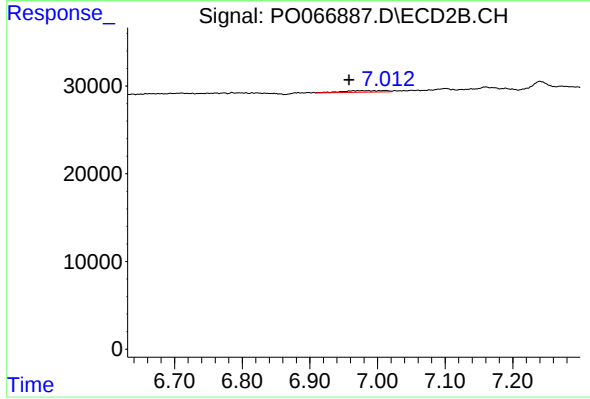

#35 AR-1260-5


R.T.: 7.012 min
Delta R.T.: 0.054 min
Response: 8009
Conc: 1.29 ng/ml

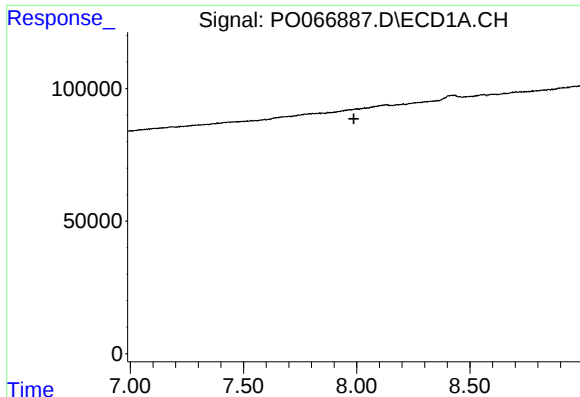

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.987 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

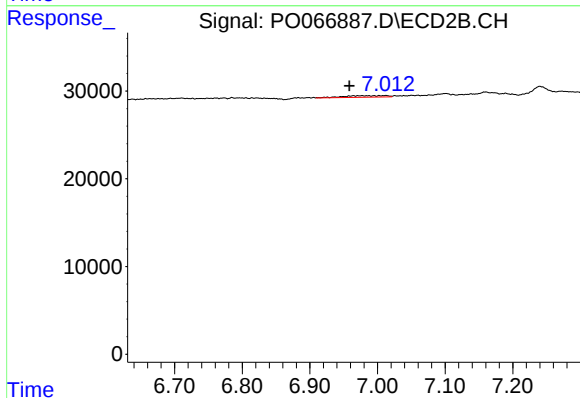


#37 AR-1262-2

R.T.: 7.012 min
Delta R.T.: 0.054 min
Response: 8009
Conc: 1.39 ng/ml

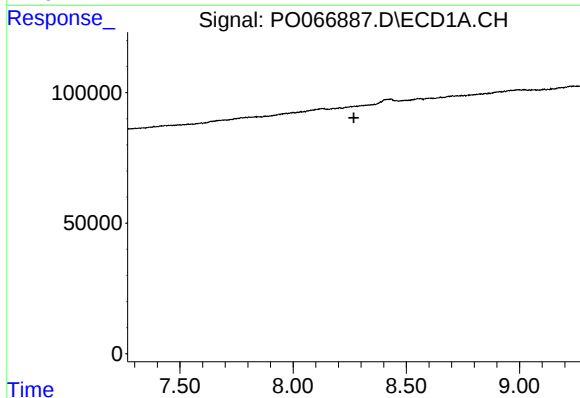


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.268 min
Response: 0
Conc: N.D.

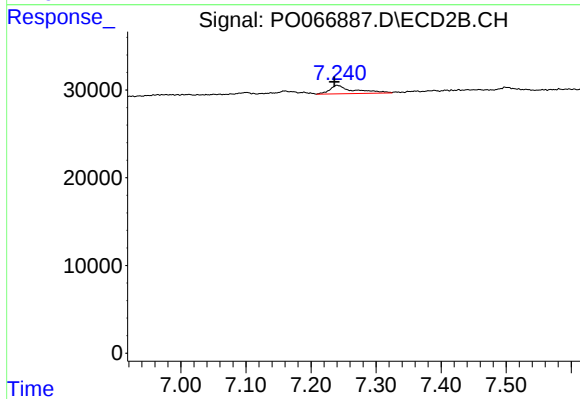

#38 AR-1262-3


R.T.: 7.241 min
Delta R.T.: 0.005 min
Response: 24584
Conc: 10.17 ng/ml

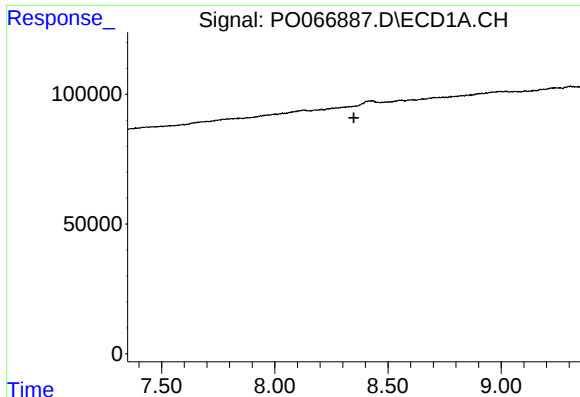

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

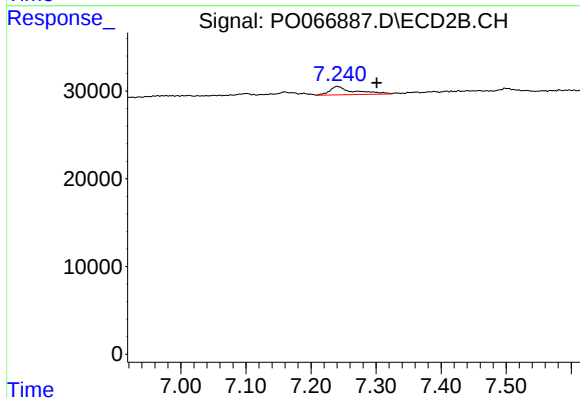


#39 AR-1262-4

R.T.: 7.241 min
Delta R.T.: -0.060 min
Response: 24584
Conc: 5.54 ng/ml

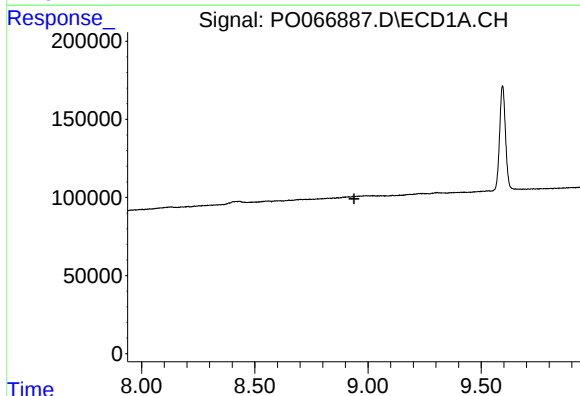


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 8.938 min
Response: 0
Conc: N.D.

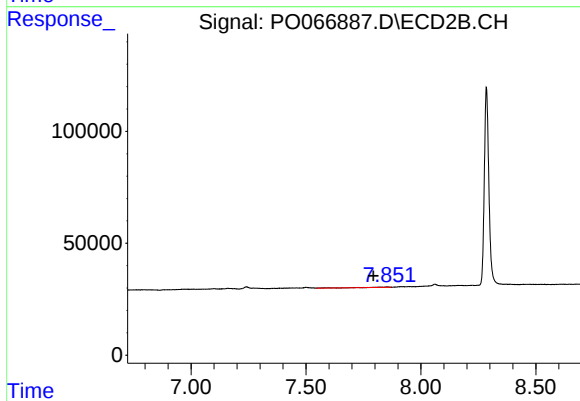

#40 AR-1262-5


R.T.: 7.852 min
Delta R.T.: 0.058 min
Response: 9743
Conc: 4.80 ng/ml

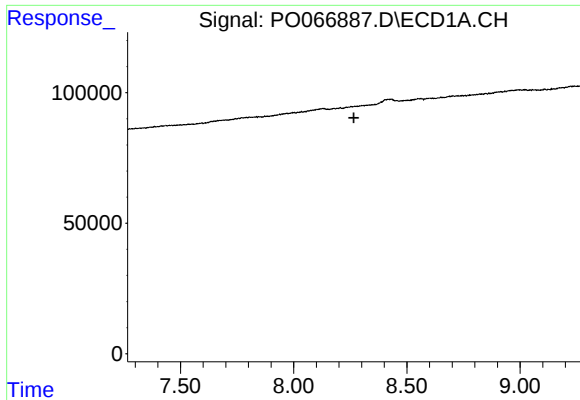

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.266 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

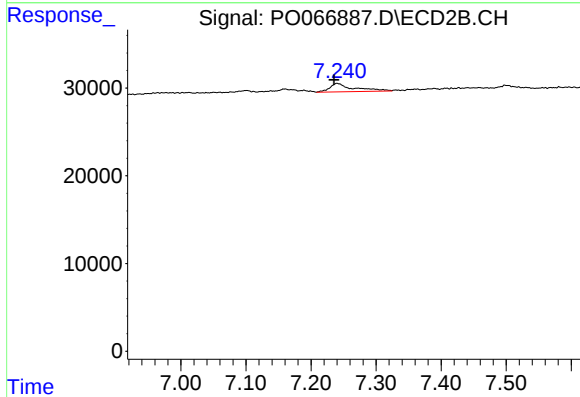


#41 AR-1268-1

R.T.: 7.241 min
Delta R.T.: 0.005 min
Response: 24584
Conc: 3.41 ng/ml

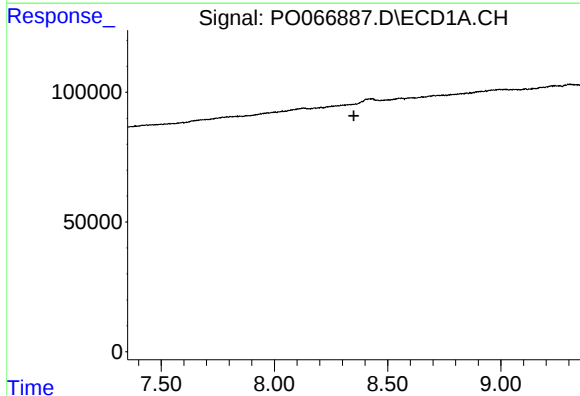


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.351 min
Response: 0
Conc: N.D.

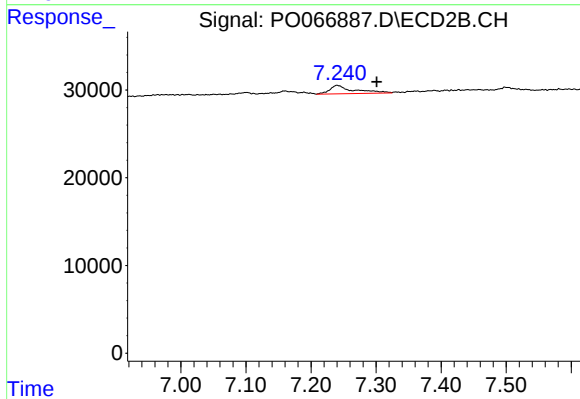

#42 AR-1268-2


R.T.: 7.241 min
Delta R.T.: -0.060 min
Response: 24584
Conc: 3.69 ng/ml

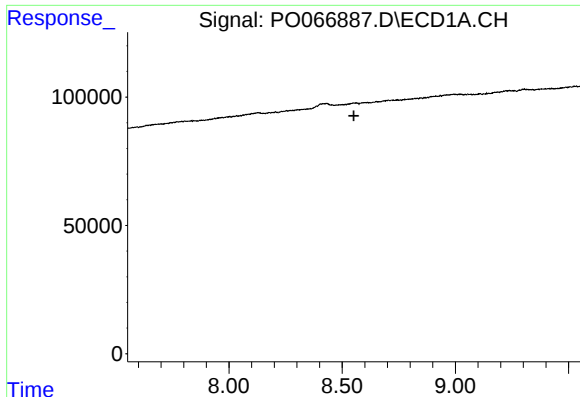

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

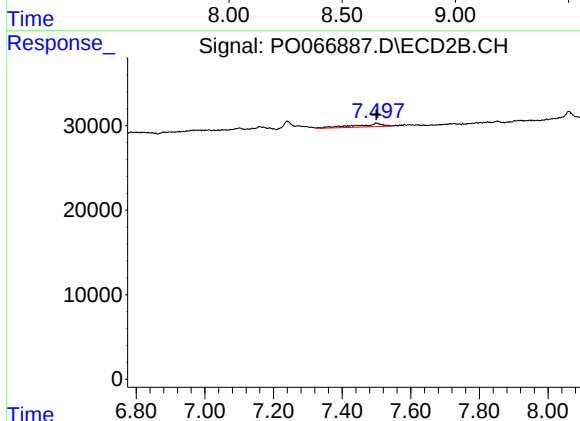


#43 AR-1268-3

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 22421
Conc: 4.05 ng/ml

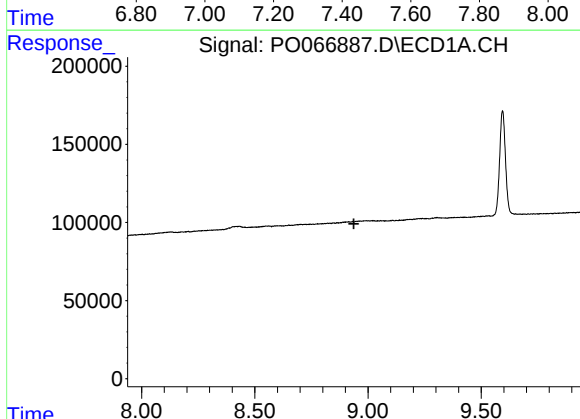


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.938 min
Response: 0
Conc: N.D.

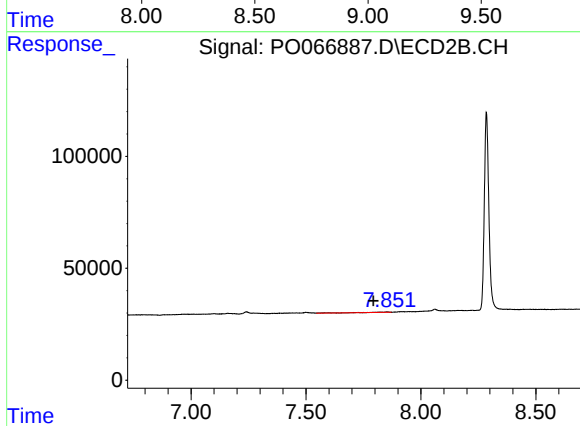

#44 AR-1268-4


R.T.: 7.852 min
Delta R.T.: 0.059 min
Response: 9743
Conc: 4.00 ng/ml

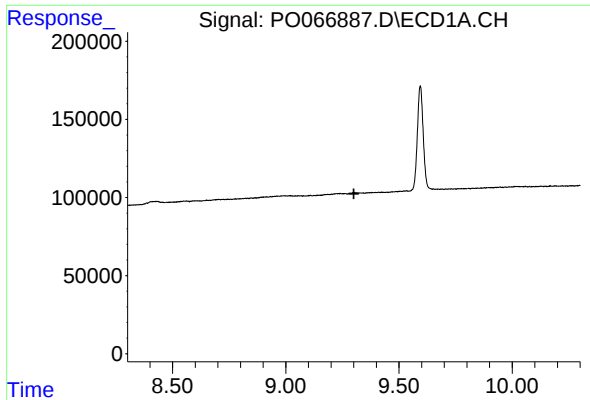

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.301 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

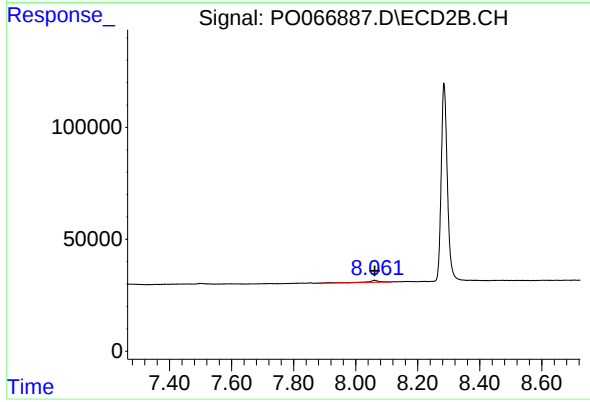

#45 AR-1268-5

R.T.: 8.061 min
Delta R.T.: -0.001 min
Response: 25803
Conc: 1.47 ng/ml