

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
 Data File : P0066886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2020 12:40
 Operator : DD\AJ
 Sample : L1737-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-013-ABCD

Manual Integrations
 APPROVED

Sohil
 3/3/2020 4:44:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 15:33:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 26 14:12:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.135	3.404	978921	967390	24.006	21.905
2) SA Decachlor...	9.613	8.293	1054091	1068421	21.608m	21.240

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
Data File : P0066886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2020 12:40
Operator : DD\AJ
Sample : L1737-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-013-ABCD


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 15:33:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 26 14:12:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

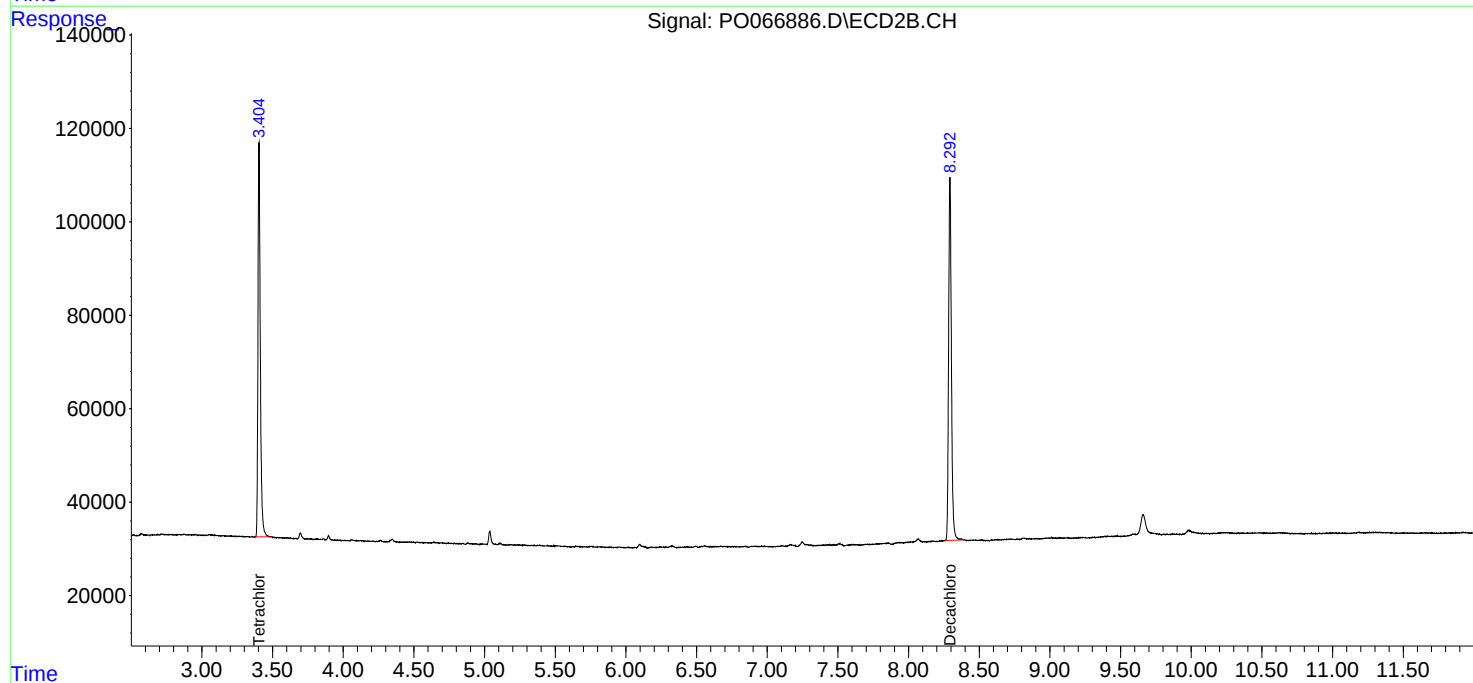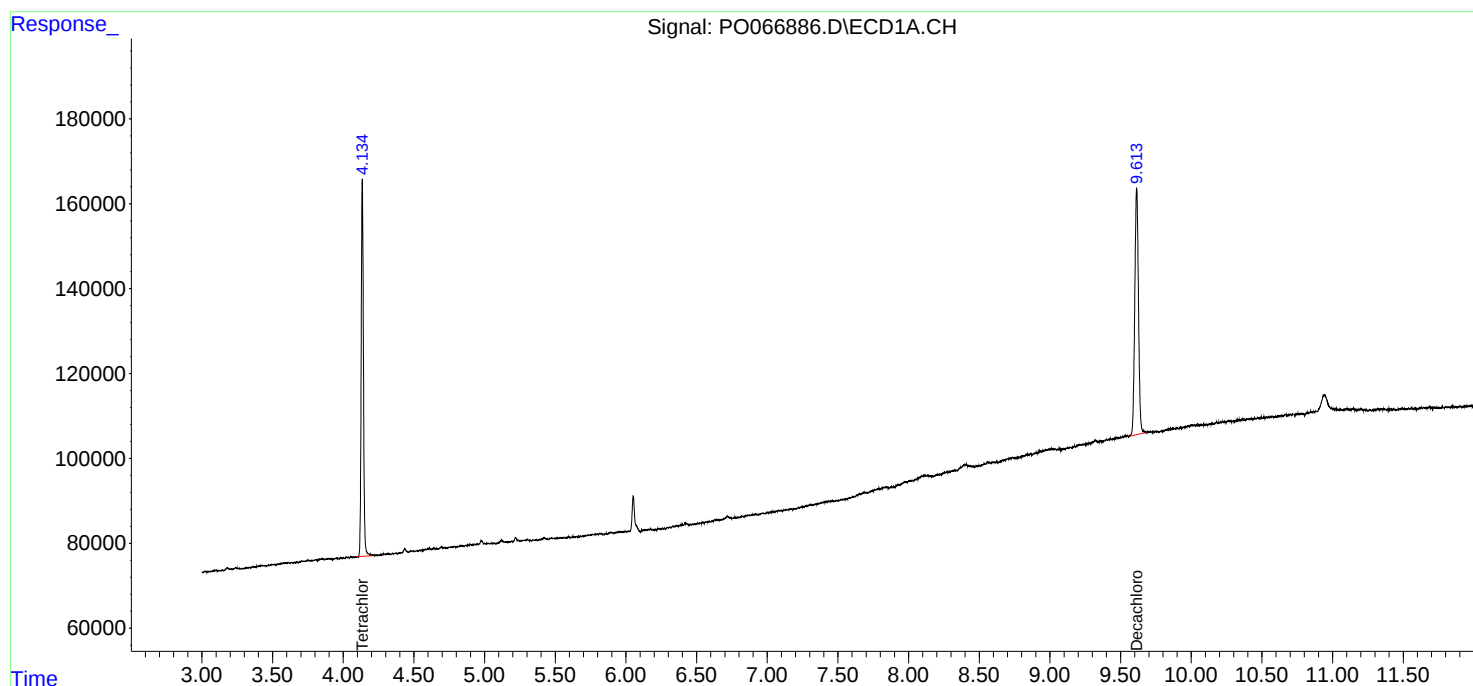

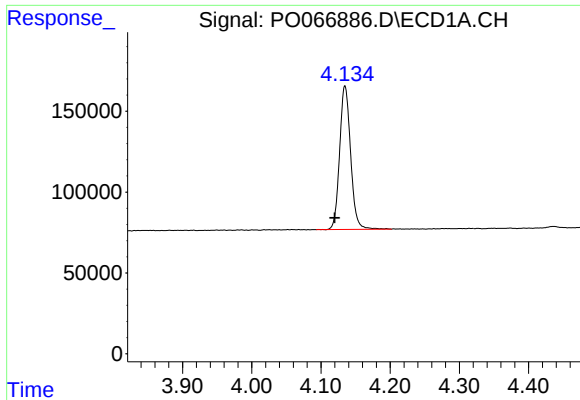


#1 Tetrachloro-m-xylene

R.T.: 4.135 min
Delta R.T.: 0.015 min
Response: 978921
Conc: 24.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-013-ABCD


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:26 PM

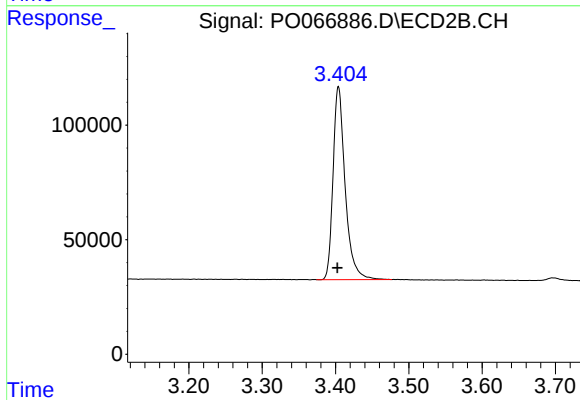


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: 0.001 min
Response: 967390
Conc: 21.91 ng/ml

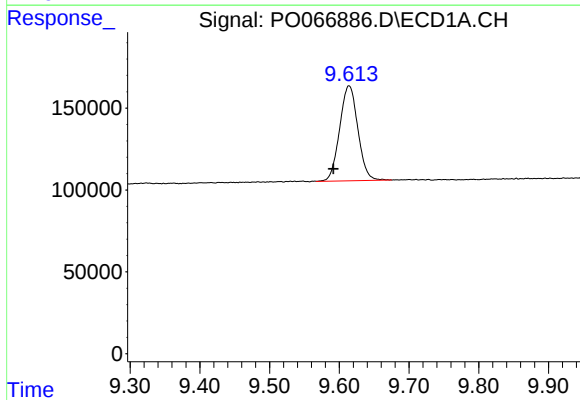

#2 Decachlorobiphenyl

R.T.: 9.613 min
Delta R.T.: 0.022 min
Response: 1054091
Conc: 21.61 ng/ml m

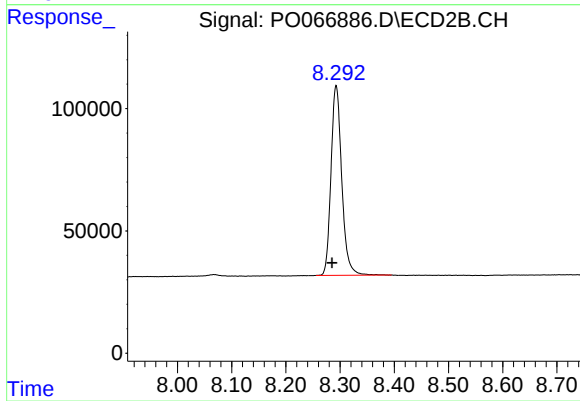

#2 Decachlorobiphenyl

R.T.: 8.293 min
Delta R.T.: 0.008 min
Response: 1068421
Conc: 21.24 ng/ml