

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
 Data File : P0066887.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2020 12:57
 Operator : DD\AJ
 Sample : L1738-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-G0-G1-G0A-G1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 14:20:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 26 14:12:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.121	3.402	991554	1026753	24.316	23.249
2) SA Decachlor...	9.594	8.285	1188896	1205515	24.372	23.965

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
Data File : P0066887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2020 12:57
Operator : DD\AJ
Sample : L1738-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 14:20:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 26 14:12:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

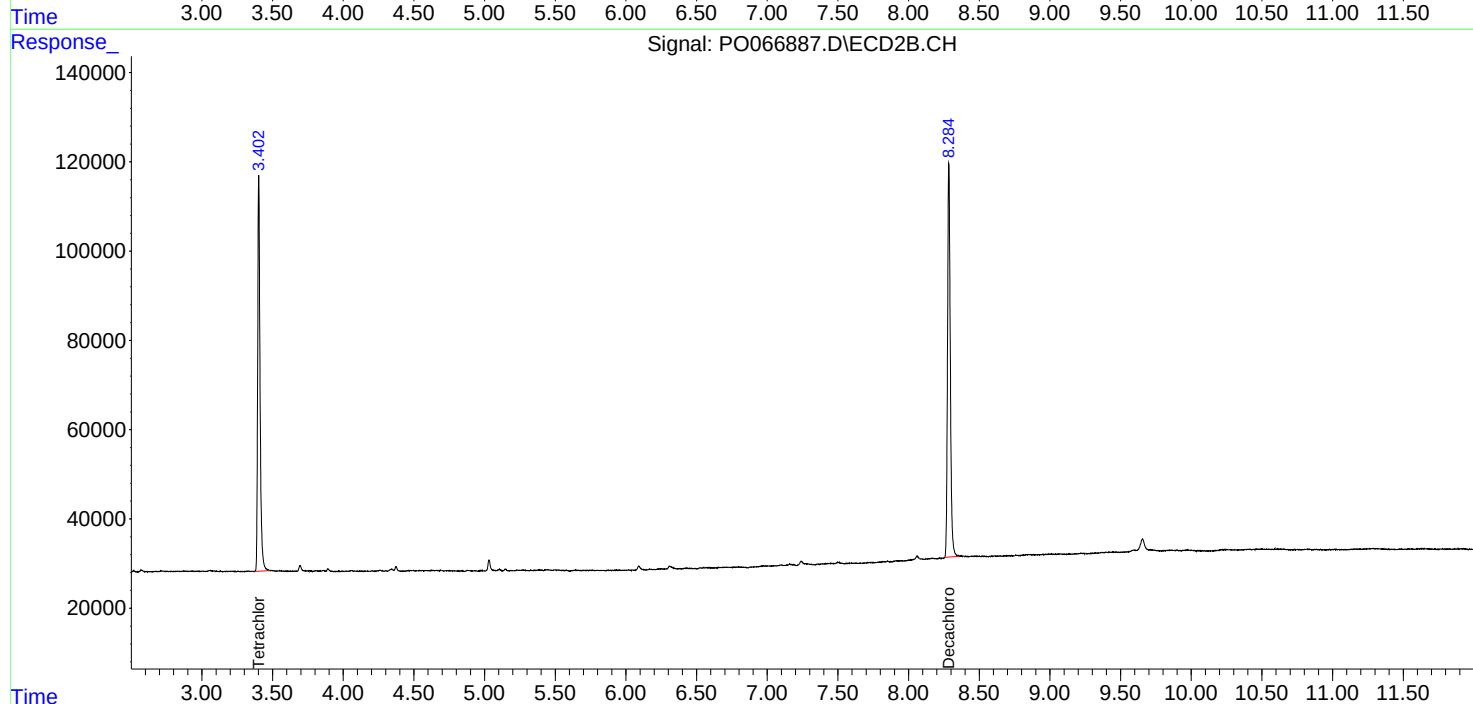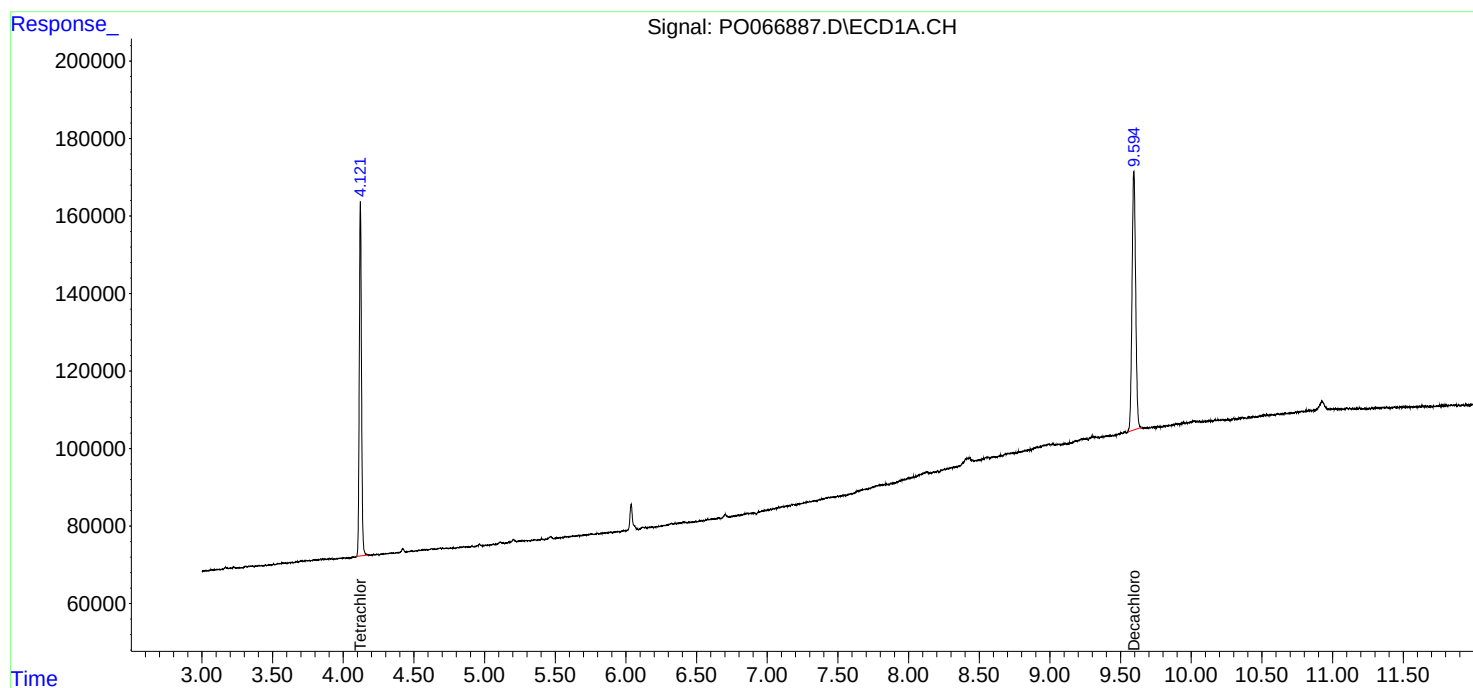


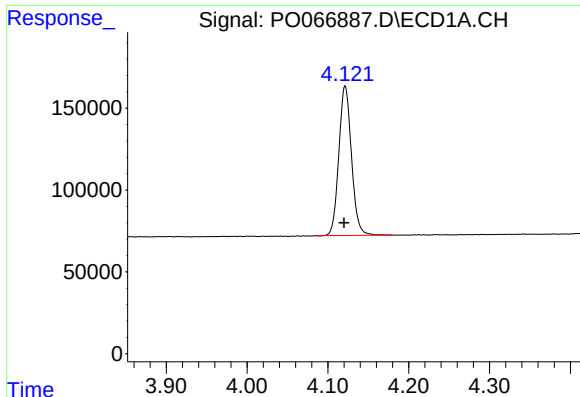

#1 Tetrachloro-m-xylene


R.T.: 4.121 min
Delta R.T.: 0.001 min
Response: 991554
Conc: 24.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-G0-G1-G0A-G1A

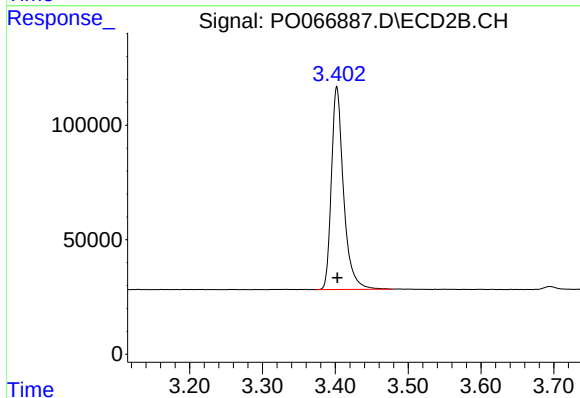


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 1026753
Conc: 23.25 ng/ml

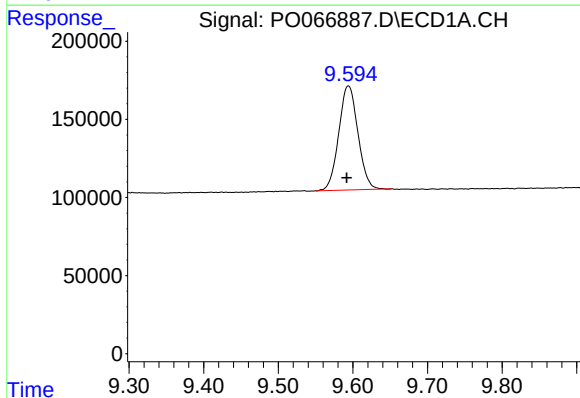

#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: 0.002 min
Response: 1188896
Conc: 24.37 ng/ml

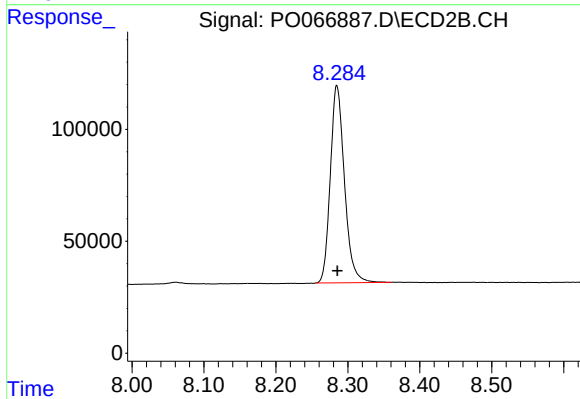

#2 Decachlorobiphenyl

R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 1205515
Conc: 23.96 ng/ml