

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
 Data File : P0066907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2020 19:00
 Operator : DD\AJ
 Sample : L1736-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-01-010-B

Manual Integrations
 APPROVED

Sohil
 3/3/2020 4:44:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:28:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 26 14:12:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.119	3.402	983293	978616	24.114m	22.159
2) SA Decachlor...	9.590	8.286	856174	830275	17.551	16.505

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030220\
Data File : PO066907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2020 19:00
Operator : DD\AJ
Sample : L1736-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-01-010-B


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:28:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022620.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 26 14:12:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

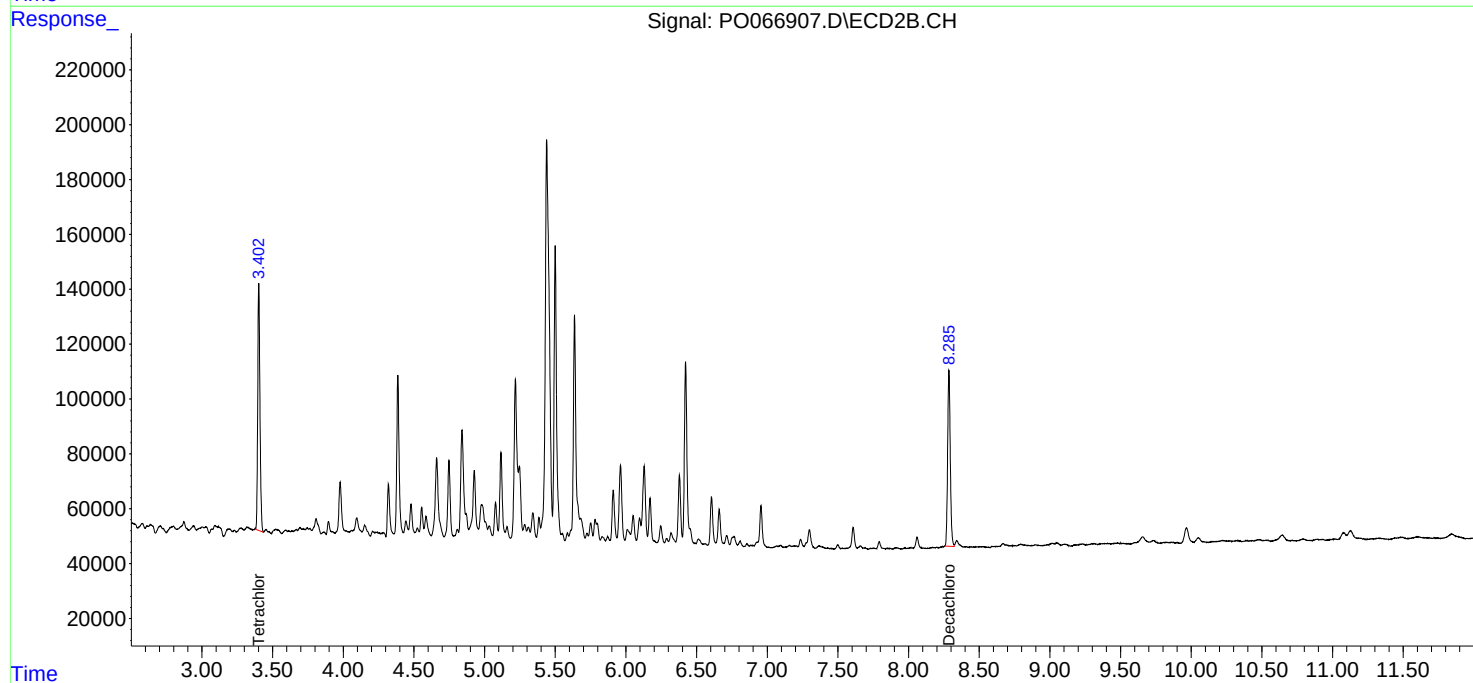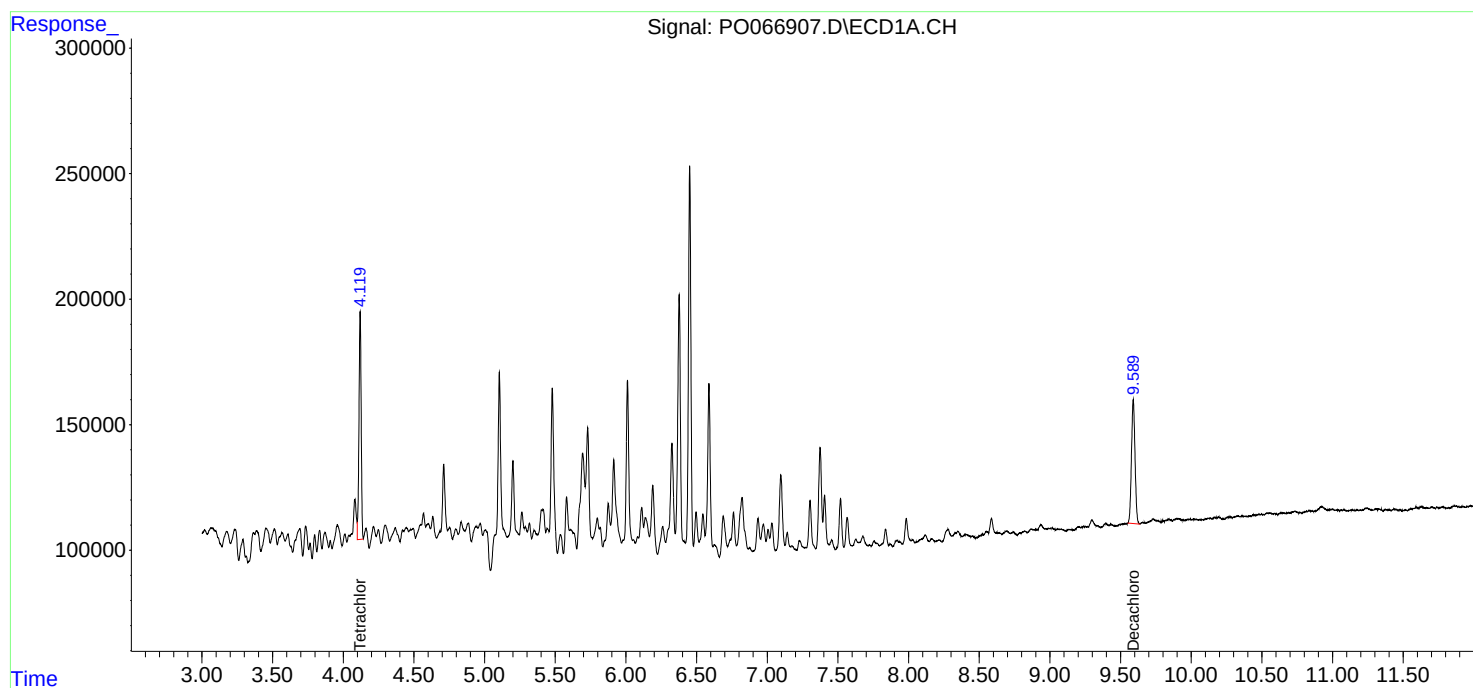

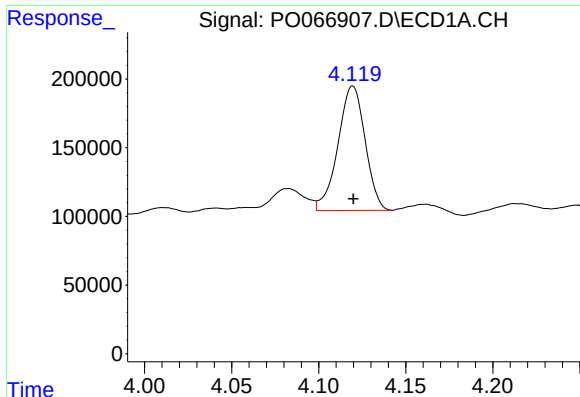


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 983293
Conc: 24.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-010-B


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:33 PM

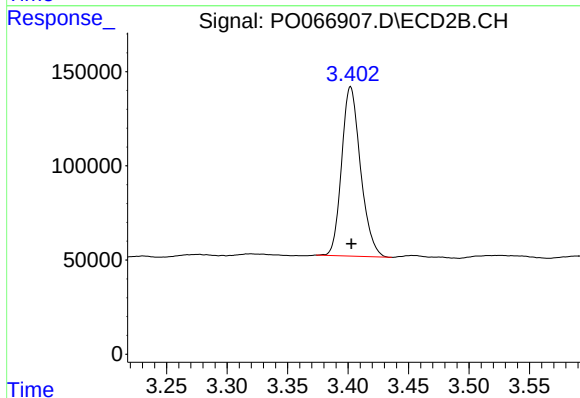


#1 Tetrachloro-m-xylene

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 978616
Conc: 22.16 ng/ml

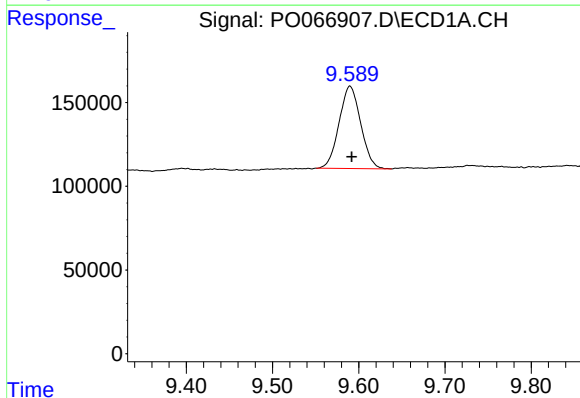

#2 Decachlorobiphenyl

R.T.: 9.590 min
Delta R.T.: -0.002 min
Response: 856174
Conc: 17.55 ng/ml

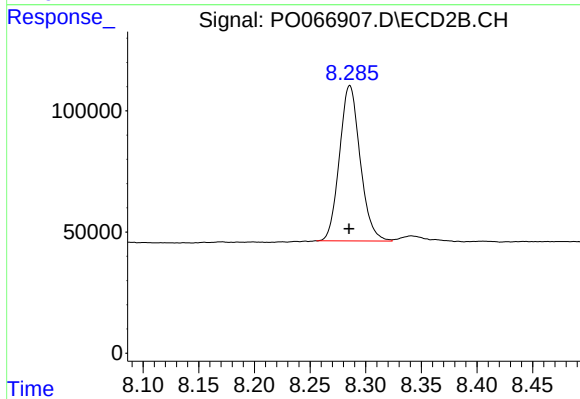

#2 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 830275
Conc: 16.51 ng/ml