

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
 Data File : P0066908.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Mar 2020 19:17
 Operator : DD\AJ
 Sample : L1736-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-01-010-A

Manual Integrations
 APPROVED

Sohil
 3/3/2020 4:44:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 03:28:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 26 14:12:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.120	3.403	947929	966577	23.246m	21.887
2) SA Decachlor...	9.593	8.286	789693	796806	16.188	15.840

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030220\
Data File : P0066908.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2020 19:17
Operator : DD\AJ
Sample : L1736-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-01-010-A


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 03:28:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022620.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 26 14:12:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

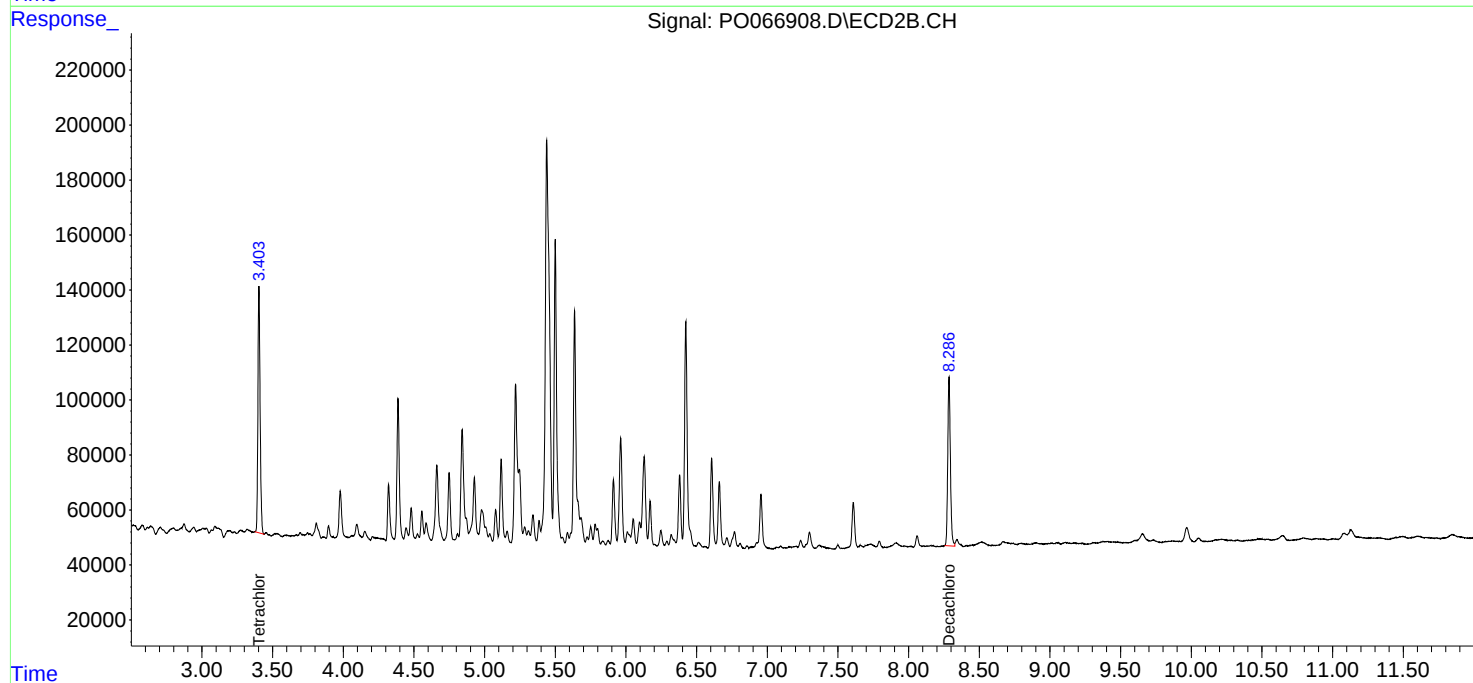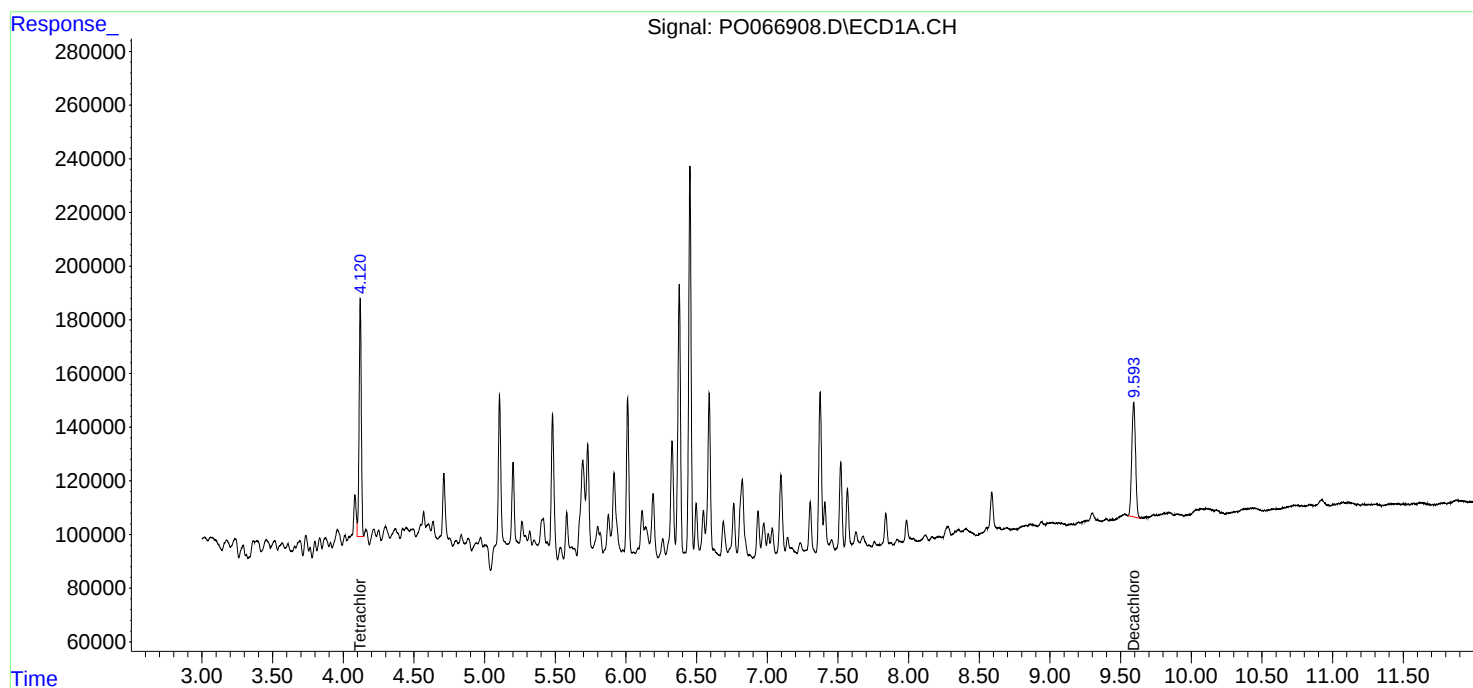

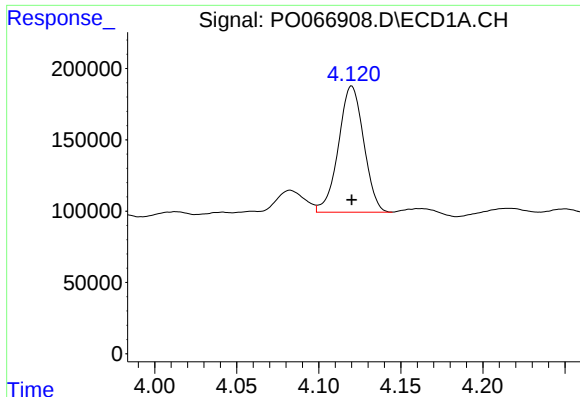


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: 0.000 min
Response: 947929
Conc: 23.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-01-010-A


Manual Integrations
APPROVED

Sohil
3/3/2020 4:44:34 PM

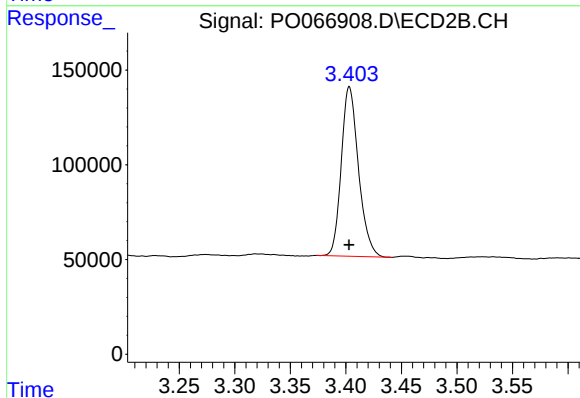


#1 Tetrachloro-m-xylene

R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 966577
Conc: 21.89 ng/ml

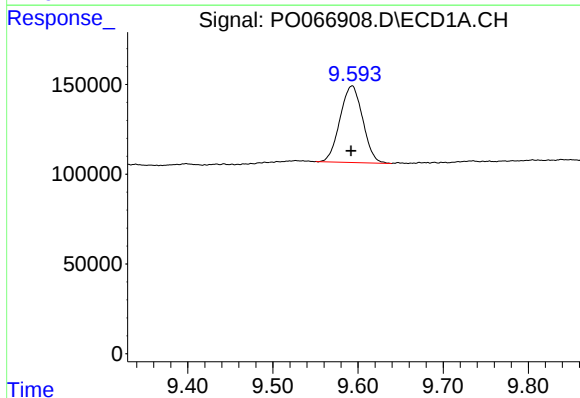

#2 Decachlorobiphenyl

R.T.: 9.593 min
Delta R.T.: 0.001 min
Response: 789693
Conc: 16.19 ng/ml

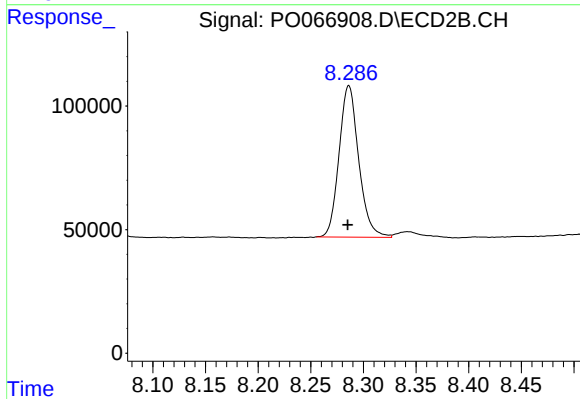

#2 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 796806
Conc: 15.84 ng/ml