Quantitation Report (Not Reviewed)

Data Path : P:\HPCHEM1\ECD_O\Data\PO030318\
Data File : PO042741.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2018 14:26
Operator : SM/UA
Sample : PB106870BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : PB106870BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 14:46:49 2018
Quant Method : P:\HPCHEM1\ECD_O\methods\PO022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
	System Monitoring Compounds							
1)	SA Tetrachlo...	4.094	3.342	4282243	6168001	17.287	16.691	
2)	SA Decachlor...	9.475	8.127	4757126	5895544	18.823	15.288	
	Target Compounds							
7)	L1 AR-1016-5	6.067	0.000	1301237	0	180.757	N.D.	#
22)	L5 AR-1248-2	0.000	4.938	0	675275	N.D.	69.447	#
23)	L5 AR-1248-3	6.067	0.000	1301237	0	142.298	N.D.	#
29)	L6 AR-1254-4	0.000	5.978	0	545291	N.D.	27.984	#
32)	L7 AR-1260-2	0.000	5.978	0	545291	N.D.	16.233	#
36)	L8 AR-1262-1	0.000	5.978	0	545291	N.D.	24.551	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : P:\HPCHEM1\ECD_O\Data\PO030318\
Data File : PO042741.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2018 14:26
Operator : SM/UA
Sample : PB106870BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : PB106870BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 14:46:49 2018
Quant Method : P:\HPCHEM1\ECD_O\methods\PO022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

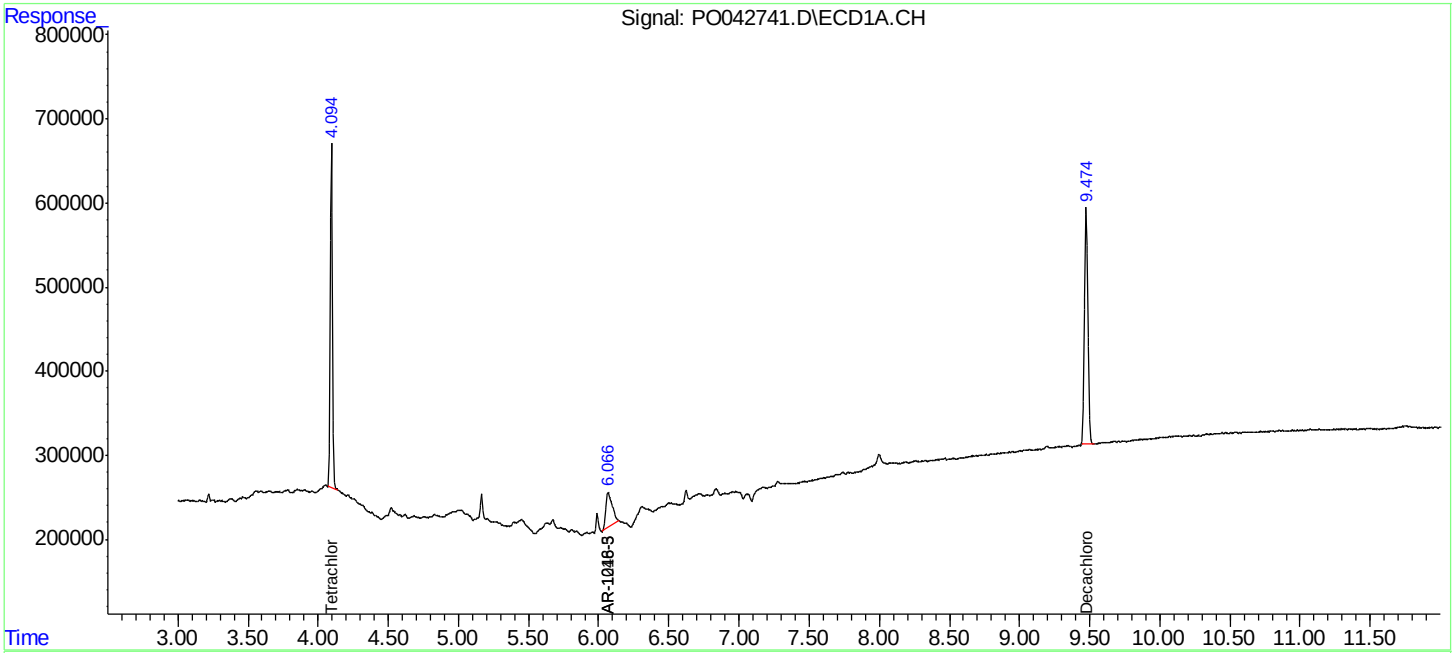

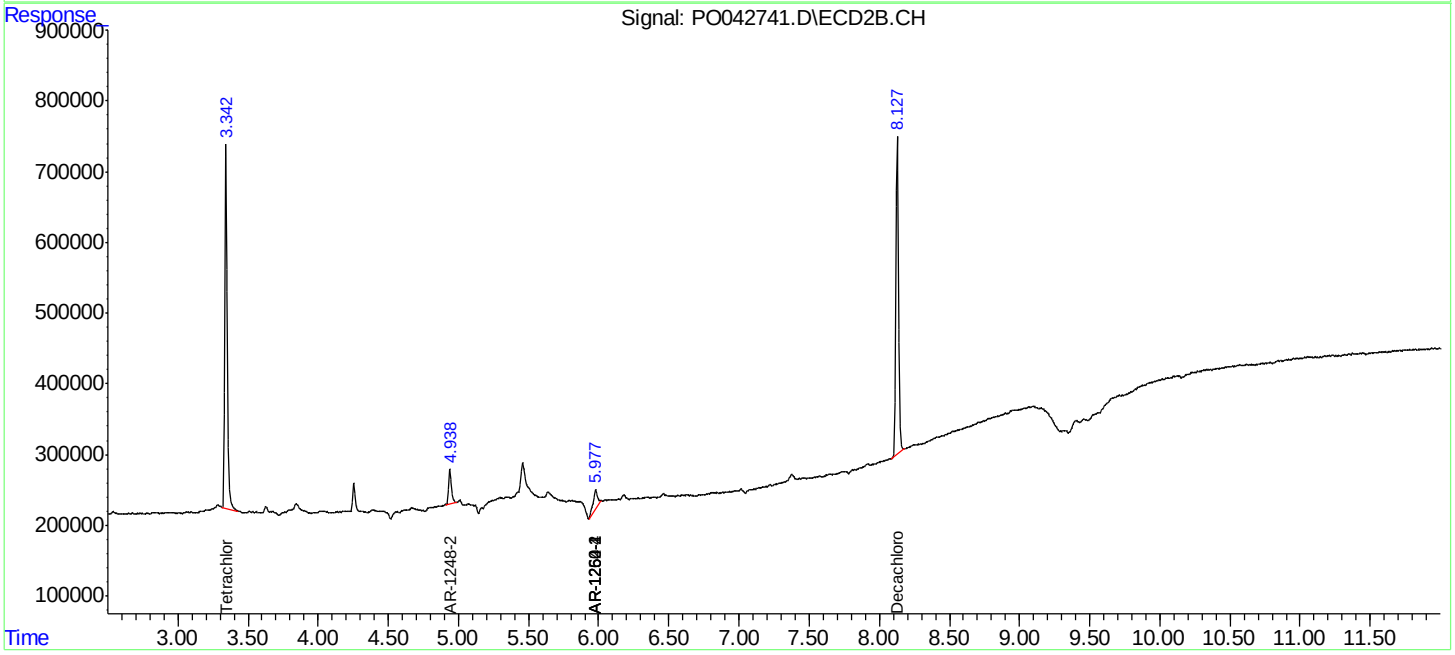

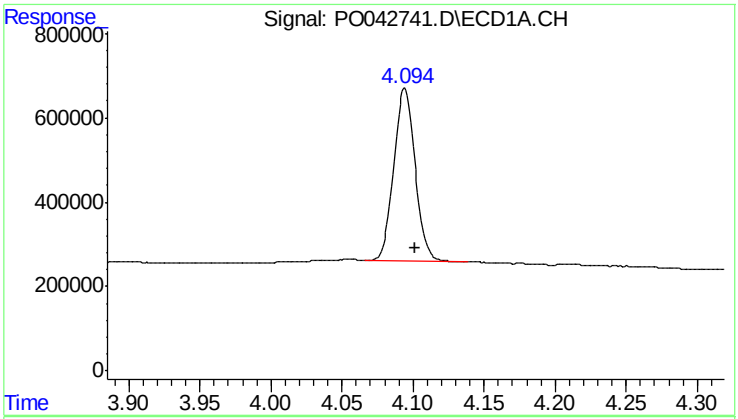

#1 Tetrachloro-m-xylene

R.T.: 4.094 min
Delta R.T.: -0.007 min
Response: 4282243
Conc: 17.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB106870BL

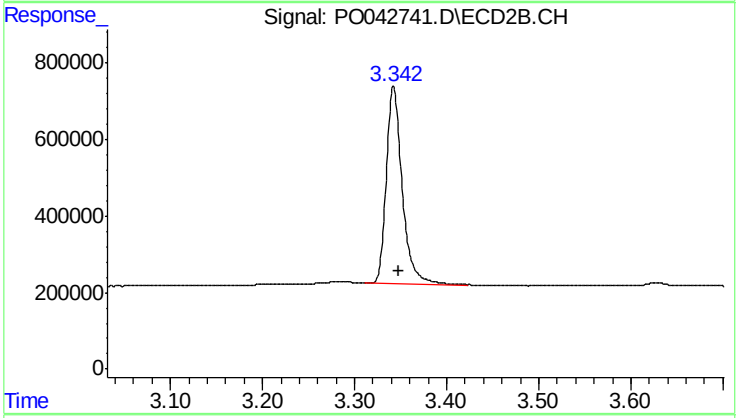

#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: -0.006 min
Response: 6168001
Conc: 16.69 ng/ml

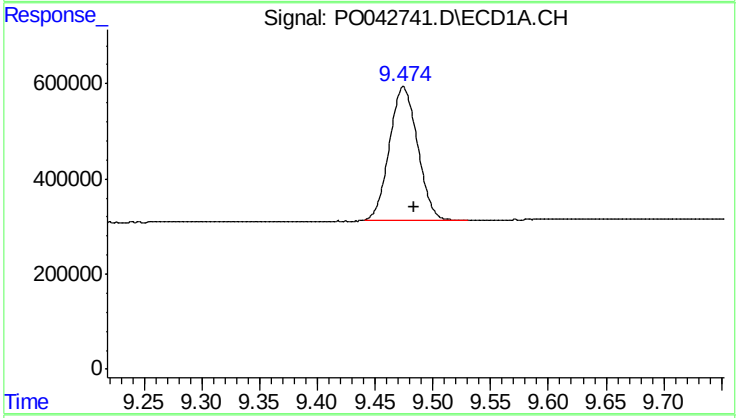

#2 Decachlorobiphenyl

R.T.: 9.475 min
Delta R.T.: -0.010 min
Response: 4757126
Conc: 18.82 ng/ml

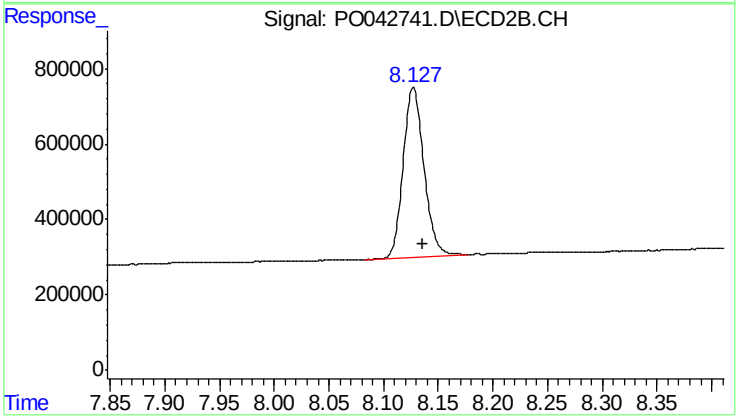

#2 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: -0.009 min
Response: 5895544
Conc: 15.29 ng/ml

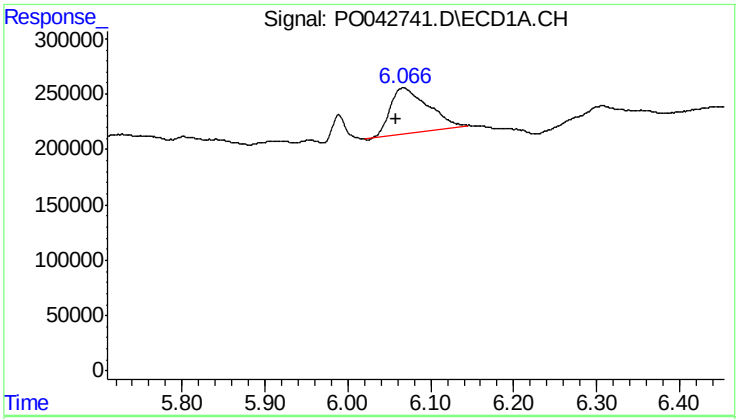

#7 AR-1016-5

R.T.: 6.067 min
Delta R.T.: 0.009 min
Response: 1301237
Conc: 180.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB106870BL

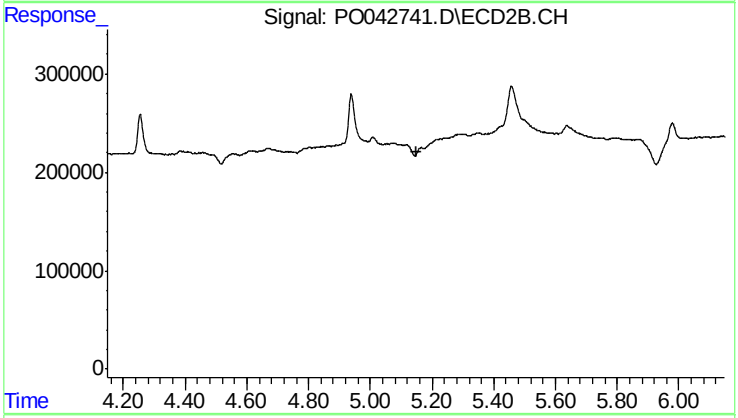

#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.148 min
Response: 0
Conc: N.D.

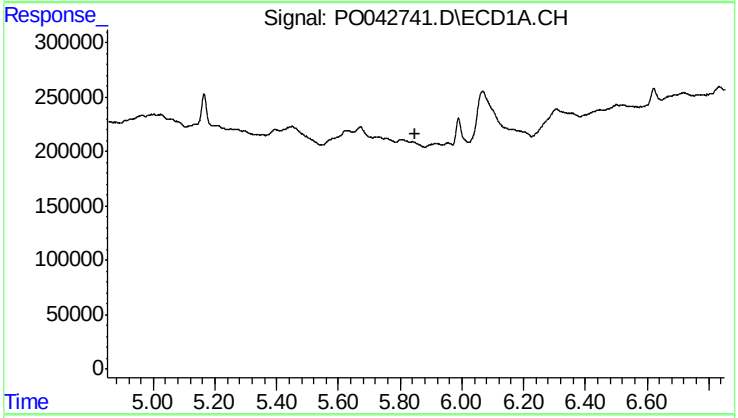

#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.851 min
Response: 0
Conc: N.D.

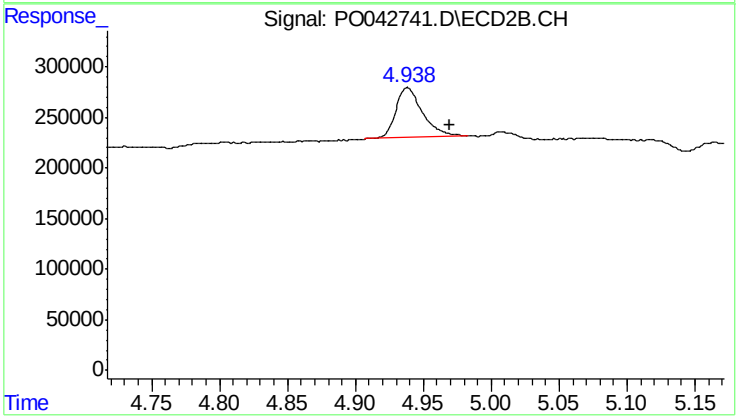

#22 AR-1248-2

R.T.: 4.938 min
Delta R.T.: -0.031 min
Response: 675275
Conc: 69.45 ng/ml

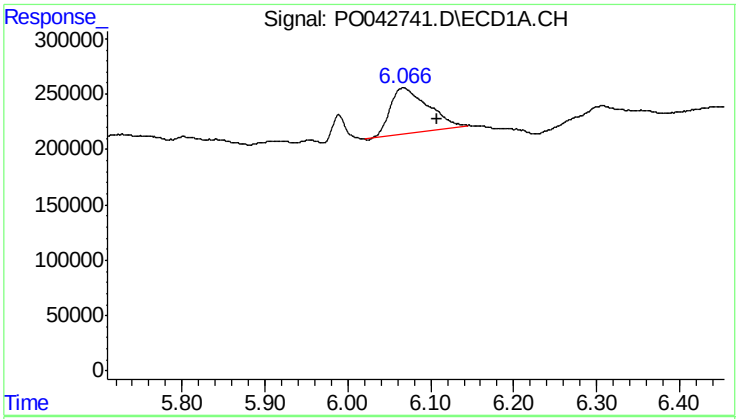

#23 AR-1248-3

R.T.: 6.067 min
Delta R.T.: -0.041 min
Response: 1301237
Conc: 142.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB106870BL

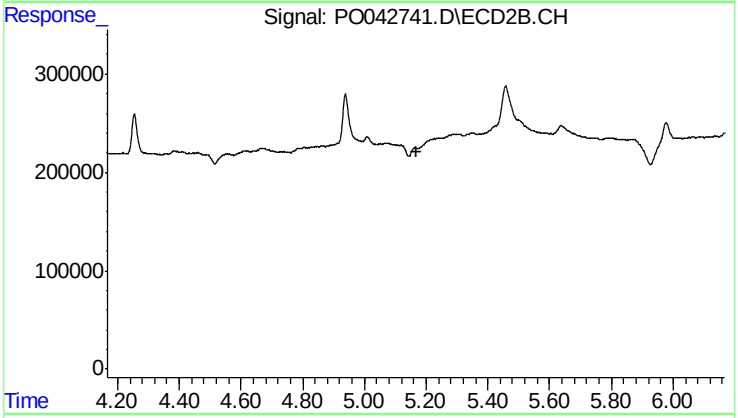

#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.167 min
Response: 0
Conc: N.D.

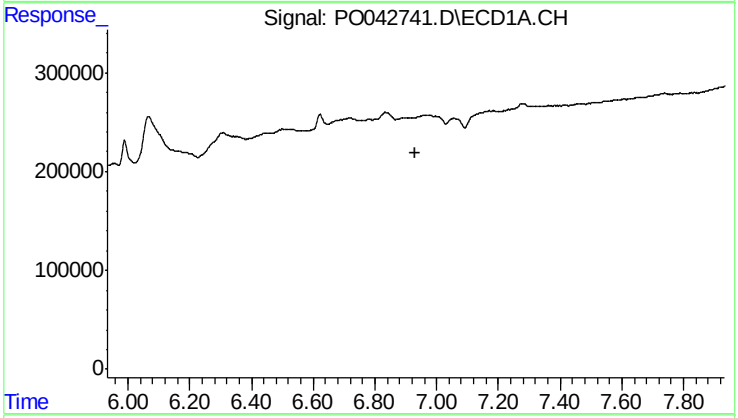

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

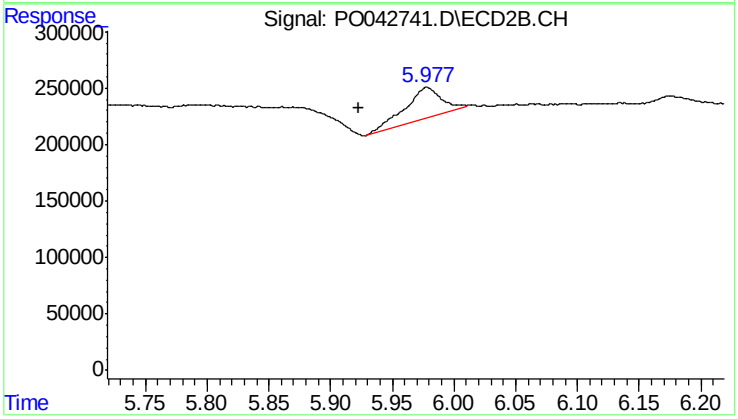

#29 AR-1254-4

R.T.: 5.978 min
Delta R.T.: 0.055 min
Response: 545291
Conc: 27.98 ng/ml

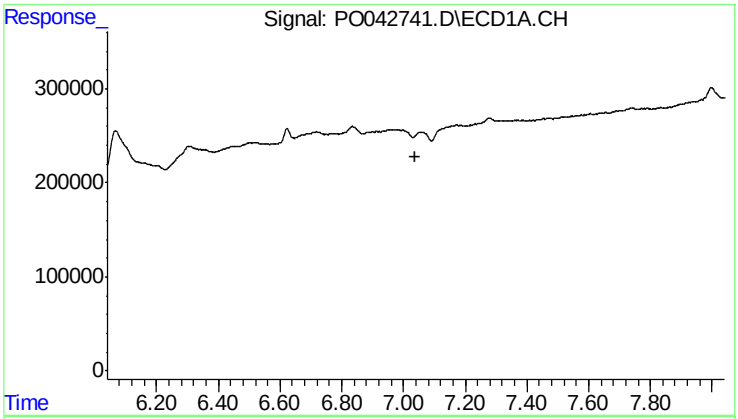

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PB106870BL

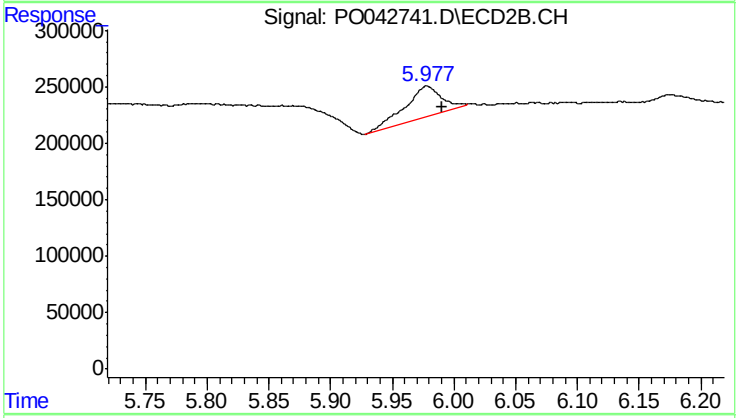

#32 AR-1260-2

R.T.: 5.978 min
Delta R.T.: -0.013 min
Response: 545291
Conc: 16.23 ng/ml

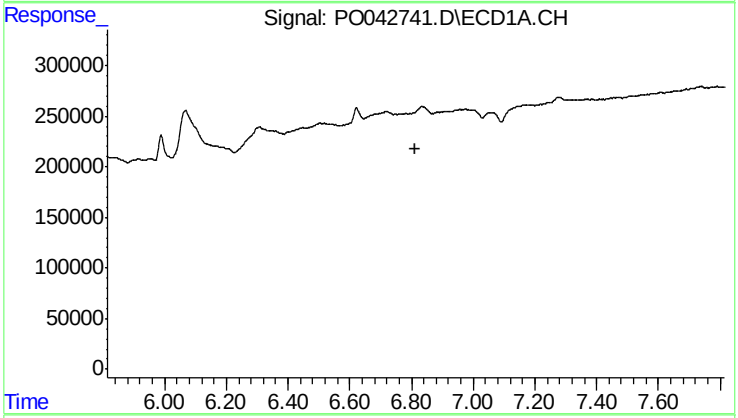

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

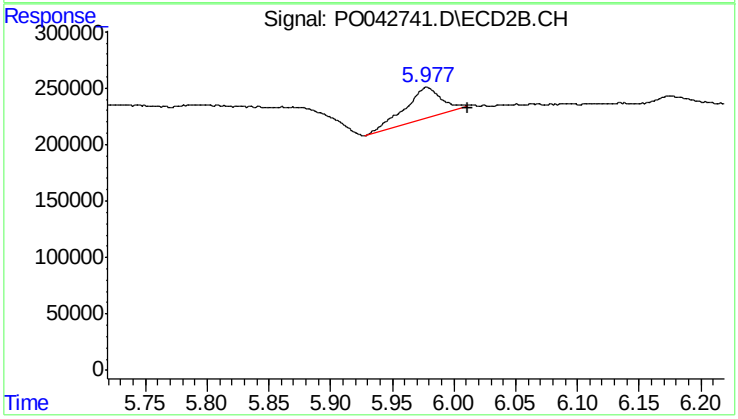

#36 AR-1262-1

R.T.: 5.978 min
Delta R.T.: -0.033 min
Response: 545291
Conc: 24.55 ng/ml