

Data Path : P:\HPCHEM1\ECD_0\Data\P0030418\
Data File : P0042751.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2018 18:55
Operator : SM/UA
Sample : J1736-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OILY-WATER

Manual Integrations
APPROVED

ugo
3/6/2018 8:24:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 22:52:48 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.093	3.342	4074557	5807165	16.448	15.715
2) SA Decachlor...	9.470	8.124	4317569	5812757	17.084m	15.074

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0030418\
Data File : P0042751.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Mar 2018 18:55
Operator : SM/UA
Sample : J1736-06
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

ugo
3/6/2018 8:24:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 22:52:48 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0022118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 26 14:24:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

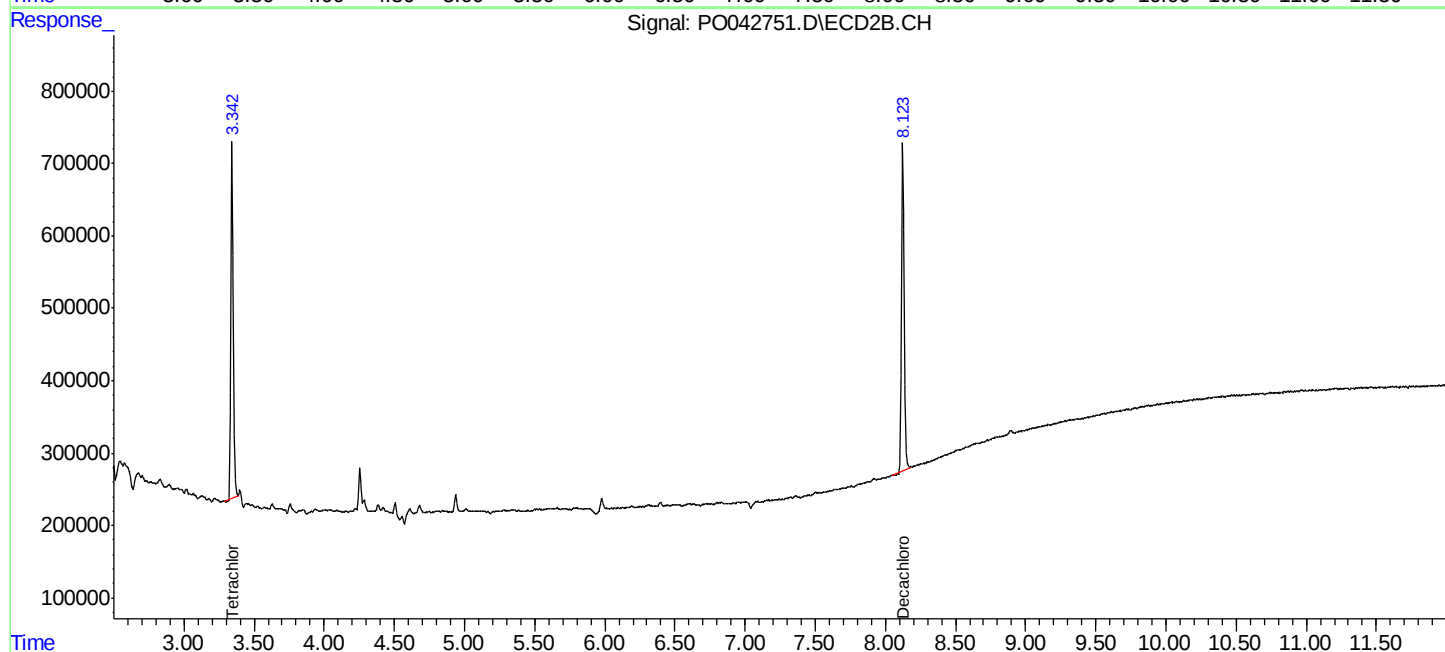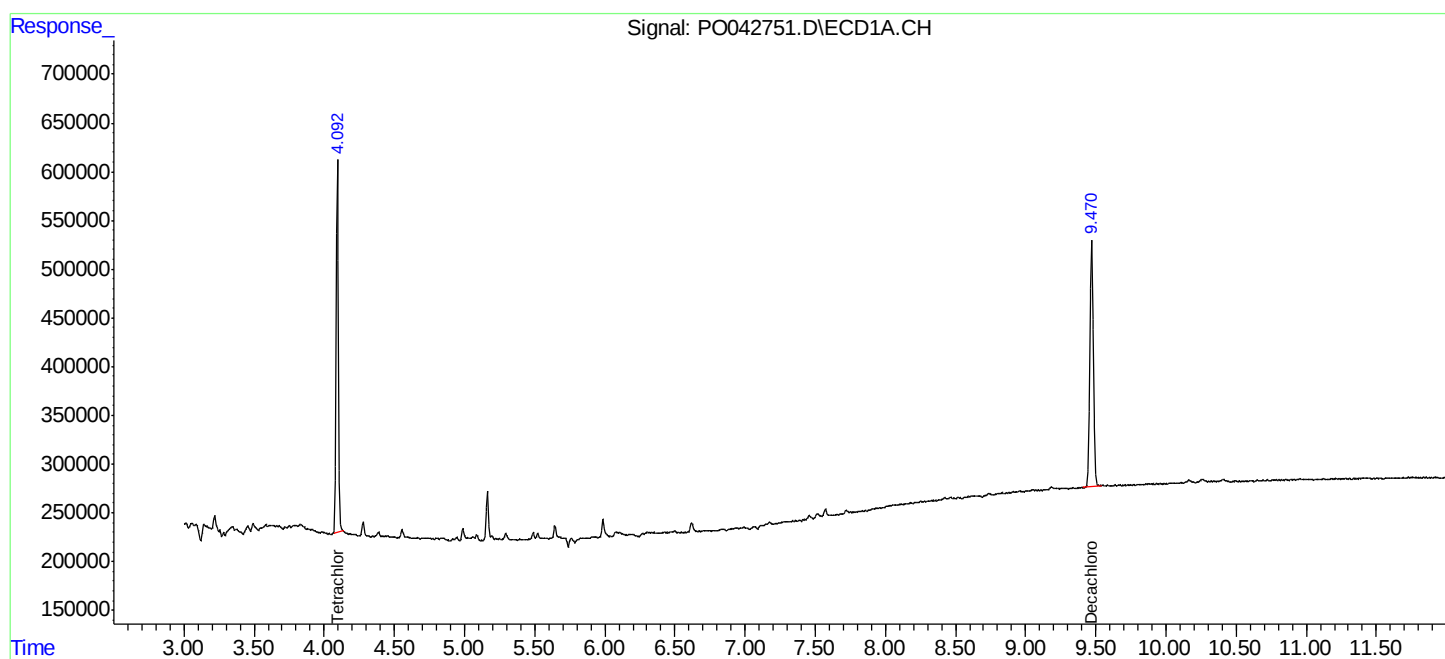

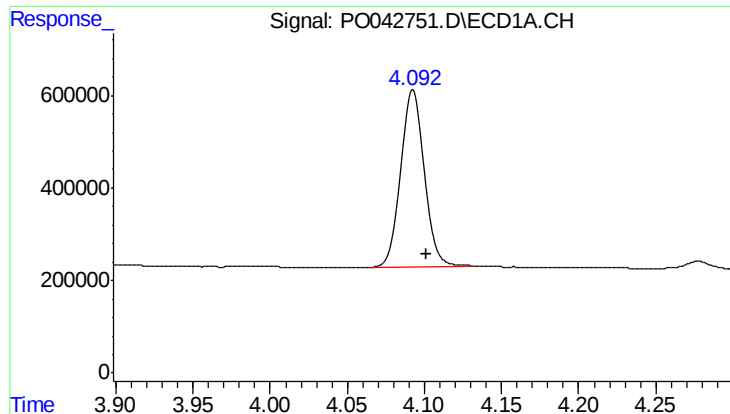


#1 Tetrachloro-m-xylene

R.T.: 4.093 min
Delta R.T.: -0.009 min
Response: 4074557
Conc: 16.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

ugo
3/6/2018 8:24:55 PM

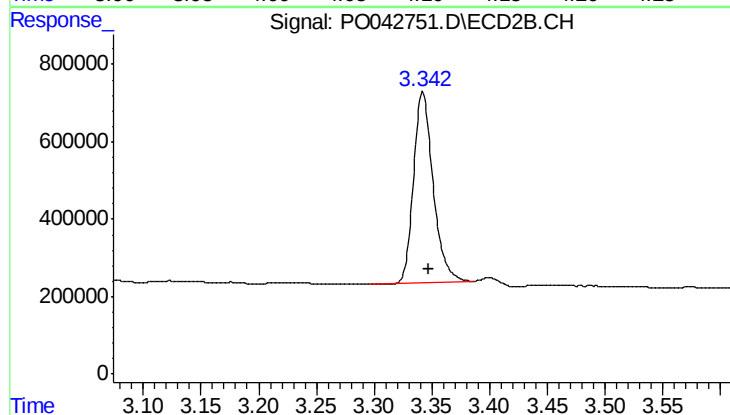


#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: -0.006 min
Response: 5807165
Conc: 15.71 ng/ml

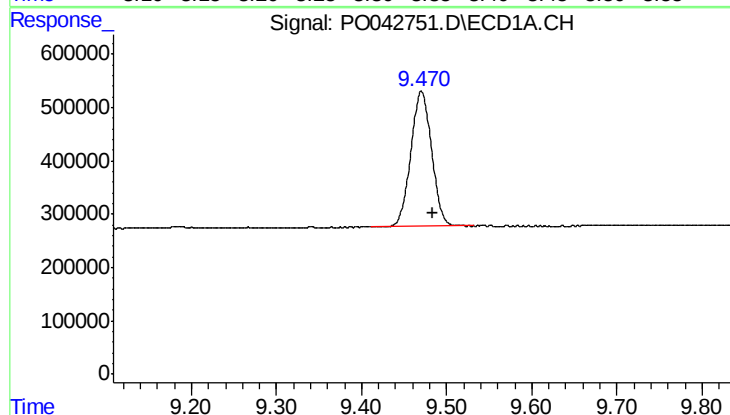

#2 Decachlorobiphenyl

R.T.: 9.470 min
Delta R.T.: -0.015 min
Response: 4317569
Conc: 17.08 ng/ml m

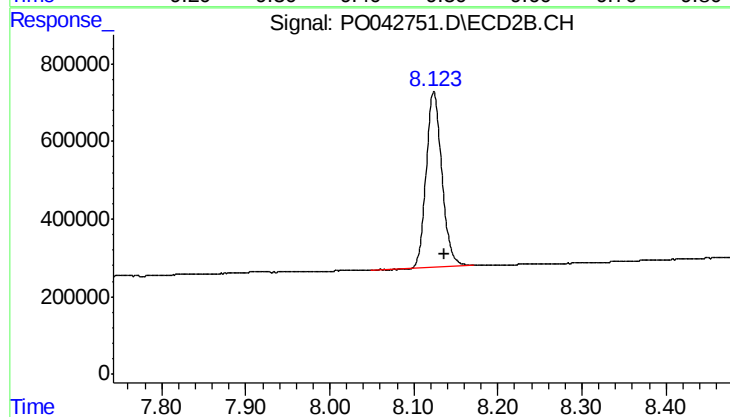

#2 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.013 min
Response: 5812757
Conc: 15.07 ng/ml